


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032120\
 Data File : VU037359.D
 Acq On : 21 Mar 2020 17:03
 Operator : JC/MD
 Sample : BFB32
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB32

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032120WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 23 04:26:12 2020

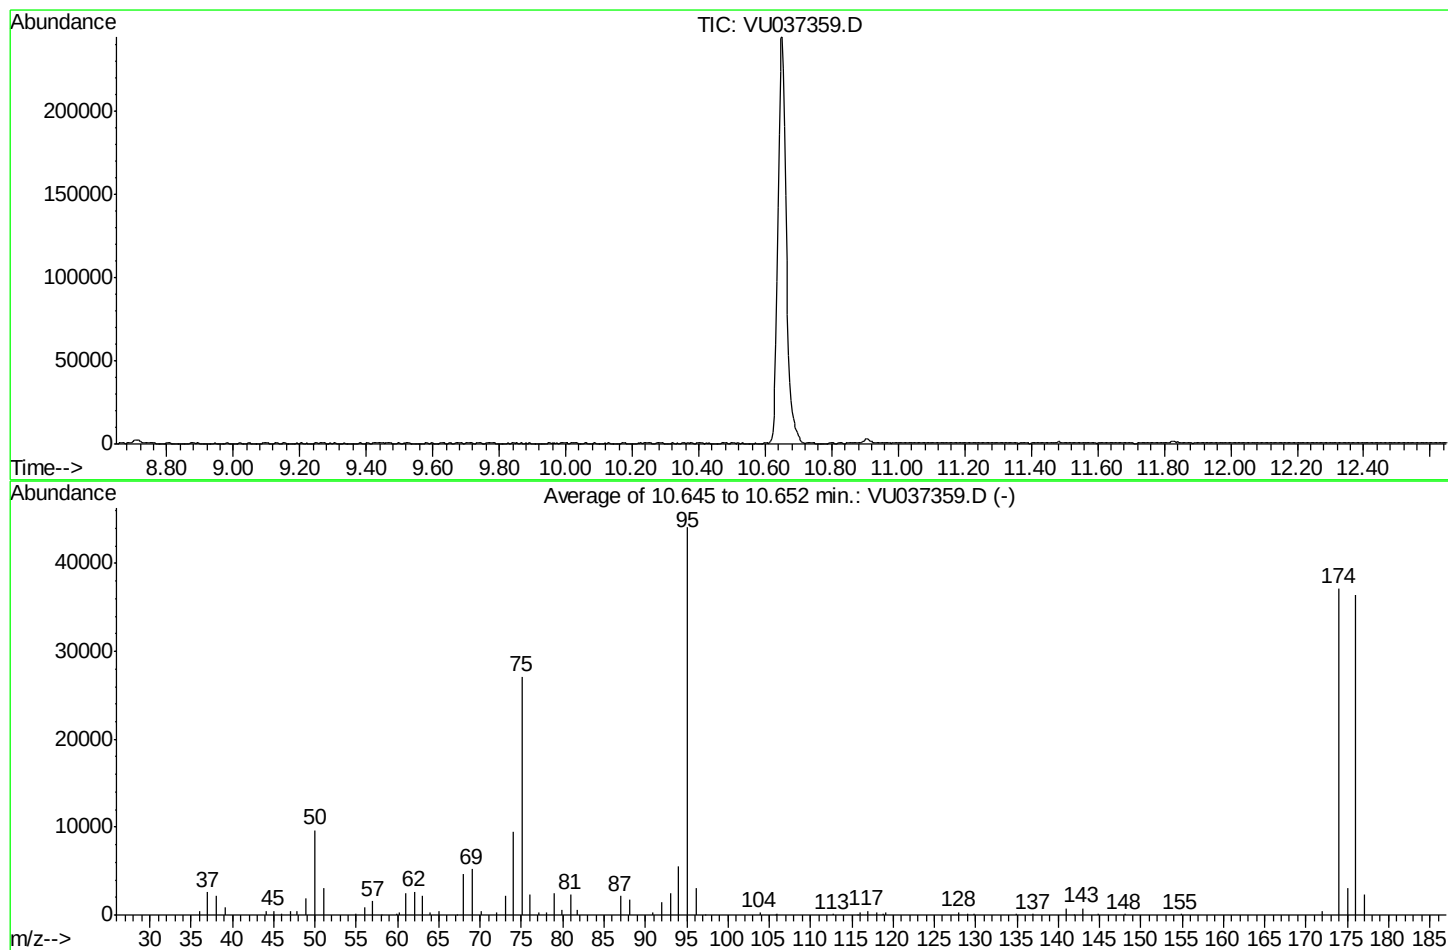

AutoFind: Scans 2894, 2895, 2896; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	9650	PASS
75	95	30	80	61.5	27109	PASS
95	95	100	100	100.0	44112	PASS
96	95	5	9	7.0	3067	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	37088	PASS
175	174	5	9	8.2	3037	PASS
176	174	95	101	98.2	36424	PASS
177	176	5	9	6.3	2291	PASS

m/z	Abundance
35.90	477.0
37.00	2653.0
38.00	2311.0
39.10	935.0
44.10	725.0
45.00	536.0
46.00	118.0
47.10	480.0
47.90	474.0
49.00	1990.0
50.00	10033.0
51.00	3058.0
55.00	161.0
56.00	866.0
57.00	1643.0
58.00	102.0
60.20	392.0
61.00	2569.0
62.00	2718.0
63.00	2279.0
63.90	322.0
65.00	430.0
68.00	4801.0
69.00	5301.0
70.00	427.0
72.00	295.0
73.00	2262.0
74.00	9867.0
75.00	27952.0
76.00	2442.0
77.10	294.0
78.00	294.0
78.90	2523.0
79.90	658.0
81.00	2353.0
81.80	543.0
87.00	2219.0
88.00	1788.0
90.90	301.0
92.00	1539.0
93.00	2529.0
94.00	5715.0
95.10	45192.0
96.10	3154.0
103.90	291.0
106.00	234.0
112.80	107.0
116.00	234.0
116.90	520.0
118.00	244.0
119.00	399.0
127.90	314.0
128.90	127.0
129.80	219.0
134.90	131.0
137.00	133.0
140.90	782.0
143.00	791.0
144.90	217.0
148.10	124.0
154.80	120.0
172.00	482.0
174.10	38184.0
175.10	3145.0
176.10	37384.0
177.00	2369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
35.90	442.0
37.00	2414.0
38.00	2188.0
39.00	863.0
43.90	563.0
45.00	466.0
46.00	117.0
47.10	459.0
47.80	429.0
49.00	1814.0
50.00	9101.0
51.00	2868.0
55.00	134.0
56.00	858.0
57.00	1369.0
60.10	433.0
61.00	2410.0
62.00	2648.0
63.00	2103.0
63.90	324.0
65.10	365.0
68.00	4560.0
69.00	5019.0
70.00	389.0
71.90	264.0
73.00	2050.0
74.00	9085.0
75.00	26000.0
76.00	2250.0
77.10	331.0
78.10	242.0
78.90	2398.0
79.80	564.0
81.00	2271.0
81.80	560.0
87.00	2064.0
88.00	1693.0
90.90	286.0
92.00	1415.0
93.00	2254.0
94.00	5316.0
95.10	42032.0
96.10	2912.0
103.90	200.0
105.70	198.0
115.70	191.0
116.00	195.0
116.90	449.0
118.00	208.0
118.80	375.0
127.90	280.0
128.90	123.0
129.90	197.0
136.90	137.0
140.90	709.0
141.90	126.0
142.90	824.0
144.90	160.0
148.10	103.0
172.00	463.0
174.10	34272.0
175.10	2602.0
176.00	33432.0
177.00	2192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

Scan 2882 (10.607 min): VU037359.D
BFB32

m/z	Abundance
39.80	105.0
43.90	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	523.0
37.00	2685.0
38.00	2264.0
39.10	866.0
39.80	136.0
44.10	789.0
45.00	513.0
47.10	440.0
47.90	432.0
48.90	2052.0
50.00	9816.0
51.00	3106.0
55.00	160.0
56.00	876.0
57.00	1731.0
59.90	384.0
61.00	2592.0
62.00	2567.0
63.00	2197.0
64.00	295.0
65.00	420.0
67.10	221.0
68.00	4792.0
69.00	5218.0
70.10	449.0
72.00	341.0
73.10	2197.0
74.00	9530.0
75.10	27376.0
76.00	2317.0
77.00	297.0
78.00	273.0
78.90	2392.0
79.90	746.0
80.90	2361.0
81.80	524.0
87.00	2083.0
88.10	1753.0
91.00	243.0
92.00	1549.0
93.00	2597.0
94.00	5616.0
95.10	45112.0
96.10	3135.0
97.20	106.0
103.90	377.0
106.00	386.0
112.70	128.0
115.90	263.0
116.90	575.0
117.90	251.0
119.10	377.0
128.00	298.0
129.00	112.0
129.80	203.0
134.90	147.0
137.00	124.0
140.90	752.0
143.00	767.0
144.90	198.0
148.00	120.0
154.90	116.0
172.00	447.0
174.00	38808.0
175.10	3366.0
176.10	38456.0
177.00	2314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32