

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032122\
 Data File : VU047625.D
 Acq On : 21 Mar 2022 10:49
 Operator : SY/MD
 Sample : VU0321WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0321WBL01

Quant Time: Mar 22 01:46:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Mar 18 13:19:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	28225	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.635	95	9333	0.887	ug/l	0.00
Spiked Amount 1.000			Recovery	=	89.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	11791	0.924	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032122\
Data File : VU047625.D
Acq On : 21 Mar 2022 10:49
Operator : SY/MD
Sample : VU0321WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0321WBL01

Quant Time: Mar 22 01:46:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Mar 18 13:19:37 2022
Response via : Initial Calibration




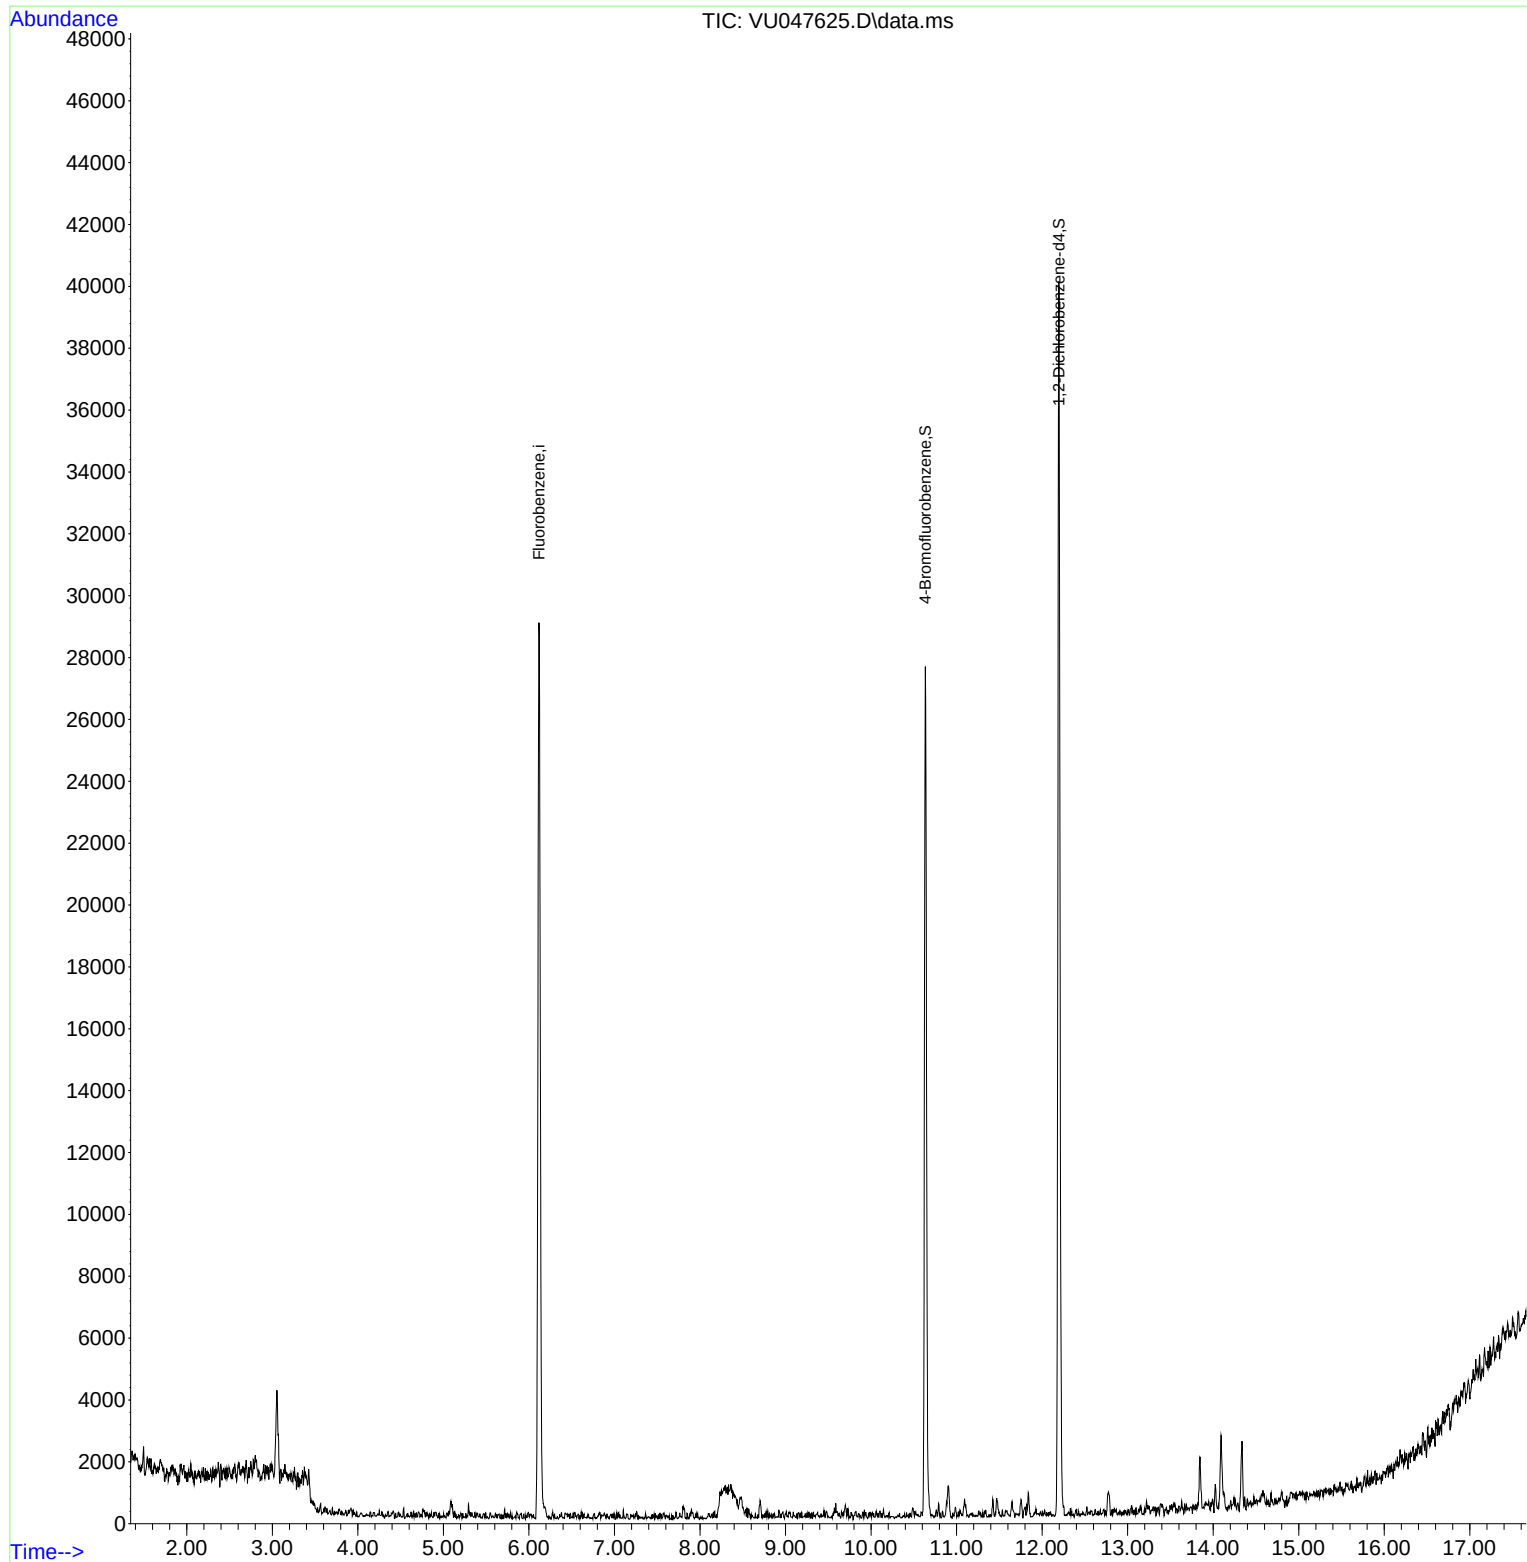


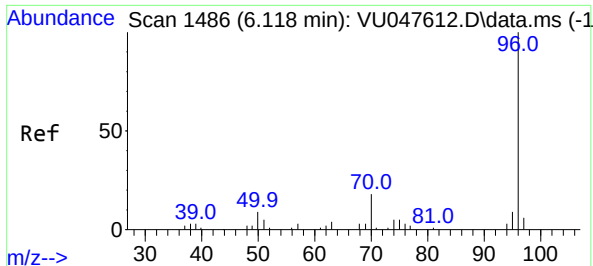

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. -0.000 min
Lab File: VU047625.D
Acq: 21 Mar 2022 10:49




Instrument :
MSVOA_U
ClientSampleId :
VU0321WBL01


Tgt Ion: 96	Resp: 28225
Ion Ratio	Lower Upper
96 100	
70 18.1	16.8 25.2
95 8.9	7.3 10.9
97 6.5	0.0 0.0#

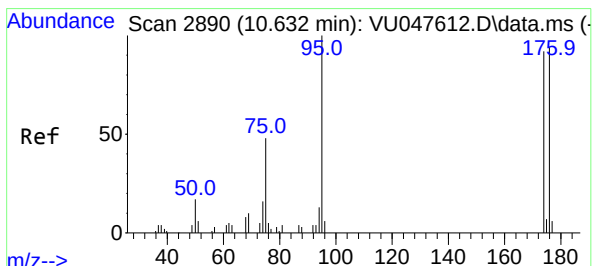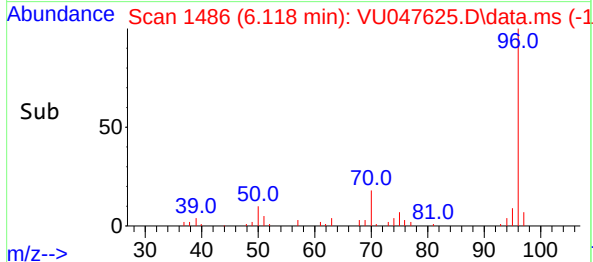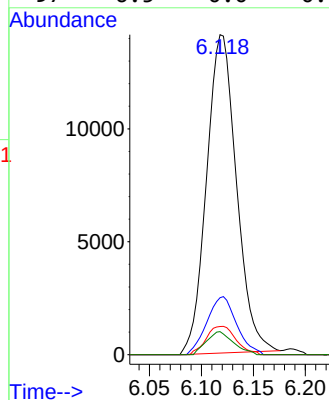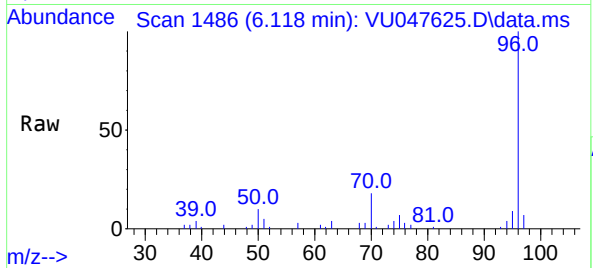

#57
4-Bromofluorobenzene
Concen: 0.887 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU047625.D
Acq: 21 Mar 2022 10:49


Tgt Ion: 95	Resp: 9333
Ion Ratio	Lower Upper
95 100	
174 97.9	56.6 84.8#
176 93.2	54.3 81.5#

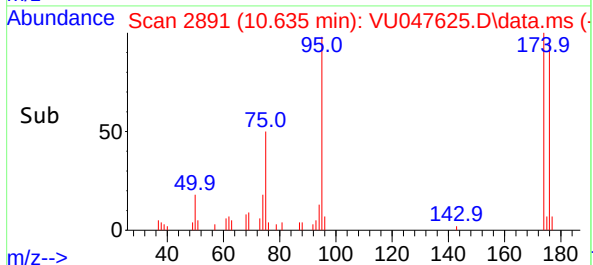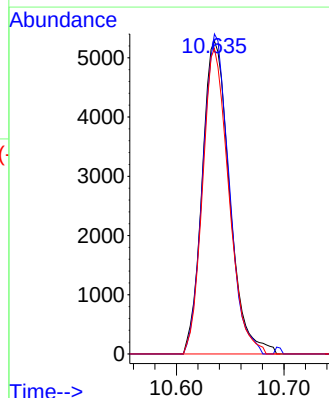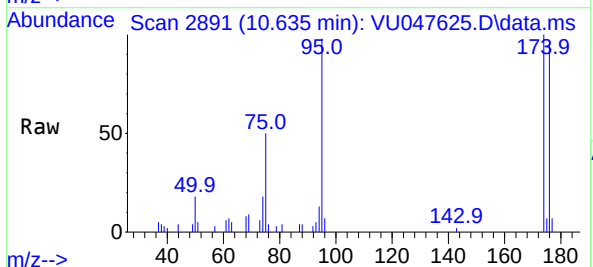

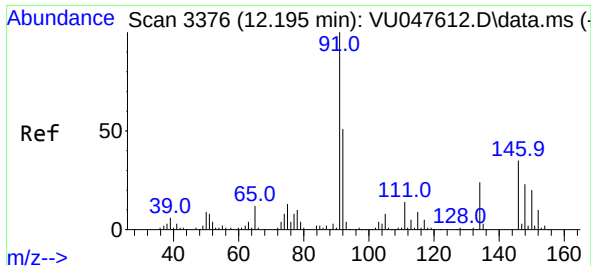

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.924 ug/l
 RT: 12.198 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU047625.D
 Acq: 21 Mar 2022 10:49

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0321WBL01

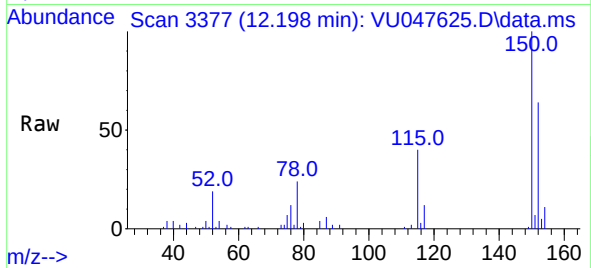

Tgt Ion:	152	Resp:	11791
Ion Ratio	Lower	Upper	
152	100		
115	63.9	0.0	251.0
150	157.1	0.0	613.8

