


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032122\
 Data File : VU047623.D
 Acq On : 21 Mar 2022 09:05
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Mar 18 13:19:37 2022

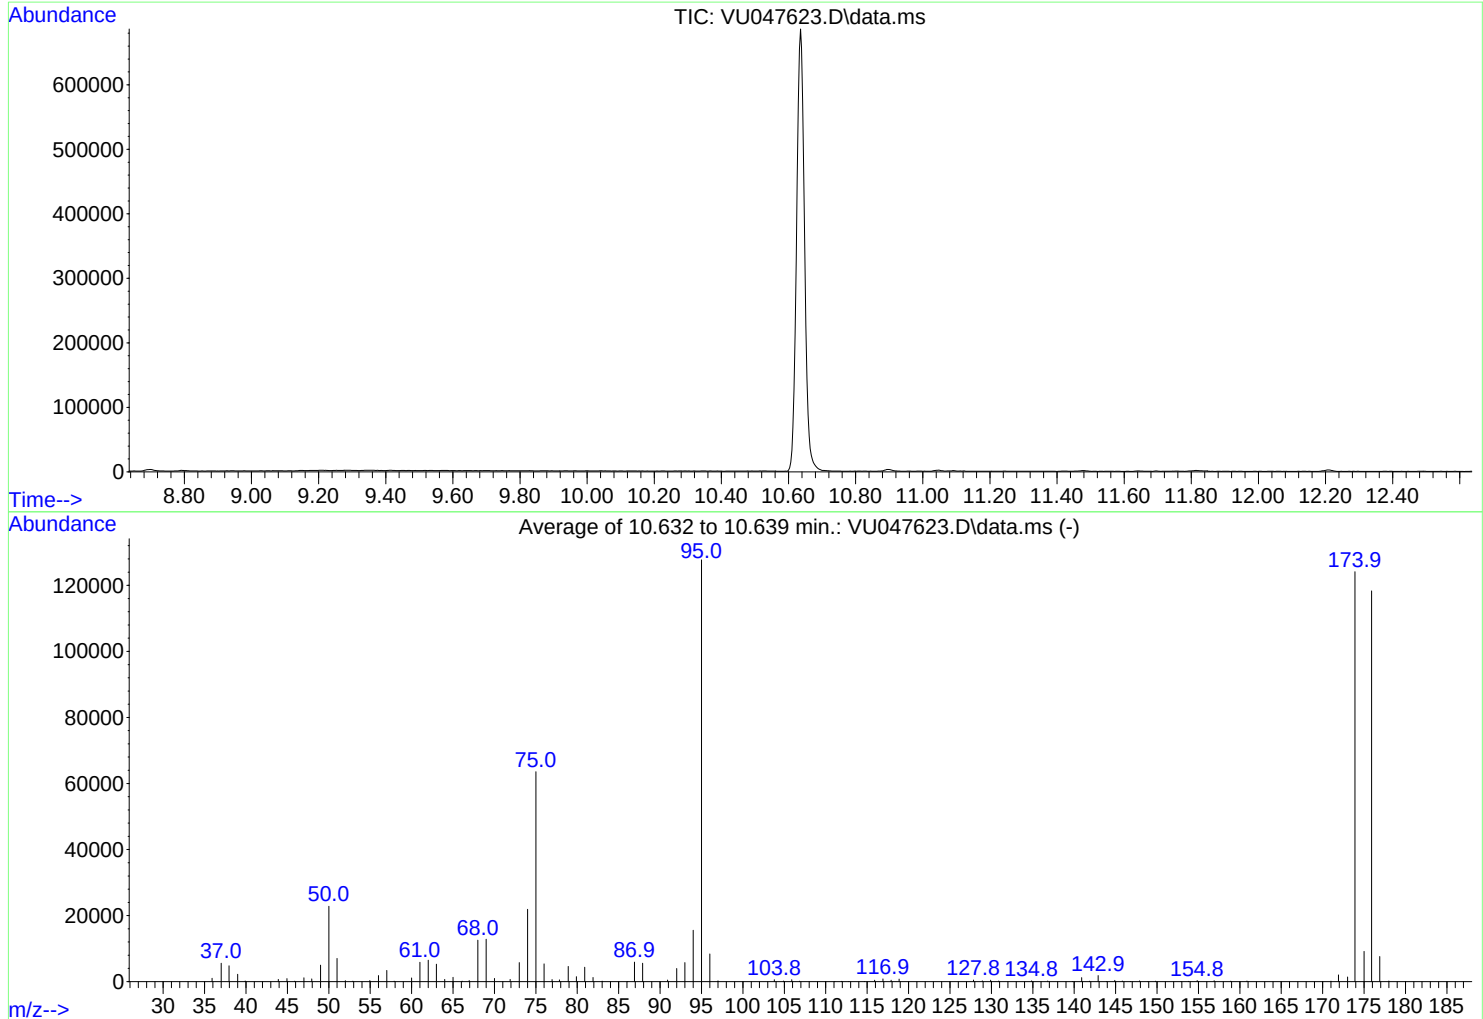

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	22805	PASS
75	95	30	60	49.8	63584	PASS
95	95	100	100	100.0	127725	PASS
96	95	5	9	6.6	8405	PASS
173	174	0.00	2	1.1	1417	PASS
174	95	50	100	97.2	124104	PASS
175	174	5	9	7.4	9164	PASS
176	174	95	101	95.3	118333	PASS
177	176	5	9	6.4	7594	PASS