




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053335.D
 Acq On : 21 Mar 2023 19:30
 Operator : JC/MD
 Sample : 01995-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM8

Manual IntegrationsAPPROVED

Quant Time: Mar 22 03:13:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 22 03:08:43 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

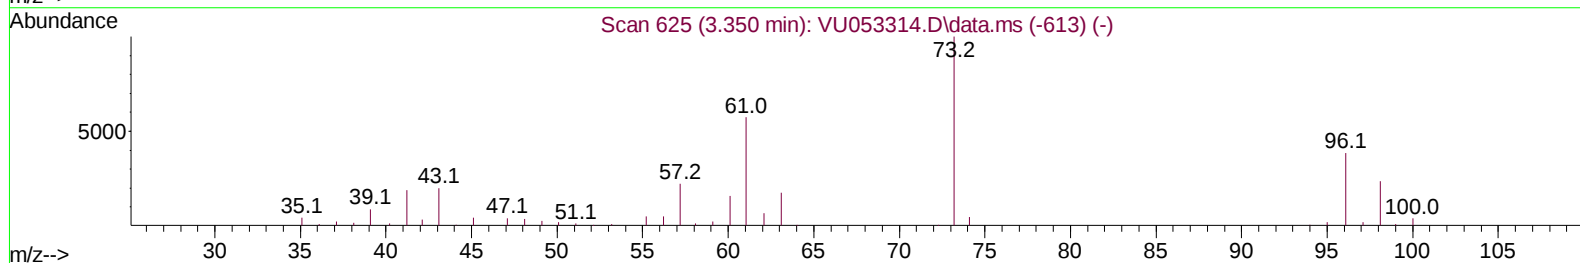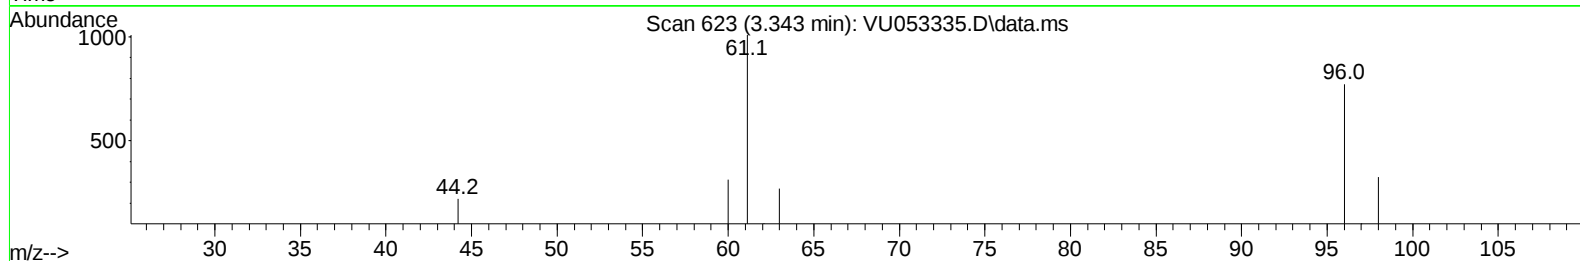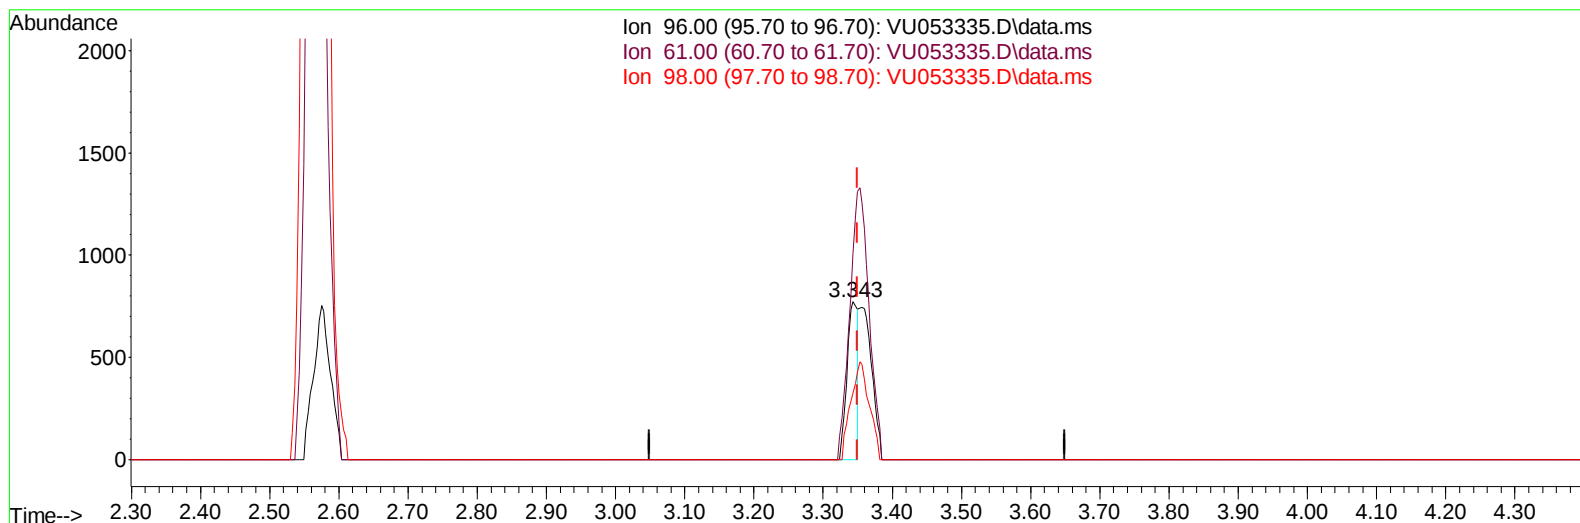

TIC: VU053335.D\data.ms

(17) trans-1,2-Dichloroethene (T)

3.343min (-0.006) 0.99 ug/L

response 826

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	142.30	130.53
98.00	65.00	42.04#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053335.D
 Acq On : 21 Mar 2023 19:30
 Operator : JC/MD
 Sample : 01995-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM8

Manual IntegrationsAPPROVED

Quant Time: Mar 22 03:13:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 22 03:08:43 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

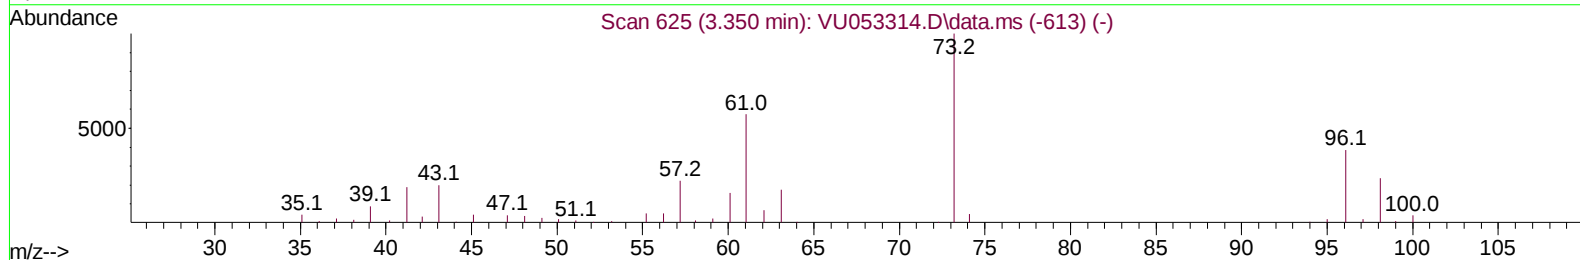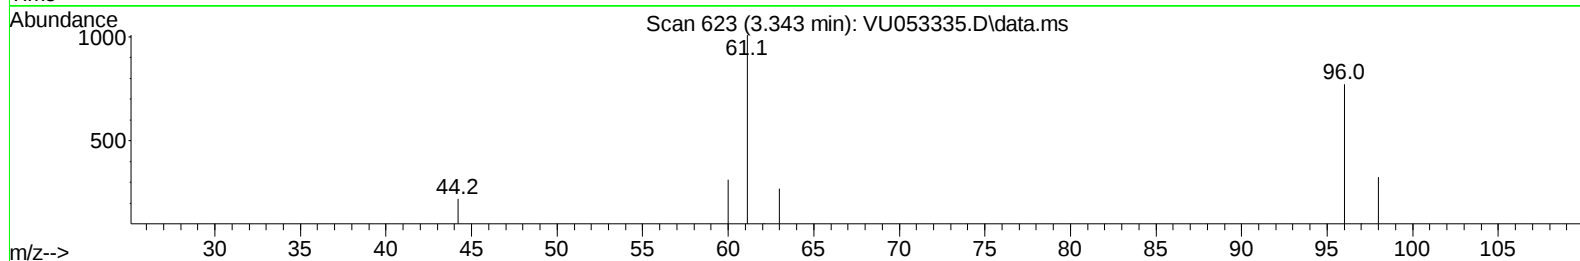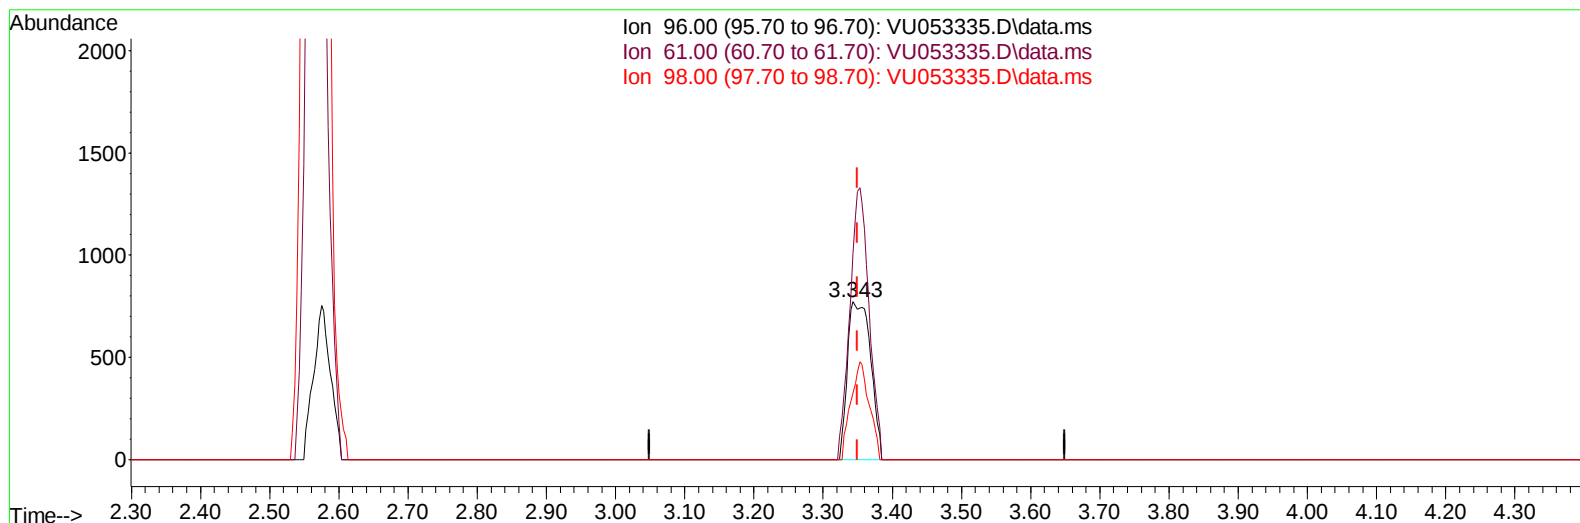

TIC: VU053335.D\data.ms

(17) trans-1,2-Dichloroethene (T)

3.343min (-0.006) 2.12 ug/L m

response 1780

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	142.30	130.53
98.00	65.00	42.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053335.D
 Acq On : 21 Mar 2023 19:30
 Operator : JC/MD
 Sample : 01995-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM8

Manual IntegrationsAPPROVED

Quant Time: Mar 22 03:13:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 22 03:08:43 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	112498	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	105961	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	48149	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43945	42.342	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	84.680%	
7) Chloroethane-d5	1.912	69	36587	43.582	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	87.160%	
11) 1,1-Dichloroethene-d2	2.565	63	54872	30.520	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	61.040%	
21) 2-Butanone-d5	4.620	46	49689	103.226	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	103.230%	
24) Chloroform-d	5.057	84	70183	41.057	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	82.120%	
26) 1,2-Dichloroethane-d4	5.697	65	48845	46.010	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.020%	
32) Benzene-d6	5.723	84	149232	43.421	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.840%	
36) 1,2-Dichloropropane-d6	6.687	67	49609	44.724	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	89.440%	
41) Toluene-d8	7.893	98	134582	42.059	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.120%	
43) trans-1,3-Dichloroprop...	8.176	79	22802	41.664	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.320%	
47) 2-Hexanone-d5	8.629	63	32703	94.302	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	94.300%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	65551	45.619	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.240%	
66) 1,2-Dichlorobenzene-d4	12.189	152	44604	47.843	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.680%	
Target Compounds						
5) Vinyl chloride	1.604	62	14842	12.539	ug/L	83
12) 1,1-Dichloroethene	2.575	96	1298	1.571	ug/L #	1
17) trans-1,2-Dichloroethene	3.343	96	1780m	2.123	ug/L	
20) cis-1,2-Dichloroethene	4.662	96	246800	250.663	ug/L	98
34) Trichloroethene	6.536	95	93016	97.108	ug/L	99
46) Tetrachloroethene	8.549	164	76307	122.448	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053335.D
Acq On : 21 Mar 2023 19:30
Operator : JC/MD
Sample : 01995-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEM8

Manual IntegrationsAPPROVED

Quant Time: Mar 22 03:13:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 22 03:08:43 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

