

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053316.D
 Acq On : 21 Mar 2023 12:07
 Operator : JC/MD
 Sample : 01929-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	66980	78710	15.71%	2.154%
2	1.912	170	178	193	rVB	62667	83978	16.77%	2.298%
3	2.565	369	381	397	rVB	100763	164901	32.92%	4.513%
4	3.041	526	529	533	rBV2	606	591	0.12%	0.016%
5	3.179	564	572	582	rBV2	936	1836	0.37%	0.050%
6	3.388	634	637	639	rBV	190	108	0.02%	0.003%
7	3.549	684	687	690	rBV	144	94	0.02%	0.003%
8	3.944	807	810	812	rBV	197	144	0.03%	0.004%
9	4.301	916	921	924	rBV	192	254	0.05%	0.007%
10	4.369	938	942	945	rBV	215	234	0.05%	0.006%
11	4.546	994	997	999	rBV	205	160	0.03%	0.004%
12	4.623	1009	1021	1044	rBV	35811	91360	18.24%	2.500%
13	4.809	1074	1079	1085	rVB2	270	300	0.06%	0.008%
14	4.838	1085	1088	1093	rVB2	306	248	0.05%	0.007%
15	4.864	1094	1096	1098	rBV	265	133	0.03%	0.004%
16	4.931	1114	1117	1121	rBV	197	220	0.04%	0.006%
17	5.057	1140	1156	1182	rBV	88958	194892	38.91%	5.333%
18	5.282	1223	1226	1229	rBB	149	97	0.02%	0.003%
19	5.304	1230	1233	1239	rBV	220	291	0.06%	0.008%
20	5.436	1268	1274	1277	rBV	219	285	0.06%	0.008%
21	5.722	1341	1363	1393	rBV2	178244	500899	100.00%	13.707%
22	5.838	1397	1399	1402	rVB	164	93	0.02%	0.003%
23	5.941	1428	1431	1433	rBV	139	123	0.02%	0.003%
24	6.044	1461	1463	1466	rVB	264	131	0.03%	0.004%
25	6.105	1479	1482	1485	rBV	177	188	0.04%	0.005%
26	6.176	1500	1504	1508	rBB	324	291	0.06%	0.008%
27	6.243	1509	1525	1543	rBV	146940	275066	54.91%	7.527%
28	6.369	1561	1564	1568	rBV2	259	258	0.05%	0.007%
29	6.488	1598	1601	1603	rBV	179	156	0.03%	0.004%
30	6.626	1640	1644	1646	rBB	169	114	0.02%	0.003%
31	6.687	1649	1663	1682	rBV2	113473	220266	43.97%	6.028%
32	6.828	1705	1707	1709	rVB	245	116	0.02%	0.003%
33	6.845	1709	1712	1714	rBV	146	122	0.02%	0.003%
34	6.886	1721	1725	1728	rBV	184	215	0.04%	0.006%
35	6.947	1741	1744	1746	rBV	179	151	0.03%	0.004%
36	6.996	1756	1759	1762	rBB	213	163	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053316.D
 Acq On : 21 Mar 2023 12:07
 Operator : JC/MD
 Sample : 01929-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.031	1767	1770	1774	rBV	142	166	0.03%	0.005%
38	7.099	1789	1791	1793	rBV	144	98	0.02%	0.003%
39	7.259	1833	1841	1845	rBB	286	387	0.08%	0.011%
40	7.365	1871	1874	1878	rBB	130	139	0.03%	0.004%
41	7.394	1879	1883	1886	rBV	174	165	0.03%	0.005%
42	7.443	1895	1898	1901	rBB	236	163	0.03%	0.004%
43	7.465	1902	1905	1907	rBV	150	124	0.02%	0.003%
44	7.507	1914	1918	1921	rBV	200	206	0.04%	0.006%
45	7.562	1923	1935	1953	rVV	64286	114334	22.83%	3.129%
46	7.626	1953	1955	1959	rVB2	346	230	0.05%	0.006%
47	7.648	1960	1962	1966	rBV2	299	257	0.05%	0.007%
48	7.703	1977	1979	1982	rBB	256	122	0.02%	0.003%
49	7.722	1982	1985	1987	rBV	160	127	0.03%	0.003%
50	7.767	1996	1999	2001	rVB	267	163	0.03%	0.004%
51	7.790	2002	2006	2007	rBV	265	137	0.03%	0.004%
52	7.893	2026	2038	2054	rBV	232721	391491	78.16%	10.713%
53	8.041	2078	2084	2087	rBV2	364	401	0.08%	0.011%
54	8.176	2114	2126	2143	rBV	43848	75227	15.02%	2.059%
55	8.237	2143	2145	2148	rVB	269	145	0.03%	0.004%
56	8.394	2191	2194	2196	rBV	182	145	0.03%	0.004%
57	8.507	2223	2229	2232	rBV	194	266	0.05%	0.007%
58	8.574	2244	2250	2254	rBV	172	257	0.05%	0.007%
59	8.629	2256	2267	2300	rVV3	99368	194913	38.91%	5.334%
60	8.819	2322	2326	2331	rBB	221	274	0.05%	0.007%
61	8.857	2332	2338	2341	rBV	225	282	0.06%	0.008%
62	8.912	2352	2355	2358	rBV	202	187	0.04%	0.005%
63	9.044	2392	2396	2400	rBV	171	227	0.05%	0.006%
64	9.124	2418	2421	2423	rBV	180	150	0.03%	0.004%
65	9.188	2438	2441	2444	rBV	138	143	0.03%	0.004%
66	9.237	2453	2456	2461	rBV	138	188	0.04%	0.005%
67	9.304	2475	2477	2479	rBV	128	92	0.02%	0.003%
68	9.414	2497	2511	2530	rBV	210241	348830	69.64%	9.546%
69	9.658	2585	2587	2588	rBV	228	109	0.02%	0.003%
70	9.690	2593	2597	2601	rVV2	439	351	0.07%	0.010%
71	9.761	2613	2619	2622	rBV	168	246	0.05%	0.007%
72	9.867	2648	2652	2656	rBV	249	286	0.06%	0.008%
73	9.967	2680	2683	2685	rBV	189	153	0.03%	0.004%
74	10.012	2692	2697	2700	rBV	184	233	0.05%	0.006%
75	10.118	2721	2730	2739	rBV6	2394	3451	0.69%	0.094%
76	10.198	2752	2755	2757	rBV	137	115	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053316.D
 Acq On : 21 Mar 2023 12:07
 Operator : JC/MD
 Sample : 01929-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.243	2765	2769	2772	rBV2	202	137	0.03%	0.004%
78	10.352	2799	2803	2808	rBB	334	305	0.06%	0.008%
79	10.391	2811	2815	2820	rBV	260	354	0.07%	0.010%
80	10.751	2915	2927	2941	rBV	149914	236493	47.21%	6.472%
81	10.825	2947	2950	2955	rVB3	404	405	0.08%	0.011%
82	10.995	3000	3003	3004	rBV	151	104	0.02%	0.003%
83	11.089	3030	3032	3037	rVB2	247	181	0.04%	0.005%
84	11.266	3081	3087	3088	rBV	178	217	0.04%	0.006%
85	11.304	3095	3099	3104	rBB	367	328	0.07%	0.009%
86	11.330	3104	3107	3111	rBV	159	195	0.04%	0.005%
87	11.423	3134	3136	3138	rBV	147	99	0.02%	0.003%
88	11.558	3174	3178	3180	rBV	221	202	0.04%	0.006%
89	11.658	3204	3209	3213	rBV	305	352	0.07%	0.010%
90	11.745	3231	3236	3240	rVB2	340	341	0.07%	0.009%
91	11.806	3243	3255	3280	rBV	203586	326074	65.10%	8.923%
92	12.188	3362	3374	3393	rBV	203945	330080	65.90%	9.033%
93	12.458	3455	3458	3461	rBV	267	241	0.05%	0.007%
94	13.224	3693	3696	3701	rVB2	483	440	0.09%	0.012%
95	13.847	3882	3890	3893	rBV3	1116	1124	0.22%	0.031%
96	14.089	3959	3965	3984	rVV	1229	2801	0.56%	0.077%
97	14.330	4035	4040	4050	rBV	842	1102	0.22%	0.030%
98	15.137	4288	4291	4295	rBV2	213	169	0.03%	0.005%
99	15.346	4352	4356	4357	rBV	207	170	0.03%	0.005%
100	15.555	4419	4421	4424	rBV2	258	170	0.03%	0.005%




Sum of corrected areas: 3654252

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053316.D
Acq On : 21 Mar 2023 12:07
Operator : JC/MD
Sample : 01929-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

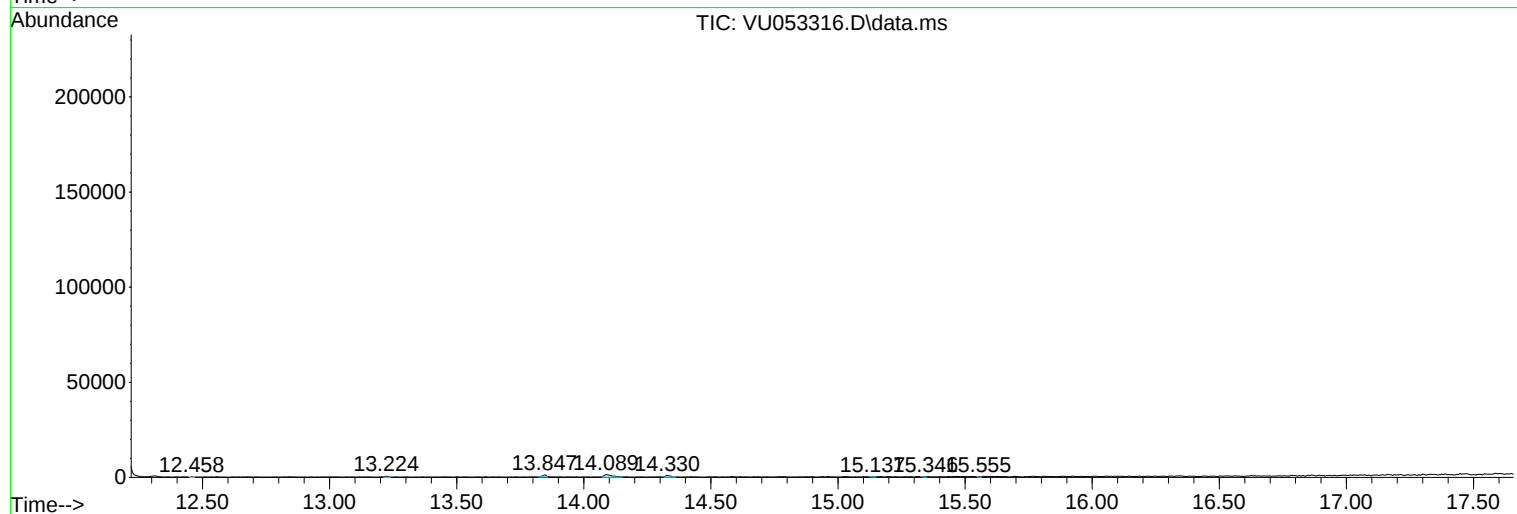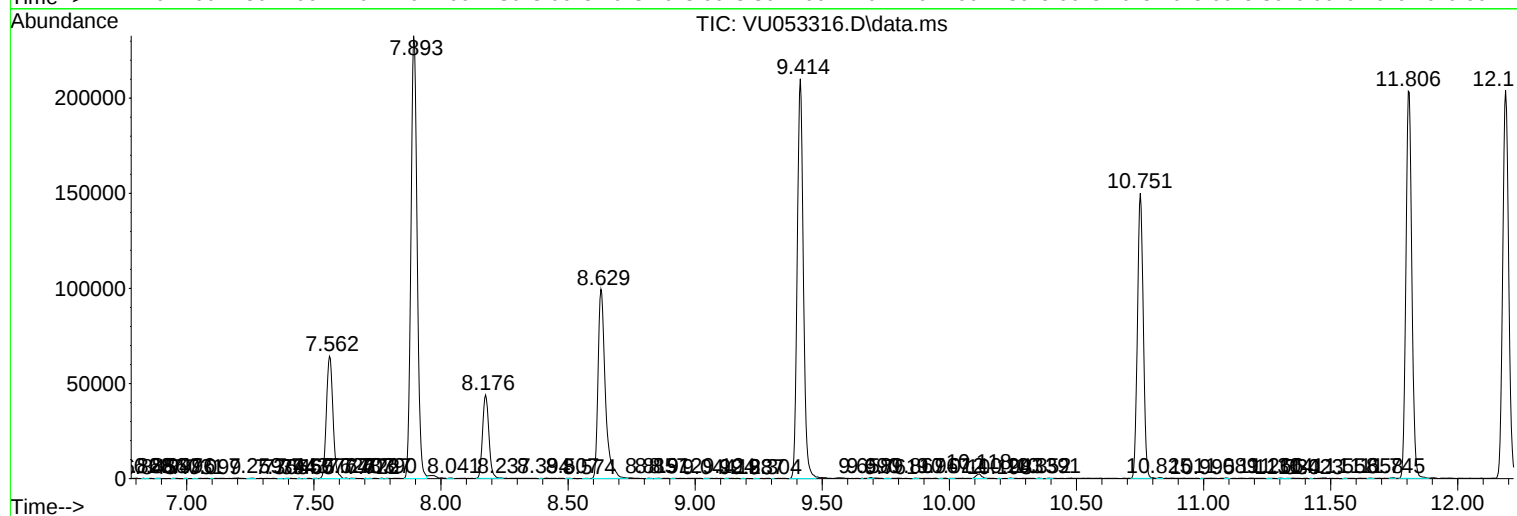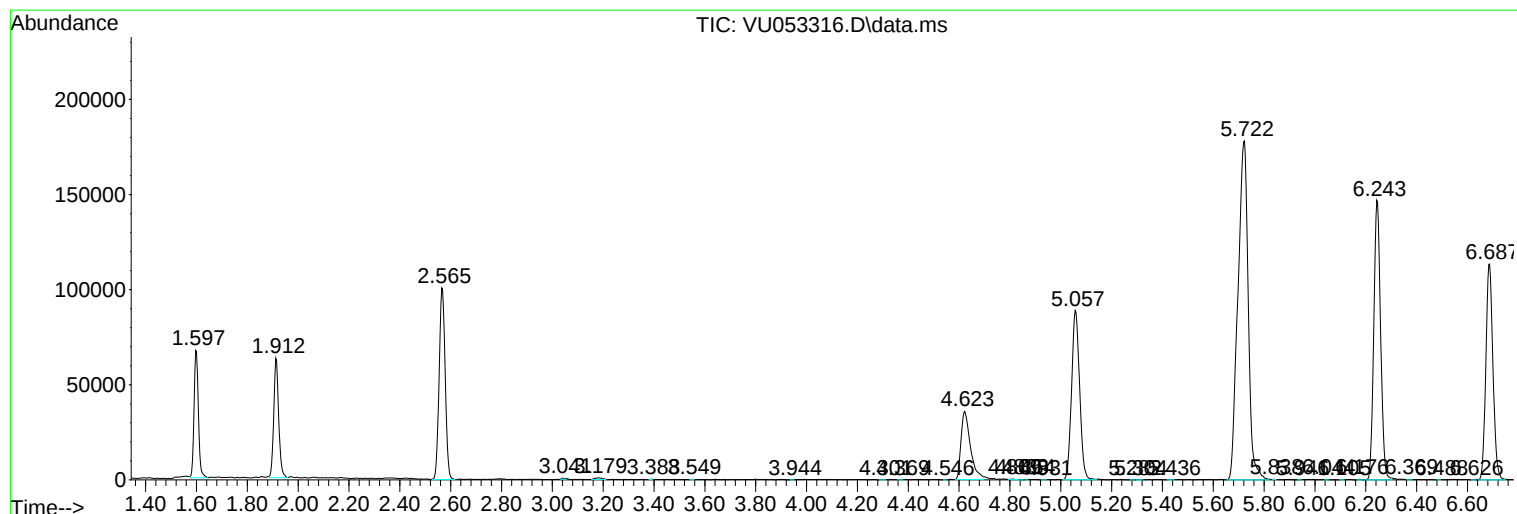

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053316.D
Acq On : 21 Mar 2023 12:07
Operator : JC/MD
Sample : 01929-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053316.D
Acq On : 21 Mar 2023 12:07
Operator : JC/MD
Sample : 01929-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc