

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053317.D
 Acq On : 21 Mar 2023 12:30
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

Signal : TIC: VU053317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB2	137701	168624	34.85%	4.697%
2	1.912	170	178	193	rVB	59338	79479	16.43%	2.214%
3	2.565	369	381	394	rBV	101287	163861	33.87%	4.564%
4	2.642	399	405	412	rBV2	342	491	0.10%	0.014%
5	2.790	446	451	462	rBV2	518	664	0.14%	0.018%
6	3.044	524	530	540	rVB2	896	1199	0.25%	0.033%
7	3.173	567	570	571	rBV	221	138	0.03%	0.004%
8	3.321	612	616	619	rBB	180	169	0.03%	0.005%
9	3.350	620	625	629	rBV2	406	464	0.10%	0.013%
10	3.623	707	710	712	rBV	197	158	0.03%	0.004%
11	4.044	839	841	843	rVB	273	130	0.03%	0.004%
12	4.060	843	846	849	rBV	204	185	0.04%	0.005%
13	4.150	871	874	876	rBV	225	171	0.04%	0.005%
14	4.404	951	953	955	rBV	194	124	0.03%	0.003%
15	4.539	992	995	996	rBV	166	114	0.02%	0.003%
16	4.623	1009	1021	1022	rBV	32437	44504	9.20%	1.240%
17	4.832	1083	1086	1088	rBV2	218	112	0.02%	0.003%
18	4.941	1118	1120	1123	rBB	146	100	0.02%	0.003%
19	4.960	1123	1126	1129	rBV	168	164	0.03%	0.005%
20	5.057	1142	1156	1175	rBV	86684	190519	39.38%	5.307%
21	5.208	1200	1203	1205	rBV	154	135	0.03%	0.004%
22	5.269	1220	1222	1224	rBV	128	90	0.02%	0.003%
23	5.504	1292	1295	1301	rBB	234	270	0.06%	0.008%
24	5.530	1301	1303	1306	rBB	175	118	0.02%	0.003%
25	5.565	1311	1314	1315	rBV	208	107	0.02%	0.003%
26	5.616	1327	1330	1332	rBV	140	127	0.03%	0.004%
27	5.719	1341	1362	1394	rBV2	175978	483804	100.00%	13.476%
28	5.829	1394	1396	1402	rBV2	268	251	0.05%	0.007%
29	5.870	1407	1409	1411	rBB	221	107	0.02%	0.003%
30	5.893	1412	1416	1418	rBV	252	192	0.04%	0.005%
31	5.935	1427	1429	1432	rBV	244	154	0.03%	0.004%
32	5.957	1432	1436	1439	rVV2	214	167	0.03%	0.005%
33	6.060	1465	1468	1470	rBV	163	129	0.03%	0.004%
34	6.124	1485	1488	1492	rBB	184	177	0.04%	0.005%
35	6.153	1493	1497	1502	rBV	194	220	0.05%	0.006%
36	6.243	1512	1525	1547	rBV	149702	278403	57.54%	7.755%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053317.D
 Acq On : 21 Mar 2023 12:30
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.388	1568	1570	1571	rBV	251	108	0.02%	0.003%
38	6.526	1610	1613	1615	rBV	281	185	0.04%	0.005%
39	6.613	1637	1640	1642	rBV	259	189	0.04%	0.005%
40	6.684	1649	1662	1681	rBV2	110101	213371	44.10%	5.943%
41	6.771	1686	1689	1691	rBV2	265	193	0.04%	0.005%
42	6.816	1702	1703	1705	rVB	248	91	0.02%	0.003%
43	6.835	1706	1709	1714	rBV	148	185	0.04%	0.005%
44	6.941	1738	1742	1745	rBV	212	180	0.04%	0.005%
45	7.002	1759	1761	1765	rBV	140	146	0.03%	0.004%
46	7.025	1765	1768	1770	rVB	222	145	0.03%	0.004%
47	7.105	1790	1793	1797	rBB	177	174	0.04%	0.005%
48	7.124	1797	1799	1801	rBV	124	90	0.02%	0.003%
49	7.189	1816	1819	1820	rBV	276	129	0.03%	0.004%
50	7.227	1828	1831	1833	rBV	199	153	0.03%	0.004%
51	7.279	1845	1847	1849	rBV	145	105	0.02%	0.003%
52	7.446	1896	1899	1902	rBV2	297	252	0.05%	0.007%
53	7.562	1923	1935	1954	rBV	62874	109080	22.55%	3.038%
54	7.655	1961	1964	1965	rBV	114	85	0.02%	0.002%
55	7.732	1986	1988	1993	rBV	159	186	0.04%	0.005%
56	7.780	1998	2003	2009	rBB	221	292	0.06%	0.008%
57	7.816	2009	2014	2017	rBV	289	264	0.05%	0.007%
58	7.893	2025	2038	2055	rBV	221137	381583	78.87%	10.629%
59	8.002	2070	2072	2079	rVV2	277	317	0.07%	0.009%
60	8.050	2083	2087	2091	rVB2	257	172	0.04%	0.005%
61	8.121	2105	2109	2112	rBV	145	148	0.03%	0.004%
62	8.173	2115	2125	2145	rVB	43321	73343	15.16%	2.043%
63	8.311	2165	2168	2170	rBV	176	152	0.03%	0.004%
64	8.488	2220	2223	2226	rBV	155	164	0.03%	0.005%
65	8.526	2233	2235	2239	rBB	139	121	0.03%	0.003%
66	8.591	2252	2255	2256	rBV	196	123	0.03%	0.003%
67	8.629	2256	2267	2294	rBV3	94977	179327	37.07%	4.995%
68	9.172	2431	2436	2440	rBV	342	319	0.07%	0.009%
69	9.414	2497	2511	2532	rBV	208267	347637	71.85%	9.683%
70	9.610	2568	2572	2575	rBB	185	175	0.04%	0.005%
71	9.639	2576	2581	2584	rBV	255	296	0.06%	0.008%
72	9.677	2590	2593	2596	rVB2	190	120	0.02%	0.003%
73	9.697	2596	2599	2600	rBV	235	137	0.03%	0.004%
74	9.754	2613	2617	2619	rBV	152	154	0.03%	0.004%
75	9.796	2628	2630	2633	rBV	192	149	0.03%	0.004%
76	9.896	2659	2661	2663	rBV	186	132	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053317.D
 Acq On : 21 Mar 2023 12:30
 Operator : JC/MD
 Sample : 01930-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.015	2695	2698	2700	rBV	208	174	0.04%	0.005%
78	10.111	2721	2728	2738	rBV4	1557	2756	0.57%	0.077%
79	10.176	2743	2748	2751	rBV	181	240	0.05%	0.007%
80	10.407	2817	2820	2823	rBV	213	209	0.04%	0.006%
81	10.491	2841	2846	2849	rBV2	400	349	0.07%	0.010%
82	10.545	2861	2863	2867	rBV	271	235	0.05%	0.007%
83	10.751	2915	2927	2942	rBV	144947	228618	47.25%	6.368%
84	10.822	2946	2949	2963	rVB3	442	524	0.11%	0.015%
85	10.983	2992	2999	3003	rBV	218	337	0.07%	0.009%
86	11.063	3021	3024	3027	rBV	183	134	0.03%	0.004%
87	11.127	3042	3044	3047	rVB	195	85	0.02%	0.002%
88	11.806	3243	3255	3281	rBV	201037	317614	65.65%	8.847%
89	11.896	3281	3283	3286	rVV	268	162	0.03%	0.005%
90	11.922	3288	3291	3294	rVB2	303	153	0.03%	0.004%
91	12.188	3362	3374	3391	rBV	194572	308736	63.81%	8.600%
92	12.275	3398	3401	3406	rBV2	186	184	0.04%	0.005%
93	12.311	3408	3412	3419	rVB3	526	722	0.15%	0.020%
94	12.713	3530	3537	3541	rBV	254	398	0.08%	0.011%
95	12.832	3572	3574	3577	rVB	235	94	0.02%	0.003%
96	14.098	3957	3968	3980	rBV2	654	1511	0.31%	0.042%
97	14.333	4038	4041	4042	rBV2	399	229	0.05%	0.006%
98	14.934	4226	4228	4231	rVB	320	111	0.02%	0.003%
99	15.266	4327	4331	4332	rBV	227	143	0.03%	0.004%
100	15.372	4361	4364	4371	rBV	231	293	0.06%	0.008%




Sum of corrected areas: 3590004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053317.D
Acq On : 21 Mar 2023 12:30
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

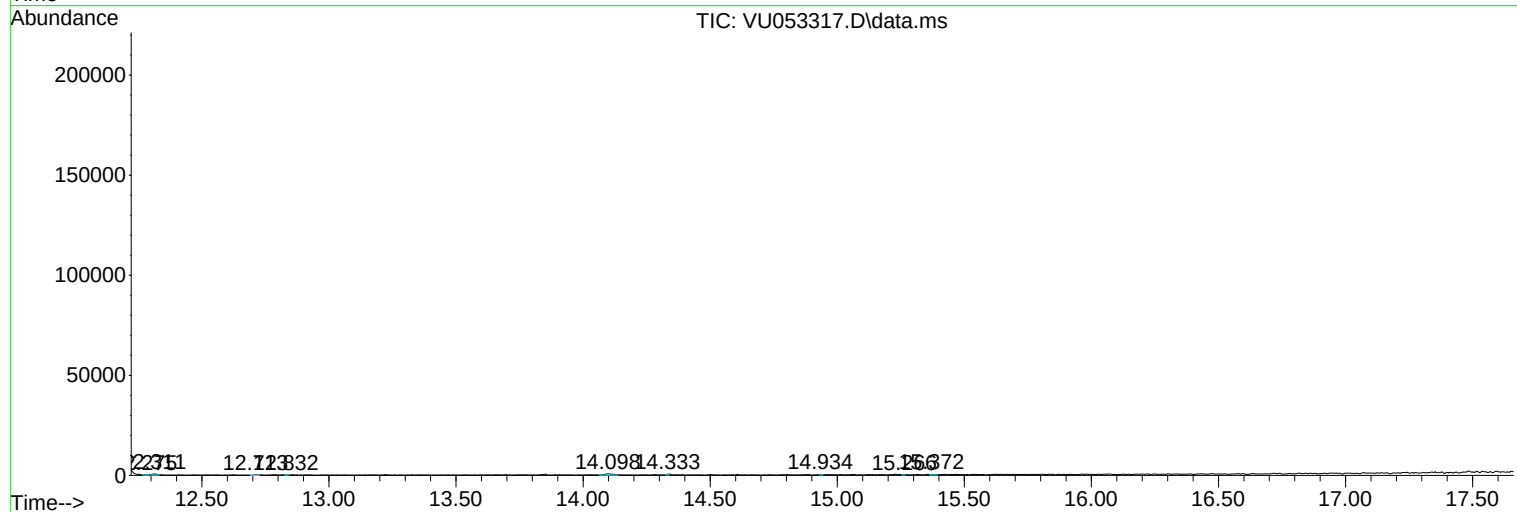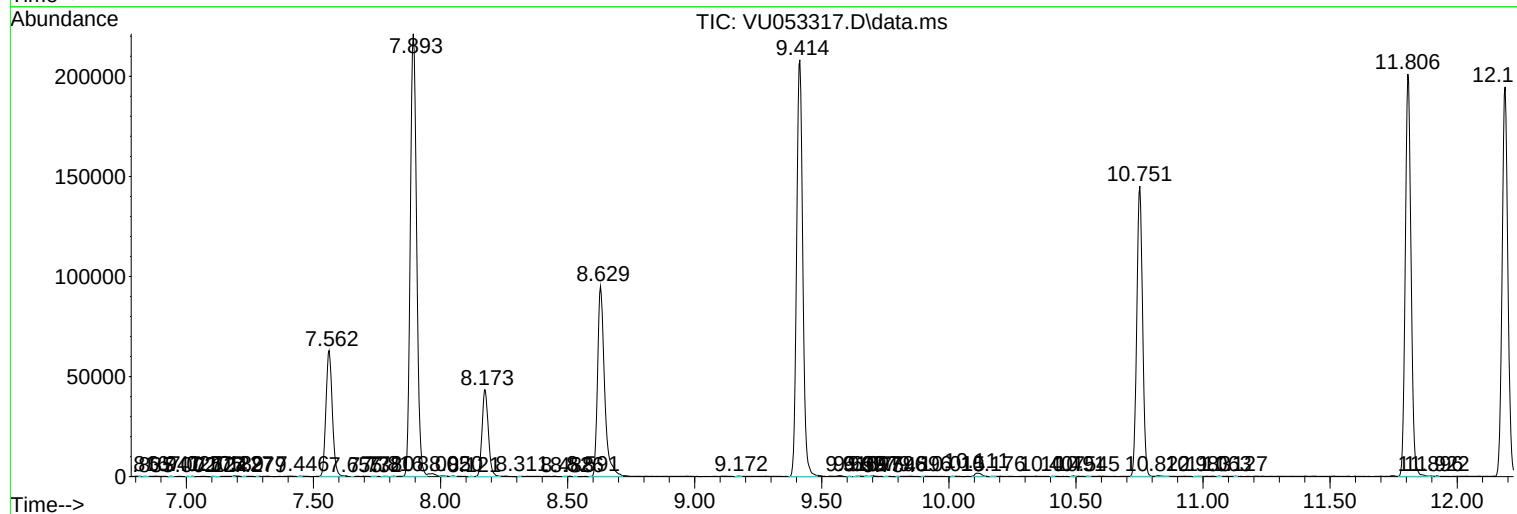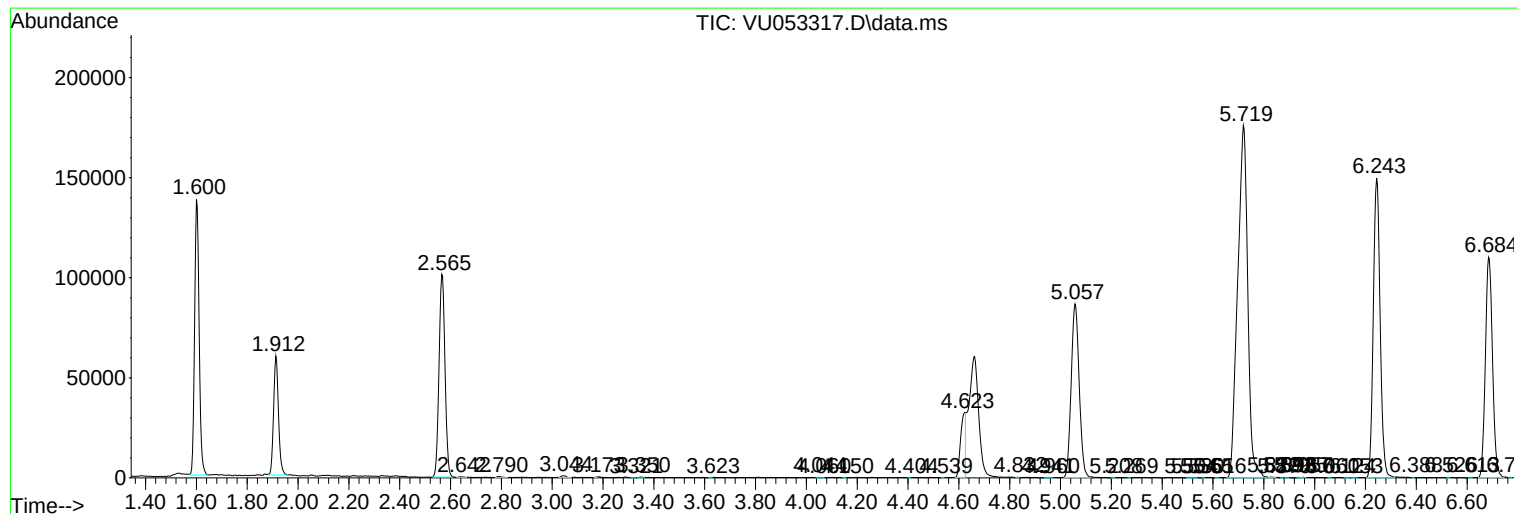

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053317.D
Acq On : 21 Mar 2023 12:30
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053317.D
Acq On : 21 Mar 2023 12:30
Operator : JC/MD
Sample : 01930-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------