

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053322.D
 Acq On : 21 Mar 2023 14:27
 Operator : JC/MD
 Sample : 01980-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	99	rVB	68213	77251	16.56%	2.209%
2	1.912	170	178	193	rVB	60068	81898	17.55%	2.342%
3	2.565	370	381	398	rVB	99665	160402	34.38%	4.587%
4	3.851	778	781	783	rBV	154	126	0.03%	0.004%
5	4.507	982	985	988	rBV	204	189	0.04%	0.005%
6	4.562	997	1002	1005	rBV	175	226	0.05%	0.006%
7	4.620	1008	1020	1051	rVV2	33643	85535	18.33%	2.446%
8	4.800	1072	1076	1080	rBV2	233	263	0.06%	0.008%
9	4.835	1085	1087	1089	rVB2	165	69	0.01%	0.002%
10	4.867	1094	1097	1100	rVV	168	82	0.02%	0.002%
11	4.903	1106	1108	1109	rBV	135	43	0.01%	0.001%
12	5.057	1141	1156	1178	rBV2	85271	185222	39.70%	5.297%
13	5.256	1215	1218	1219	rBV	135	95	0.02%	0.003%
14	5.414	1263	1267	1270	rBV	223	207	0.04%	0.006%
15	5.449	1276	1278	1283	rBV2	264	231	0.05%	0.007%
16	5.533	1301	1304	1309	rBV	231	304	0.07%	0.009%
17	5.607	1324	1327	1329	rBV	176	146	0.03%	0.004%
18	5.719	1341	1362	1392	rBV2	170925	466572	100.00%	13.342%
19	5.838	1396	1399	1407	rVB3	353	424	0.09%	0.012%
20	5.883	1408	1413	1418	rVB2	205	187	0.04%	0.005%
21	5.951	1433	1434	1435	rBB2	111	21	0.00%	0.001%
22	5.977	1439	1442	1443	rBV	115	86	0.02%	0.002%
23	6.038	1456	1461	1466	rBV	164	241	0.05%	0.007%
24	6.144	1492	1494	1496	rBV	128	91	0.02%	0.003%
25	6.243	1510	1525	1549	rBV	148349	278947	59.79%	7.977%
26	6.369	1561	1564	1569	rVB	407	383	0.08%	0.011%
27	6.395	1570	1572	1573	rBB	107	21	0.00%	0.001%
28	6.411	1573	1577	1579	rBV	140	145	0.03%	0.004%
29	6.478	1595	1598	1600	rBV	172	144	0.03%	0.004%
30	6.571	1626	1627	1628	rBV	103	20	0.00%	0.001%
31	6.623	1640	1643	1645	rBV	145	126	0.03%	0.004%
32	6.684	1649	1662	1688	rVB	109785	210672	45.15%	6.025%
33	6.893	1722	1727	1731	rBV	171	241	0.05%	0.007%
34	6.944	1740	1743	1745	rBV	191	147	0.03%	0.004%
35	6.993	1754	1758	1762	rBV	216	209	0.04%	0.006%
36	7.063	1777	1780	1782	rBV	179	93	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053322.D
 Acq On : 21 Mar 2023 14:27
 Operator : JC/MD
 Sample : 01980-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.150	1803	1807	1812	rBV	205	248	0.05%	0.007%
38	7.247	1831	1837	1839	rBV	209	250	0.05%	0.007%
39	7.279	1845	1847	1849	rBV	141	96	0.02%	0.003%
40	7.391	1878	1882	1883	rBV	142	127	0.03%	0.004%
41	7.452	1896	1901	1907	rBB	222	352	0.08%	0.010%
42	7.478	1907	1909	1911	rBV	127	91	0.02%	0.003%
43	7.559	1923	1934	1952	rBV	60902	106974	22.93%	3.059%
44	7.771	1998	2000	2002	rBV	142	92	0.02%	0.003%
45	7.893	2025	2038	2056	rBV	217519	369984	79.30%	10.580%
46	8.012	2073	2075	2081	rVB2	349	235	0.05%	0.007%
47	8.044	2081	2085	2087	rBV2	244	181	0.04%	0.005%
48	8.176	2115	2126	2148	rBV	41278	70435	15.10%	2.014%
49	8.298	2160	2164	2166	rBV	179	186	0.04%	0.005%
50	8.337	2172	2176	2179	rBV	189	197	0.04%	0.006%
51	8.440	2201	2208	2211	rBV	193	293	0.06%	0.008%
52	8.555	2242	2244	2247	rBB	127	65	0.01%	0.002%
53	8.578	2248	2251	2254	rBV	174	173	0.04%	0.005%
54	8.629	2255	2267	2292	rBV2	100099	189238	40.56%	5.412%
55	8.832	2327	2330	2332	rBV	124	66	0.01%	0.002%
56	9.002	2376	2383	2385	rBV	179	250	0.05%	0.007%
57	9.025	2387	2390	2395	rVB	312	238	0.05%	0.007%
58	9.105	2411	2415	2417	rBV	145	148	0.03%	0.004%
59	9.411	2498	2510	2529	rBV	204717	345926	74.14%	9.892%
60	9.546	2549	2552	2554	rBV	194	124	0.03%	0.004%
61	9.610	2570	2572	2573	rBV	147	80	0.02%	0.002%
62	9.706	2597	2602	2606	rBB	214	212	0.05%	0.006%
63	9.729	2607	2609	2611	rBV	172	120	0.03%	0.003%
64	9.816	2631	2636	2638	rBV	328	328	0.07%	0.009%
65	9.970	2681	2684	2687	rBV	183	166	0.04%	0.005%
66	10.121	2724	2731	2738	rVB3	1606	2155	0.46%	0.062%
67	10.208	2755	2758	2762	rBB	184	174	0.04%	0.005%
68	10.230	2762	2765	2770	rBB	169	182	0.04%	0.005%
69	10.256	2770	2773	2775	rBV	213	168	0.04%	0.005%
70	10.427	2823	2826	2829	rVB	249	188	0.04%	0.005%
71	10.449	2829	2833	2837	rBB	221	219	0.05%	0.006%
72	10.475	2840	2841	2842	rBV	229	76	0.02%	0.002%
73	10.542	2861	2862	2865	rVB	262	120	0.03%	0.003%
74	10.751	2915	2927	2947	rVB	139898	223930	47.99%	6.404%
75	10.825	2947	2950	2951	rBV	211	115	0.02%	0.003%
76	11.083	3026	3030	3033	rBB	298	192	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053322.D
 Acq On : 21 Mar 2023 14:27
 Operator : JC/MD
 Sample : 01980-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.105	3034	3037	3041	rBV	210	222	0.05%	0.006%
78	11.417	3130	3134	3137	rBV	197	229	0.05%	0.007%
79	11.507	3160	3162	3164	rBV	177	62	0.01%	0.002%
80	11.806	3244	3255	3269	rBV	204094	320936	68.79%	9.178%
81	11.883	3278	3279	3280	rBV	245	90	0.02%	0.003%
82	12.099	3343	3346	3352	rBV	167	190	0.04%	0.005%
83	12.189	3362	3374	3388	rBV	189395	308308	66.08%	8.817%
84	12.282	3399	3403	3406	rBV	266	182	0.04%	0.005%
85	12.681	3524	3527	3532	rBV	195	177	0.04%	0.005%
86	12.841	3574	3577	3582	rBV2	155	121	0.03%	0.003%
87	13.751	3858	3860	3862	rBV	146	47	0.01%	0.001%
88	14.105	3965	3970	3976	rVB	520	516	0.11%	0.015%
89	14.243	4011	4013	4016	rVB	165	44	0.01%	0.001%
90	14.812	4188	4190	4191	rBV	139	46	0.01%	0.001%
91	15.246	4321	4325	4327	rBV	335	222	0.05%	0.006%
92	15.394	4369	4371	4373	rBV	144	67	0.01%	0.002%




Sum of corrected areas: 3496912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053322.D
Acq On : 21 Mar 2023 14:27
Operator : JC/MD
Sample : 01980-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

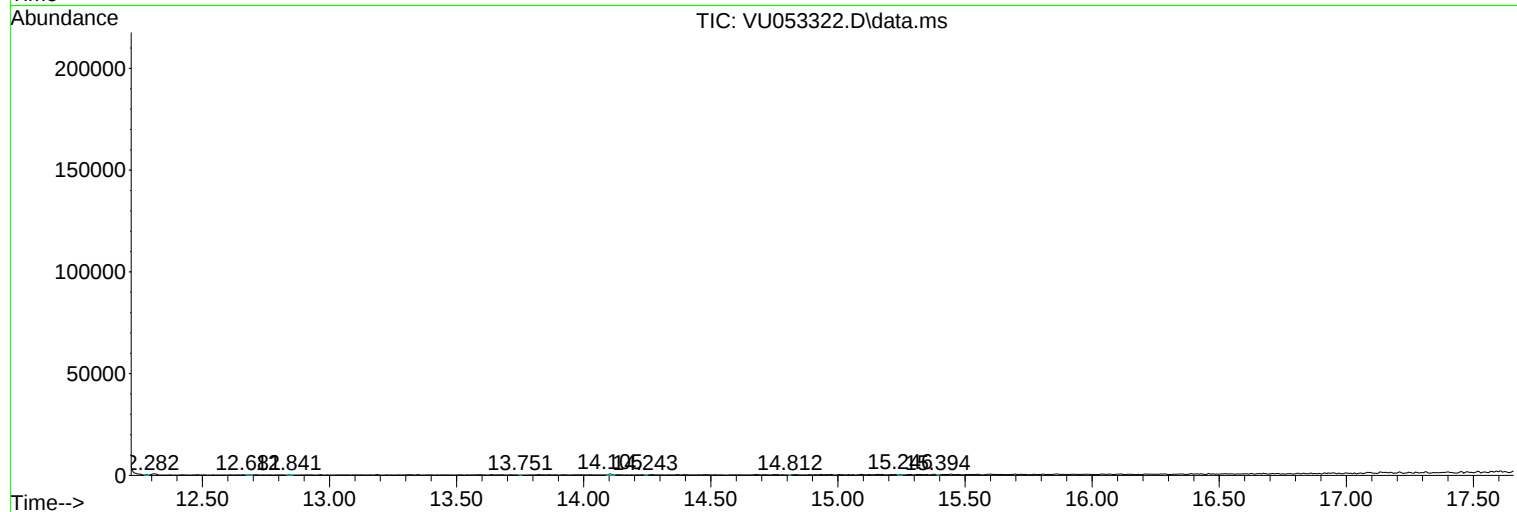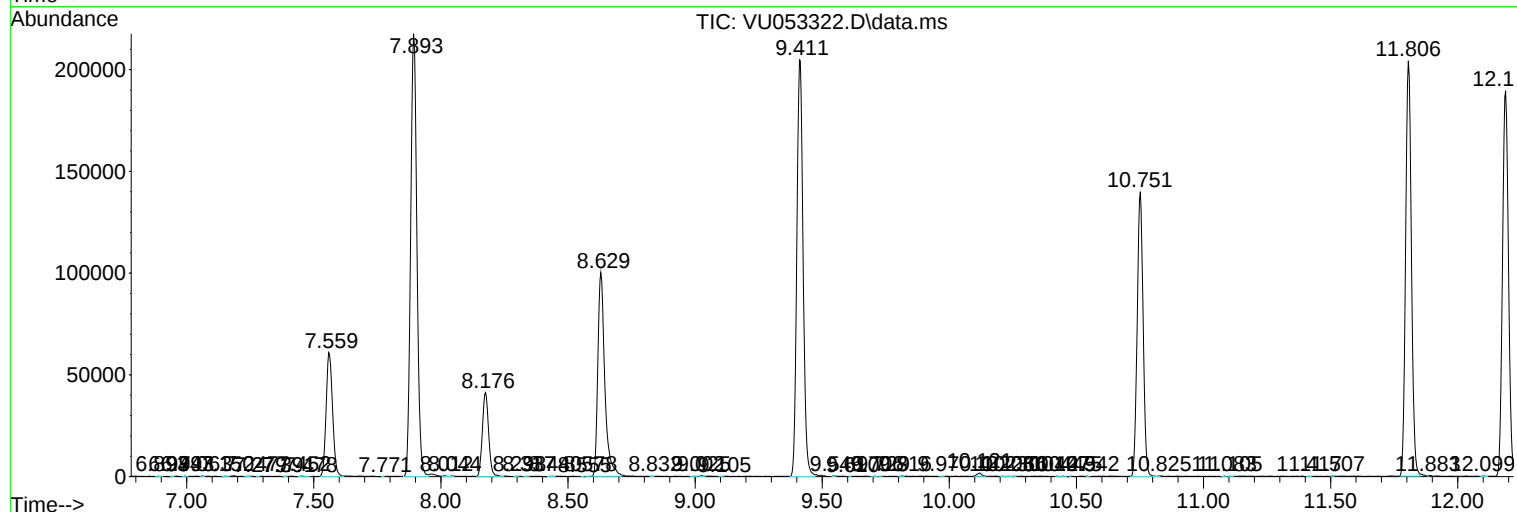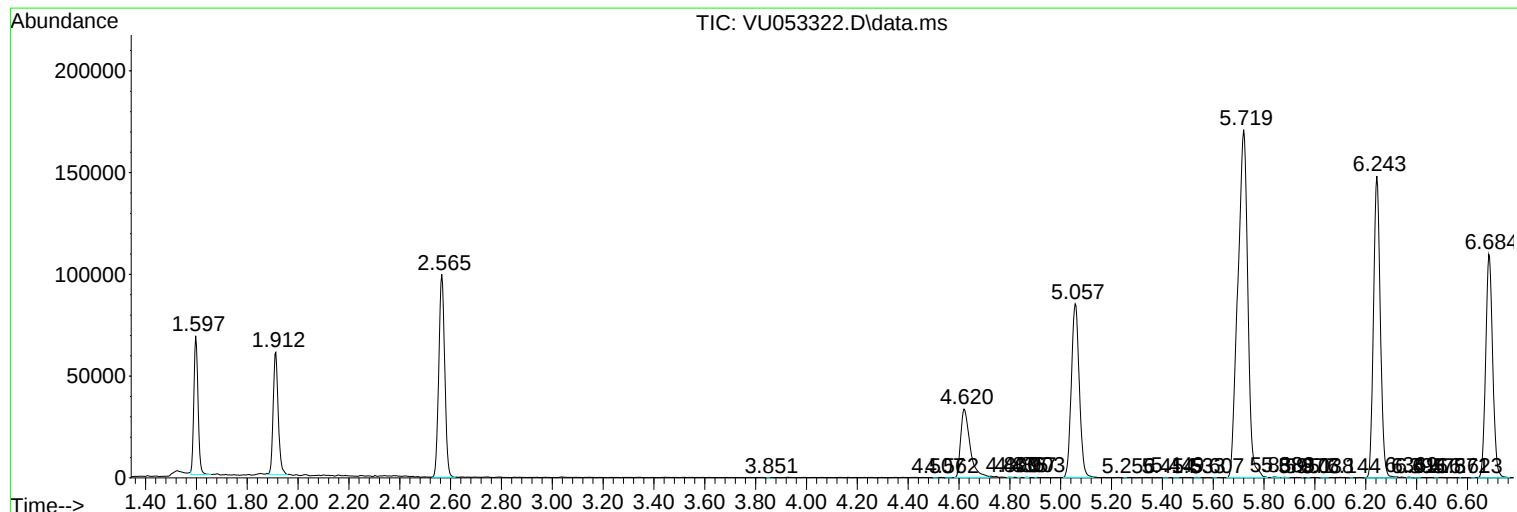

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053322.D
Acq On : 21 Mar 2023 14:27
Operator : JC/MD
Sample : 01980-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053322.D
Acq On : 21 Mar 2023 14:27
Operator : JC/MD
Sample : 01980-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc