

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053324.D
 Acq On : 21 Mar 2023 15:13
 Operator : JC/MD
 Sample : 01961-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	66699	75414	16.14%	2.168%
2	1.912	170	178	194	rVB	56657	77047	16.49%	2.215%
3	2.565	369	381	394	rBV	96746	154248	33.01%	4.434%
4	2.633	394	402	417	rVB	2094	3876	0.83%	0.111%
5	3.620	705	709	710	rBV	176	141	0.03%	0.004%
6	3.816	768	770	772	rBV	202	90	0.02%	0.003%
7	3.957	811	814	816	rBV	170	134	0.03%	0.004%
8	4.125	863	866	867	rBV	176	121	0.03%	0.003%
9	4.224	893	897	902	rBV	167	273	0.06%	0.008%
10	4.318	923	926	927	rBV	279	153	0.03%	0.004%
11	4.346	933	935	942	rVB	188	85	0.02%	0.002%
12	4.620	1008	1020	1042	rBV2	33095	83092	17.78%	2.389%
13	4.973	1126	1130	1134	rBV	215	248	0.05%	0.007%
14	5.057	1141	1156	1176	rBV2	83968	181207	38.77%	5.209%
15	5.179	1187	1194	1199	rBV	233	372	0.08%	0.011%
16	5.234	1208	1211	1213	rBV	131	113	0.02%	0.003%
17	5.327	1238	1240	1243	rVB	186	76	0.02%	0.002%
18	5.411	1262	1266	1274	rBV	202	341	0.07%	0.010%
19	5.446	1274	1277	1279	rBV	120	72	0.02%	0.002%
20	5.636	1332	1336	1338	rBV	307	221	0.05%	0.006%
21	5.719	1342	1362	1394	rBV2	168000	467340	100.00%	13.435%
22	5.854	1402	1404	1406	rVB2	140	61	0.01%	0.002%
23	5.932	1423	1428	1430	rBV	290	272	0.06%	0.008%
24	5.986	1438	1445	1449	rBV	228	339	0.07%	0.010%
25	6.102	1479	1481	1482	rBV	145	78	0.02%	0.002%
26	6.157	1495	1498	1500	rBV	202	172	0.04%	0.005%
27	6.243	1511	1525	1547	rBV2	151321	278388	59.57%	8.003%
28	6.353	1555	1559	1562	rBV	212	256	0.05%	0.007%
29	6.391	1568	1571	1574	rBV	186	102	0.02%	0.003%
30	6.427	1579	1582	1583	rBV	294	161	0.03%	0.005%
31	6.494	1600	1603	1607	rBV	207	223	0.05%	0.006%
32	6.510	1607	1608	1609	rBV	134	35	0.01%	0.001%
33	6.565	1623	1625	1628	rBV	144	47	0.01%	0.001%
34	6.684	1649	1662	1682	rBV2	106081	205676	44.01%	5.913%
35	6.758	1683	1685	1686	rVV	195	74	0.02%	0.002%
36	6.777	1689	1691	1693	rVB	322	170	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053324.D
 Acq On : 21 Mar 2023 15:13
 Operator : JC/MD
 Sample : 01961-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.793	1694	1696	1698	rBB	125	48	0.01%	0.001%
38	6.809	1699	1701	1702	rBV	245	118	0.03%	0.003%
39	6.829	1705	1707	1709	rVB	120	51	0.01%	0.001%
40	6.896	1724	1728	1732	rBV	255	293	0.06%	0.008%
41	7.015	1759	1765	1772	rBB	201	352	0.08%	0.010%
42	7.047	1773	1775	1776	rBV	152	81	0.02%	0.002%
43	7.337	1863	1865	1867	rBV	162	113	0.02%	0.003%
44	7.427	1890	1893	1895	rBB	117	64	0.01%	0.002%
45	7.456	1895	1902	1908	rBB	202	380	0.08%	0.011%
46	7.485	1908	1911	1914	rBV	149	163	0.03%	0.005%
47	7.562	1923	1935	1952	rVB	59387	106799	22.85%	3.070%
48	7.629	1952	1956	1959	rBV2	177	191	0.04%	0.005%
49	7.697	1975	1977	1978	rBV2	140	34	0.01%	0.001%
50	7.761	1995	1997	2000	rBV	179	82	0.02%	0.002%
51	7.809	2010	2012	2018	rBV	162	208	0.04%	0.006%
52	7.893	2026	2038	2057	rBV	214023	364512	78.00%	10.479%
53	8.079	2094	2096	2097	rBV	156	84	0.02%	0.002%
54	8.128	2108	2111	2113	rBB	188	124	0.03%	0.004%
55	8.176	2113	2126	2141	rBV	40979	69980	14.97%	2.012%
56	8.253	2147	2150	2151	rBV	301	151	0.03%	0.004%
57	8.343	2173	2178	2183	rBV	236	362	0.08%	0.010%
58	8.462	2212	2215	2220	rBV	208	247	0.05%	0.007%
59	8.523	2230	2234	2237	rBV	203	201	0.04%	0.006%
60	8.629	2255	2267	2298	rBV3	100331	188914	40.42%	5.431%
61	8.768	2308	2310	2313	rVB	202	108	0.02%	0.003%
62	8.915	2353	2356	2357	rBV	138	57	0.01%	0.002%
63	9.025	2386	2390	2393	rBV	248	192	0.04%	0.006%
64	9.337	2486	2487	2491	rVB	243	120	0.03%	0.003%
65	9.359	2492	2494	2495	rBV	122	66	0.01%	0.002%
66	9.411	2498	2510	2535	rVV	208643	345896	74.01%	9.944%
67	9.526	2542	2546	2547	rBV	263	178	0.04%	0.005%
68	9.607	2568	2571	2576	rBB	220	225	0.05%	0.006%
69	9.639	2577	2581	2588	rBV	247	354	0.08%	0.010%
70	9.694	2593	2598	2602	rVB2	209	220	0.05%	0.006%
71	9.751	2611	2616	2619	rBV	207	272	0.06%	0.008%
72	9.845	2639	2645	2649	rBV	173	293	0.06%	0.008%
73	9.954	2677	2679	2682	rBV	249	137	0.03%	0.004%
74	9.993	2685	2691	2694	rBV	298	390	0.08%	0.011%
75	10.028	2700	2702	2707	rVB	174	109	0.02%	0.003%
76	10.092	2720	2722	2724	rBV	143	54	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053324.D
 Acq On : 21 Mar 2023 15:13
 Operator : JC/MD
 Sample : 01961-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.115	2724	2729	2738	rBV3	1435	1896	0.41%	0.055%
78	10.317	2789	2792	2794	rBV	180	137	0.03%	0.004%
79	10.645	2891	2894	2898	rBV	188	219	0.05%	0.006%
80	10.690	2905	2908	2912	rBV	218	225	0.05%	0.006%
81	10.751	2913	2927	2940	rVV	138893	224279	47.99%	6.448%
82	10.835	2949	2953	2956	rVB2	327	213	0.05%	0.006%
83	10.854	2956	2959	2960	rBV	135	75	0.02%	0.002%
84	10.902	2972	2974	2977	rVB2	236	122	0.03%	0.004%
85	10.922	2977	2980	2984	rBV	133	135	0.03%	0.004%
86	11.224	3070	3074	3077	rBV	217	239	0.05%	0.007%
87	11.738	3233	3234	3237	rBV	132	44	0.01%	0.001%
88	11.806	3244	3255	3272	rBV	210000	325413	69.63%	9.355%
89	11.899	3281	3284	3289	rBV2	346	338	0.07%	0.010%
90	12.189	3361	3374	3394	rBV	195376	310998	66.55%	8.941%
91	13.201	3687	3689	3691	rBV	173	54	0.01%	0.002%
92	13.291	3715	3717	3720	rVB	200	88	0.02%	0.003%
93	14.134	3977	3979	3982	rBV	209	137	0.03%	0.004%
94	14.221	4003	4006	4008	rBV	180	113	0.02%	0.003%
95	14.253	4015	4016	4018	rVB	291	81	0.02%	0.002%
96	14.269	4019	4021	4023	rBV	199	87	0.02%	0.003%
97	14.436	4070	4073	4079	rBV2	206	161	0.03%	0.005%
98	14.976	4239	4241	4243	rBV	325	153	0.03%	0.004%
99	15.012	4249	4252	4254	rBV	256	141	0.03%	0.004%
100	15.639	4443	4447	4449	rBV	267	218	0.05%	0.006%




Sum of corrected areas: 3478507

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053324.D
Acq On : 21 Mar 2023 15:13
Operator : JC/MD
Sample : 01961-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

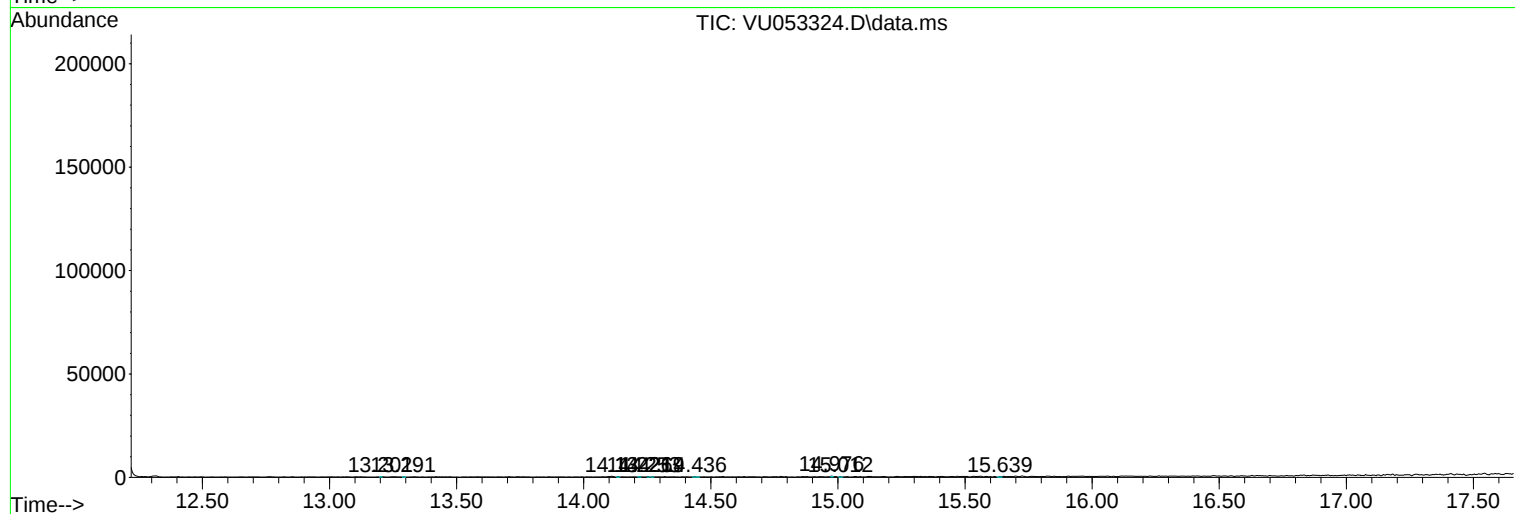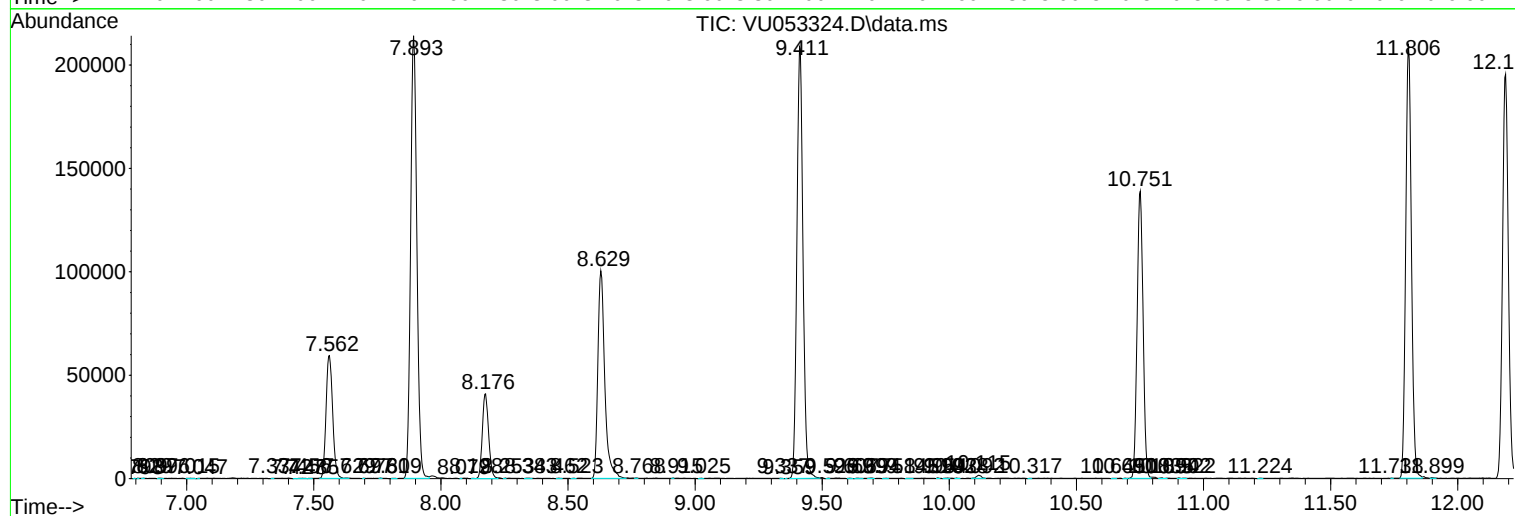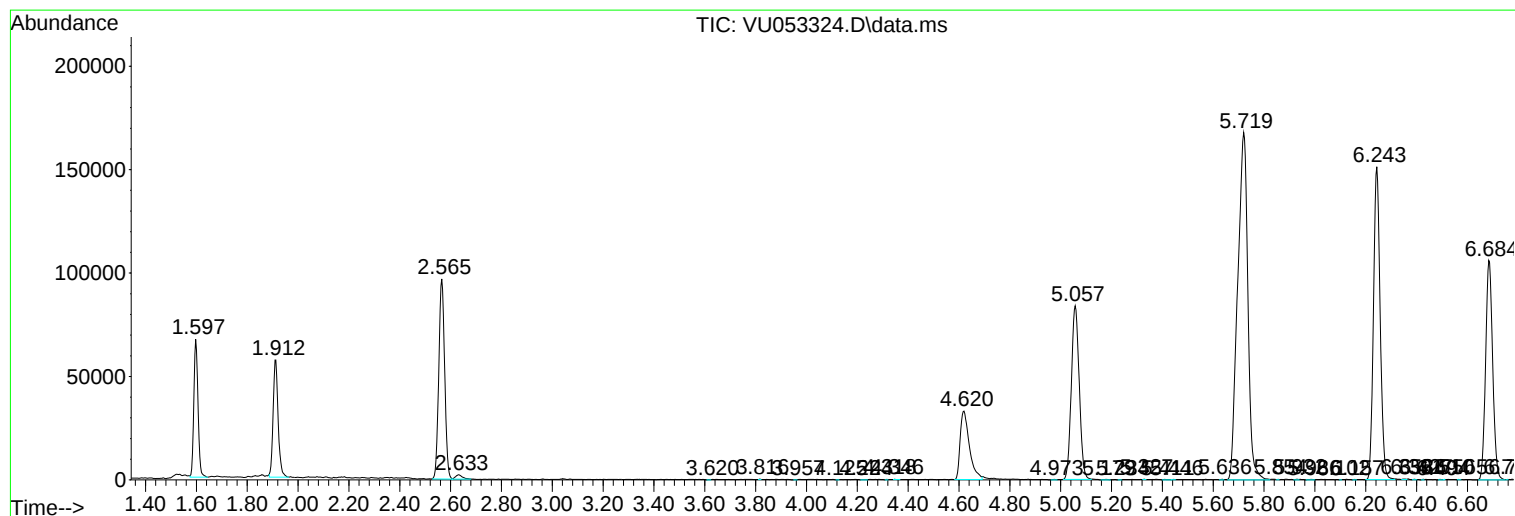

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053324.D
Acq On : 21 Mar 2023 15:13
Operator : JC/MD
Sample : 01961-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053324.D
Acq On : 21 Mar 2023 15:13
Operator : JC/MD
Sample : 01961-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------