

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053325.D
 Acq On : 21 Mar 2023 15:36
 Operator : JC/MD
 Sample : 01961-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rVB	65012	72533	16.01%	2.170%
2	1.913	170	178	192	rVB	53598	70780	15.62%	2.118%
3	2.565	370	381	399	rVB	94359	150063	33.12%	4.490%
4	2.974	505	508	510	rBV	188	96	0.02%	0.003%
5	3.366	627	630	637	rBV	192	200	0.04%	0.006%
6	3.482	663	666	668	rBV	180	140	0.03%	0.004%
7	3.501	669	672	674	rVV2	191	139	0.03%	0.004%
8	4.035	835	838	840	rBV	140	86	0.02%	0.003%
9	4.208	888	892	893	rBV	145	98	0.02%	0.003%
10	4.256	902	907	912	rBV	198	311	0.07%	0.009%
11	4.392	945	949	951	rBV2	268	232	0.05%	0.007%
12	4.620	1007	1020	1053	rBV	31762	79644	17.58%	2.383%
13	4.893	1101	1105	1108	rVB	253	174	0.04%	0.005%
14	5.057	1140	1156	1175	rBV	80871	179494	39.62%	5.371%
15	5.163	1186	1189	1193	rVB	194	150	0.03%	0.004%
16	5.224	1203	1208	1213	rBV	393	376	0.08%	0.011%
17	5.292	1226	1229	1232	rBV	215	193	0.04%	0.006%
18	5.334	1239	1242	1244	rBV	153	77	0.02%	0.002%
19	5.478	1283	1287	1289	rBB	135	95	0.02%	0.003%
20	5.494	1290	1292	1294	rBV	161	110	0.02%	0.003%
21	5.559	1310	1312	1313	rBV	254	131	0.03%	0.004%
22	5.600	1323	1325	1326	rBV	113	43	0.01%	0.001%
23	5.636	1331	1336	1338	rBB	174	169	0.04%	0.005%
24	5.649	1339	1340	1342	rBB	128	48	0.01%	0.001%
25	5.719	1342	1362	1389	rBV2	164278	453054	100.00%	13.556%
26	5.922	1422	1425	1426	rBV	135	94	0.02%	0.003%
27	6.089	1475	1477	1479	rBB	147	79	0.02%	0.002%
28	6.115	1482	1485	1487	rBB	145	98	0.02%	0.003%
29	6.134	1488	1491	1492	rBV	130	96	0.02%	0.003%
30	6.182	1504	1506	1509	rBV	148	123	0.03%	0.004%
31	6.244	1512	1525	1549	rVV	140088	261093	57.63%	7.812%
32	6.408	1573	1576	1578	rBV	225	153	0.03%	0.005%
33	6.488	1594	1601	1604	rBB	206	265	0.06%	0.008%
34	6.514	1605	1609	1617	rBV	213	361	0.08%	0.011%
35	6.629	1642	1645	1648	rBV	173	172	0.04%	0.005%
36	6.684	1648	1662	1683	rVB	103809	201179	44.41%	6.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053325.D
 Acq On : 21 Mar 2023 15:36
 Operator : JC/MD
 Sample : 01961-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.806	1697	1700	1702	rVB	253	142	0.03%	0.004%
38	6.822	1702	1705	1710	rBV	212	245	0.05%	0.007%
39	6.903	1726	1730	1732	rBB	180	143	0.03%	0.004%
40	6.919	1733	1735	1737	rBV	157	102	0.02%	0.003%
41	6.973	1748	1752	1757	rBV	179	257	0.06%	0.008%
42	7.080	1780	1785	1789	rBV	254	311	0.07%	0.009%
43	7.176	1812	1815	1819	rBV2	387	364	0.08%	0.011%
44	7.369	1871	1875	1877	rBV	205	184	0.04%	0.006%
45	7.488	1906	1912	1917	rBV	225	335	0.07%	0.010%
46	7.510	1917	1919	1922	rVB	266	155	0.03%	0.005%
47	7.562	1923	1935	1954	rBV	61644	106191	23.44%	3.177%
48	7.668	1966	1968	1972	rBV	196	105	0.02%	0.003%
49	7.716	1980	1983	1985	rBB	229	127	0.03%	0.004%
50	7.735	1985	1989	1994	rBB	191	236	0.05%	0.007%
51	7.758	1994	1996	1997	rBV	128	68	0.02%	0.002%
52	7.893	2025	2038	2060	rBV	207710	357153	78.83%	10.686%
53	8.018	2075	2077	2083	rVB2	299	325	0.07%	0.010%
54	8.063	2083	2091	2096	rBV2	265	436	0.10%	0.013%
55	8.089	2097	2099	2104	rVV2	160	106	0.02%	0.003%
56	8.173	2116	2125	2144	rBV	41060	68492	15.12%	2.049%
57	8.369	2182	2186	2188	rBV	216	196	0.04%	0.006%
58	8.539	2235	2239	2242	rBV	181	180	0.04%	0.005%
59	8.629	2256	2267	2296	rBV3	93652	182958	40.38%	5.474%
60	8.822	2324	2327	2329	rBV	173	94	0.02%	0.003%
61	9.047	2395	2397	2401	rBV	227	104	0.02%	0.003%
62	9.182	2436	2439	2445	rBV	302	341	0.08%	0.010%
63	9.288	2469	2472	2474	rBV	217	181	0.04%	0.005%
64	9.343	2487	2489	2491	rBV	133	90	0.02%	0.003%
65	9.411	2499	2510	2529	rBV	190131	319711	70.57%	9.566%
66	9.655	2584	2586	2588	rBB	113	42	0.01%	0.001%
67	9.684	2588	2595	2600	rBV	234	415	0.09%	0.012%
68	9.768	2617	2621	2623	rBV	160	161	0.04%	0.005%
69	9.819	2635	2637	2641	rVB	354	222	0.05%	0.007%
70	9.841	2641	2644	2646	rBV	141	117	0.03%	0.004%
71	9.899	2660	2662	2664	rBV	155	71	0.02%	0.002%
72	9.951	2676	2678	2680	rBV	158	97	0.02%	0.003%
73	10.076	2714	2717	2720	rBV	155	128	0.03%	0.004%
74	10.118	2722	2730	2737	rVB4	1550	2052	0.45%	0.061%
75	10.259	2772	2774	2777	rVB	266	111	0.02%	0.003%
76	10.414	2819	2822	2825	rBV	201	192	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053325.D
 Acq On : 21 Mar 2023 15:36
 Operator : JC/MD
 Sample : 01961-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.465	2832	2838	2844	rBV	189	386	0.09%	0.012%
78	10.562	2863	2868	2869	rBV	164	147	0.03%	0.004%
79	10.665	2897	2900	2902	rBV	181	82	0.02%	0.002%
80	10.751	2915	2927	2945	rBV	137615	217797	48.07%	6.517%
81	11.250	3077	3082	3084	rBV	219	268	0.06%	0.008%
82	11.343	3108	3111	3113	rBV	232	188	0.04%	0.006%
83	11.423	3131	3136	3139	rBV	314	310	0.07%	0.009%
84	11.517	3163	3165	3168	rBV	133	84	0.02%	0.003%
85	11.806	3244	3255	3278	rBV	194983	306316	67.61%	9.165%
86	12.189	3362	3374	3391	rBV	186442	299489	66.10%	8.961%
87	12.314	3407	3413	3419	rVB2	654	848	0.19%	0.025%
88	12.449	3453	3455	3458	rBV	176	62	0.01%	0.002%
89	12.536	3480	3482	3484	rVB	234	96	0.02%	0.003%
90	12.774	3553	3556	3558	rBV	189	120	0.03%	0.004%
91	12.989	3619	3623	3627	rBV	206	184	0.04%	0.006%
92	14.703	4152	4156	4160	rBV	185	216	0.05%	0.006%
93	14.915	4220	4222	4225	rVB	230	110	0.02%	0.003%
94	14.938	4226	4229	4231	rBV2	227	152	0.03%	0.005%
95	15.037	4257	4260	4263	rBV2	252	164	0.04%	0.005%


Sum of corrected areas: 3342108

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053325.D
Acq On : 21 Mar 2023 15:36
Operator : JC/MD
Sample : 01961-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

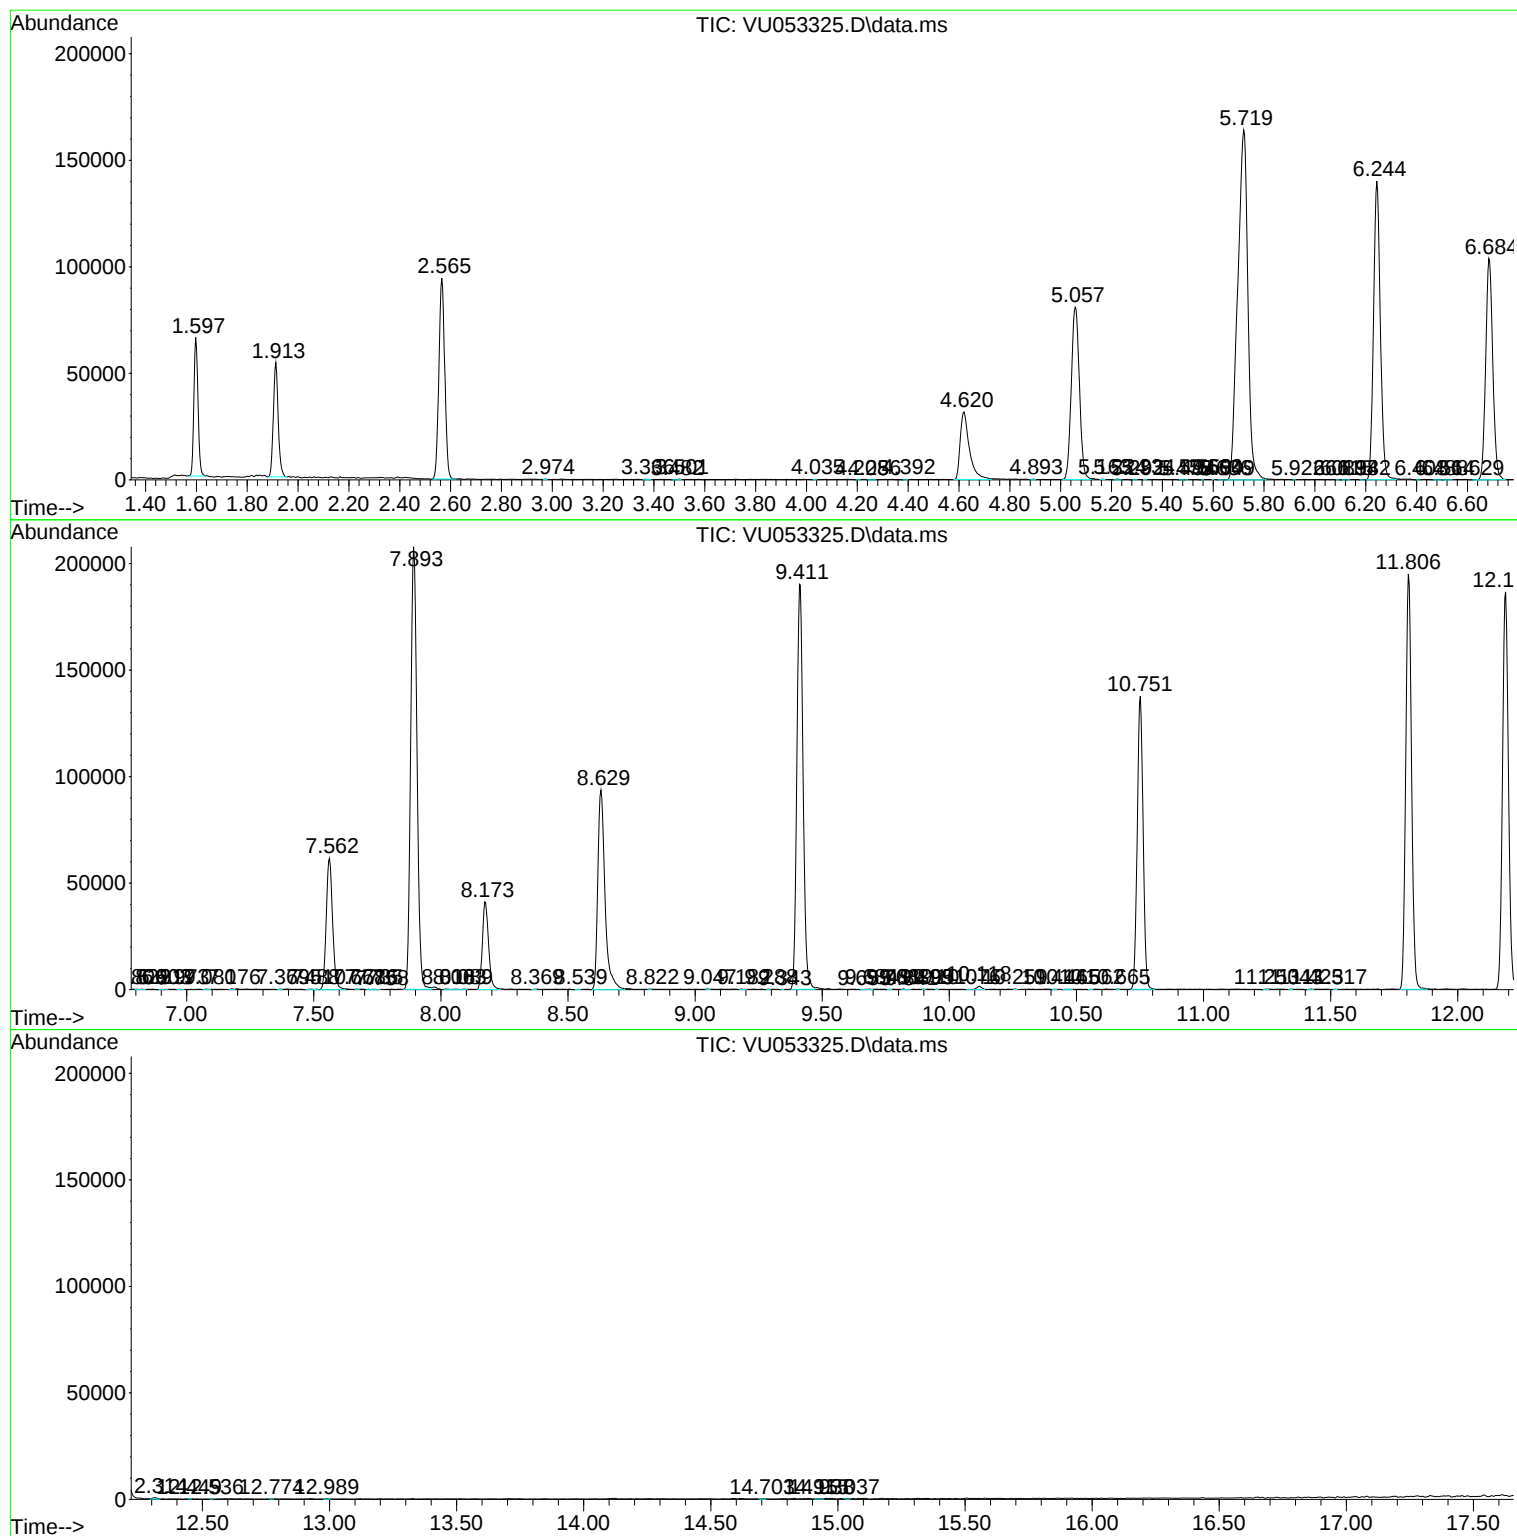

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053325.D
Acq On : 21 Mar 2023 15:36
Operator : JC/MD
Sample : 01961-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053325.D
Acq On : 21 Mar 2023 15:36
Operator : JC/MD
Sample : 01961-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------