

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053326.D
 Acq On : 21 Mar 2023 15:59
 Operator : JC/MD
 Sample : 01980-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	65267	72001	15.96%	2.104%
2	1.909	170	177	193	rVB	56213	76867	17.04%	2.247%
3	2.565	369	381	396	rVB	95799	152361	33.77%	4.453%
4	3.044	522	530	538	rBV3	1865	3026	0.67%	0.088%
5	3.723	739	741	744	rVB	180	75	0.02%	0.002%
6	3.838	773	777	782	rBV	266	328	0.07%	0.010%
7	4.510	984	986	989	rVB	170	73	0.02%	0.002%
8	4.620	1009	1020	1044	rBV	35607	87831	19.47%	2.567%
9	4.829	1081	1085	1089	rVB2	208	232	0.05%	0.007%
10	5.057	1140	1156	1177	rBV	81327	177970	39.45%	5.202%
11	5.157	1185	1187	1189	rBV	160	94	0.02%	0.003%
12	5.285	1222	1227	1231	rBV	187	245	0.05%	0.007%
13	5.353	1245	1248	1250	rBV	220	165	0.04%	0.005%
14	5.536	1300	1305	1308	rBV	249	254	0.06%	0.007%
15	5.552	1308	1310	1316	rVB	287	251	0.06%	0.007%
16	5.581	1316	1319	1321	rBV	152	130	0.03%	0.004%
17	5.719	1341	1362	1394	rBV2	164513	451157	100.00%	13.187%
18	5.899	1415	1418	1420	rBV	221	182	0.04%	0.005%
19	6.121	1481	1487	1490	rBV	254	298	0.07%	0.009%
20	6.179	1502	1505	1508	rVB	209	104	0.02%	0.003%
21	6.243	1512	1525	1545	rBV	145849	274993	60.95%	8.038%
22	6.375	1564	1566	1570	rVB	163	59	0.01%	0.002%
23	6.481	1596	1599	1601	rBB	178	115	0.03%	0.003%
24	6.520	1606	1611	1613	rBV	306	269	0.06%	0.008%
25	6.533	1613	1615	1618	rVB	206	98	0.02%	0.003%
26	6.565	1623	1625	1631	rVB	160	95	0.02%	0.003%
27	6.684	1649	1662	1680	rBV	105784	202470	44.88%	5.918%
28	6.809	1695	1701	1703	rBV	316	292	0.06%	0.009%
29	6.890	1721	1726	1728	rBV	175	209	0.05%	0.006%
30	6.948	1739	1744	1748	rBB	162	178	0.04%	0.005%
31	6.970	1749	1751	1753	rBB	109	41	0.01%	0.001%
32	6.989	1754	1757	1759	rBV	195	161	0.04%	0.005%
33	7.115	1793	1796	1801	rBV	209	279	0.06%	0.008%
34	7.179	1814	1816	1819	rVB	324	135	0.03%	0.004%
35	7.218	1826	1828	1831	rBV	187	79	0.02%	0.002%
36	7.266	1840	1843	1845	rBV	174	143	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053326.D
 Acq On : 21 Mar 2023 15:59
 Operator : JC/MD
 Sample : 01980-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.497	1914	1915	1917	rBB	112	42	0.01%	0.001%
38	7.517	1917	1921	1923	rBV	180	171	0.04%	0.005%
39	7.562	1923	1935	1949	rBV	58529	102296	22.67%	2.990%
40	7.649	1960	1962	1965	rVB	343	207	0.05%	0.006%
41	7.681	1966	1972	1975	rBV	282	321	0.07%	0.009%
42	7.809	2009	2012	2013	rBV	157	108	0.02%	0.003%
43	7.893	2025	2038	2056	rBV	207180	358368	79.43%	10.475%
44	8.083	2095	2097	2098	rBV	163	50	0.01%	0.001%
45	8.118	2105	2108	2111	rBV	137	118	0.03%	0.003%
46	8.131	2111	2112	2115	rVV	197	98	0.02%	0.003%
47	8.176	2115	2126	2142	rVV	40794	67529	14.97%	1.974%
48	8.327	2171	2173	2175	rBB	126	68	0.02%	0.002%
49	8.343	2176	2178	2180	rBV	167	117	0.03%	0.003%
50	8.465	2213	2216	2219	rBV	150	153	0.03%	0.004%
51	8.523	2232	2234	2235	rBV	135	75	0.02%	0.002%
52	8.555	2239	2244	2247	rBV	321	325	0.07%	0.009%
53	8.629	2255	2267	2296	rBV3	100979	191653	42.48%	5.602%
54	8.758	2305	2307	2310	rBV	253	146	0.03%	0.004%
55	9.034	2391	2393	2395	rBV	167	91	0.02%	0.003%
56	9.057	2398	2400	2402	rBV	152	107	0.02%	0.003%
57	9.308	2473	2478	2484	rBV	218	373	0.08%	0.011%
58	9.333	2484	2486	2487	rVV	140	38	0.01%	0.001%
59	9.410	2499	2510	2529	rBV	202385	337946	74.91%	9.878%
60	9.510	2539	2541	2547	rVB2	272	192	0.04%	0.006%
61	9.549	2552	2553	2554	rBV2	122	29	0.01%	0.001%
62	9.597	2566	2568	2570	rVB	168	66	0.01%	0.002%
63	9.652	2583	2585	2588	rBV	163	128	0.03%	0.004%
64	9.944	2673	2676	2679	rBV	150	120	0.03%	0.004%
65	9.983	2685	2688	2690	rBB	127	91	0.02%	0.003%
66	9.999	2691	2693	2696	rBV	185	144	0.03%	0.004%
67	10.111	2723	2728	2740	rVB4	1482	2161	0.48%	0.063%
68	10.205	2753	2757	2762	rBV	277	353	0.08%	0.010%
69	10.259	2769	2774	2775	rBV	172	143	0.03%	0.004%
70	10.462	2834	2837	2844	rBV	304	310	0.07%	0.009%
71	10.751	2915	2927	2943	rBV2	140482	221448	49.08%	6.473%
72	10.828	2946	2951	2953	rBV2	285	208	0.05%	0.006%
73	10.890	2967	2970	2973	rBV	219	190	0.04%	0.006%
74	11.494	3155	3158	3160	rBV	162	137	0.03%	0.004%
75	11.545	3172	3174	3177	rBV	160	88	0.02%	0.003%
76	11.806	3243	3255	3276	rBV	206629	326913	72.46%	9.555%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053326.D
Acq On : 21 Mar 2023 15:59
Operator : JC/MD
Sample : 01980-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

77	11.954	3299	3301	3302	rBV	135	38	0.01%	0.001%
78	12.189	3362	3374	3397	rBV	188285	303570	67.29%	8.873%
79	12.298	3404	3408	3410	rBV3	689	499	0.11%	0.015%
80	12.446	3452	3454	3456	rBV	206	120	0.03%	0.004%
81	12.841	3573	3577	3579	rBV	217	199	0.04%	0.006%
82	14.105	3967	3970	3972	rBV	276	196	0.04%	0.006%
83	14.815	4189	4191	4195	rBV	166	130	0.03%	0.004%
84	15.201	4307	4311	4314	rBV	247	201	0.04%	0.006%




Sum of corrected areas: 3421334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053326.D
Acq On : 21 Mar 2023 15:59
Operator : JC/MD
Sample : 01980-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

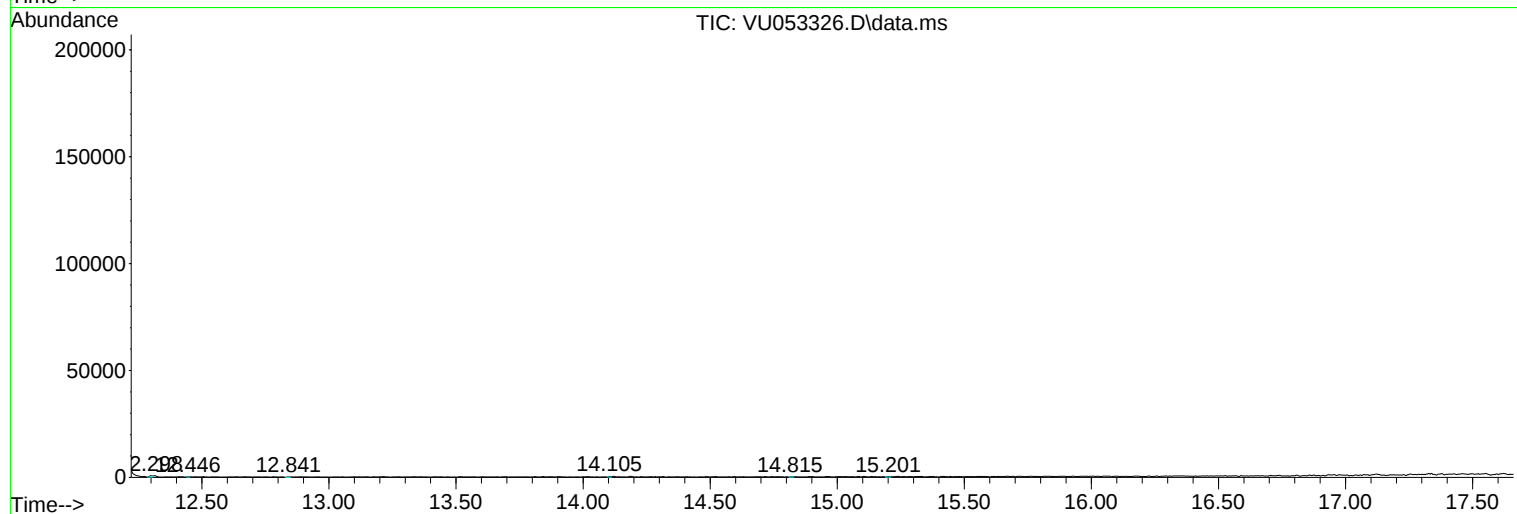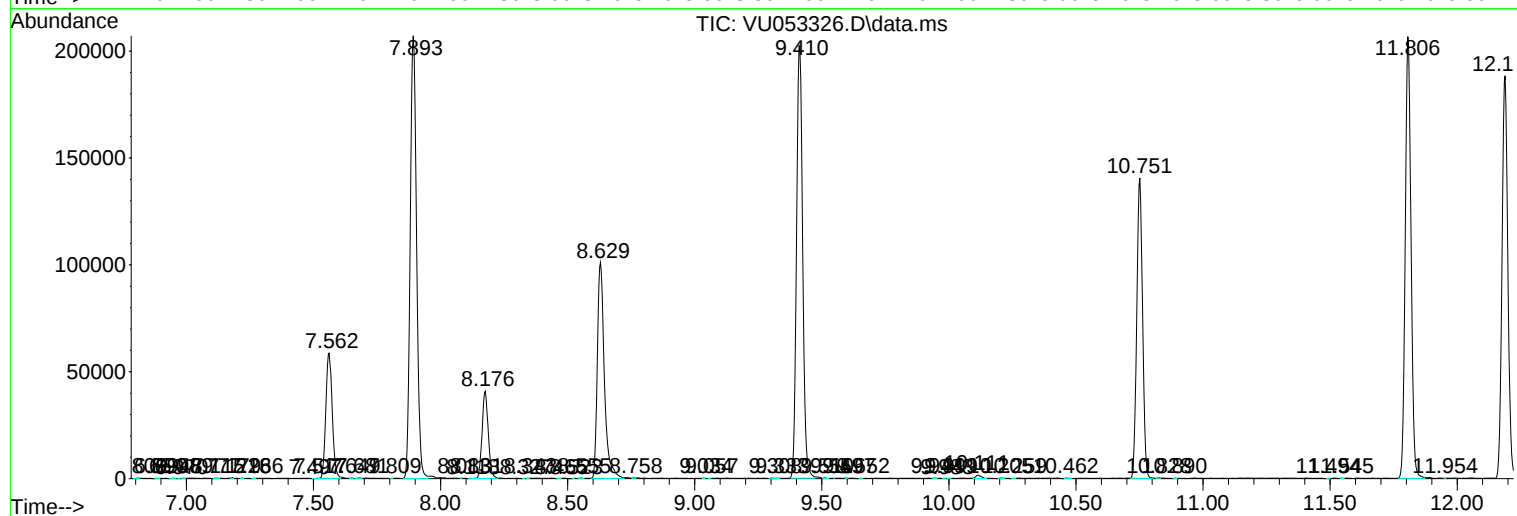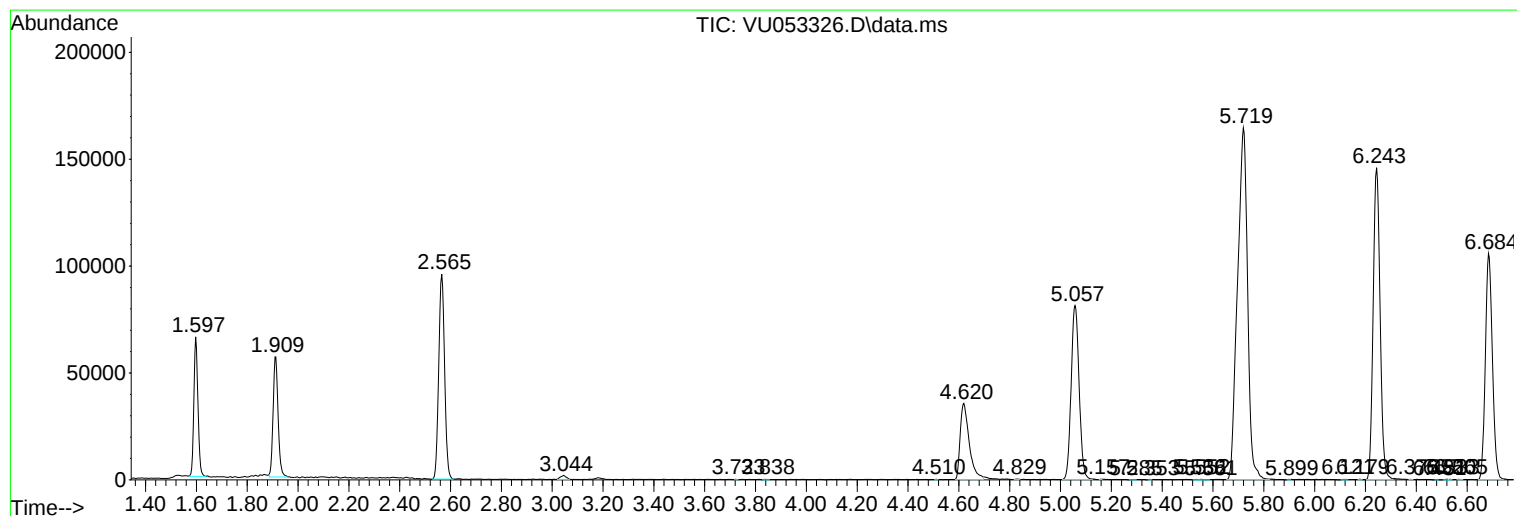

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053326.D
Acq On : 21 Mar 2023 15:59
Operator : JC/MD
Sample : 01980-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053326.D
Acq On : 21 Mar 2023 15:59
Operator : JC/MD
Sample : 01980-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------