

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053328.D
 Acq On : 21 Mar 2023 16:45
 Operator : JC/MD
 Sample : 01956-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	61303	68999	15.60%	2.070%
2	1.912	170	178	194	rVB	55580	75618	17.10%	2.269%
3	2.565	370	381	394	rVB	90437	144126	32.59%	4.324%
4	2.838	464	466	467	rBV	176	57	0.01%	0.002%
5	3.041	522	529	540	rVB3	1588	2754	0.62%	0.083%
6	3.173	564	570	572	rBV2	987	1038	0.23%	0.031%
7	3.459	656	659	660	rBV	163	92	0.02%	0.003%
8	3.671	721	725	728	rVB	198	130	0.03%	0.004%
9	3.842	776	778	781	rVB	134	54	0.01%	0.002%
10	3.951	809	812	813	rBV	259	157	0.04%	0.005%
11	4.012	827	831	834	rBV	200	218	0.05%	0.007%
12	4.182	880	884	887	rBV	227	233	0.05%	0.007%
13	4.279	911	914	917	rBV	142	144	0.03%	0.004%
14	4.343	931	934	936	rBV	190	163	0.04%	0.005%
15	4.436	961	963	966	rVB	153	47	0.01%	0.001%
16	4.520	985	989	992	rBB	181	164	0.04%	0.005%
17	4.539	992	995	999	rBB	161	157	0.04%	0.005%
18	4.571	999	1005	1009	rBV	258	376	0.09%	0.011%
19	4.620	1009	1020	1054	rBV	33754	89677	20.28%	2.691%
20	4.912	1109	1111	1114	rVB2	203	113	0.03%	0.003%
21	4.957	1121	1125	1128	rBV	240	255	0.06%	0.008%
22	5.057	1140	1156	1180	rBV2	80692	175331	39.64%	5.260%
23	5.147	1180	1184	1187	rVB2	343	302	0.07%	0.009%
24	5.166	1188	1190	1191	rBV	123	69	0.02%	0.002%
25	5.243	1211	1214	1216	rBV	173	140	0.03%	0.004%
26	5.324	1236	1239	1240	rBV	177	125	0.03%	0.004%
27	5.366	1249	1252	1254	rBV	179	149	0.03%	0.004%
28	5.378	1254	1256	1258	rVB	141	55	0.01%	0.002%
29	5.510	1295	1297	1299	rBV	132	97	0.02%	0.003%
30	5.636	1334	1336	1337	rBV	143	78	0.02%	0.002%
31	5.719	1342	1362	1393	rBV2	159175	442258	100.00%	13.269%
32	5.915	1420	1423	1425	rBV	158	132	0.03%	0.004%
33	5.948	1430	1433	1435	rBV	214	168	0.04%	0.005%
34	6.057	1464	1467	1468	rBV	157	108	0.02%	0.003%
35	6.150	1494	1496	1500	rBV	156	158	0.04%	0.005%
36	6.243	1511	1525	1543	rBV	138969	261526	59.13%	7.846%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053328.D
 Acq On : 21 Mar 2023 16:45
 Operator : JC/MD
 Sample : 01956-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.446	1585	1588	1590	rBV	141	93	0.02%	0.003%
38	6.459	1590	1592	1595	rVV	150	95	0.02%	0.003%
39	6.497	1603	1604	1606	rBB	102	39	0.01%	0.001%
40	6.517	1606	1610	1611	rBV	295	238	0.05%	0.007%
41	6.575	1626	1628	1631	rBV	162	88	0.02%	0.003%
42	6.687	1648	1663	1682	rBV	100842	197129	44.57%	5.914%
43	6.758	1682	1685	1691	rVB	430	430	0.10%	0.013%
44	6.796	1695	1697	1700	rBV	213	170	0.04%	0.005%
45	6.832	1705	1708	1710	rBV	201	167	0.04%	0.005%
46	6.877	1721	1722	1723	rBV	127	34	0.01%	0.001%
47	6.954	1741	1746	1748	rBV	154	183	0.04%	0.005%
48	6.999	1755	1760	1764	rBV	193	277	0.06%	0.008%
49	7.018	1764	1766	1768	rVB	285	130	0.03%	0.004%
50	7.041	1769	1773	1778	rBV	338	277	0.06%	0.008%
51	7.198	1819	1822	1825	rBV	316	243	0.05%	0.007%
52	7.314	1854	1858	1861	rBV	226	217	0.05%	0.007%
53	7.449	1892	1900	1904	rBV	242	367	0.08%	0.011%
54	7.513	1917	1920	1923	rBB	180	152	0.03%	0.005%
55	7.562	1923	1935	1953	rBV2	58186	101013	22.84%	3.031%
56	7.671	1966	1969	1971	rBV	207	170	0.04%	0.005%
57	7.774	1998	2001	2003	rBV2	217	113	0.03%	0.003%
58	7.838	2018	2021	2025	rBB	260	232	0.05%	0.007%
59	7.893	2025	2038	2057	rBV	202378	347277	78.52%	10.419%
60	8.124	2106	2110	2112	rBV	145	124	0.03%	0.004%
61	8.176	2114	2126	2141	rVV3	39723	66839	15.11%	2.005%
62	8.275	2154	2157	2159	rBV	186	156	0.04%	0.005%
63	8.481	2218	2221	2224	rBB	225	165	0.04%	0.005%
64	8.510	2227	2230	2233	rBV	140	140	0.03%	0.004%
65	8.533	2234	2237	2239	rVB	292	182	0.04%	0.005%
66	8.552	2240	2243	2245	rBV	166	133	0.03%	0.004%
67	8.629	2257	2267	2295	rBV2	100509	190812	43.14%	5.725%
68	8.764	2305	2309	2312	rVB	178	141	0.03%	0.004%
69	8.870	2340	2342	2347	rVB	234	97	0.02%	0.003%
70	8.915	2351	2356	2358	rBB	149	125	0.03%	0.004%
71	8.928	2358	2360	2363	rBV	154	132	0.03%	0.004%
72	9.111	2416	2417	2419	rBV	109	62	0.01%	0.002%
73	9.414	2498	2511	2529	rBV	201162	330974	74.84%	9.930%
74	9.709	2599	2603	2606	rBV	163	152	0.03%	0.005%
75	9.851	2644	2647	2651	rVB	169	87	0.02%	0.003%
76	9.928	2666	2671	2676	rBV	224	308	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053328.D
 Acq On : 21 Mar 2023 16:45
 Operator : JC/MD
 Sample : 01956-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.079	2716	2718	2722	rVB	175	66	0.01%	0.002%
78	10.111	2722	2728	2741	rVB3	1270	2062	0.47%	0.062%
79	10.169	2742	2746	2753	rBV	238	417	0.09%	0.013%
80	10.285	2781	2782	2783	rBV	125	34	0.01%	0.001%
81	10.381	2809	2812	2815	rVB	226	126	0.03%	0.004%
82	10.751	2915	2927	2942	rBV2	140039	222234	50.25%	6.668%
83	10.989	2998	3001	3003	rBV	188	156	0.04%	0.005%
84	11.156	3051	3053	3055	rBV	158	107	0.02%	0.003%
85	11.362	3115	3117	3121	rVB	179	71	0.02%	0.002%
86	11.594	3187	3189	3191	rBV	166	52	0.01%	0.002%
87	11.616	3192	3196	3198	rBV	251	194	0.04%	0.006%
88	11.806	3243	3255	3273	rBV	194993	310191	70.14%	9.307%
89	11.954	3299	3301	3304	rVB	210	91	0.02%	0.003%
90	12.131	3354	3356	3358	rVB	150	57	0.01%	0.002%
91	12.188	3362	3374	3389	rBV	181832	290186	65.61%	8.706%
92	12.262	3394	3397	3402	rVB3	321	212	0.05%	0.006%
93	12.311	3408	3412	3419	rBV	591	671	0.15%	0.020%
94	12.462	3454	3459	3461	rBV	248	261	0.06%	0.008%
95	14.130	3975	3978	3984	rBV	247	204	0.05%	0.006%
96	14.185	3992	3995	3997	rBV	184	119	0.03%	0.004%
97	14.503	4092	4094	4096	rBV	151	68	0.02%	0.002%
98	14.790	4181	4183	4187	rBV2	243	144	0.03%	0.004%
99	14.822	4191	4193	4194	rBV2	173	56	0.01%	0.002%
100	15.166	4297	4300	4303	rVB2	380	246	0.06%	0.007%




Sum of corrected areas: 3333056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053328.D
Acq On : 21 Mar 2023 16:45
Operator : JC/MD
Sample : 01956-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

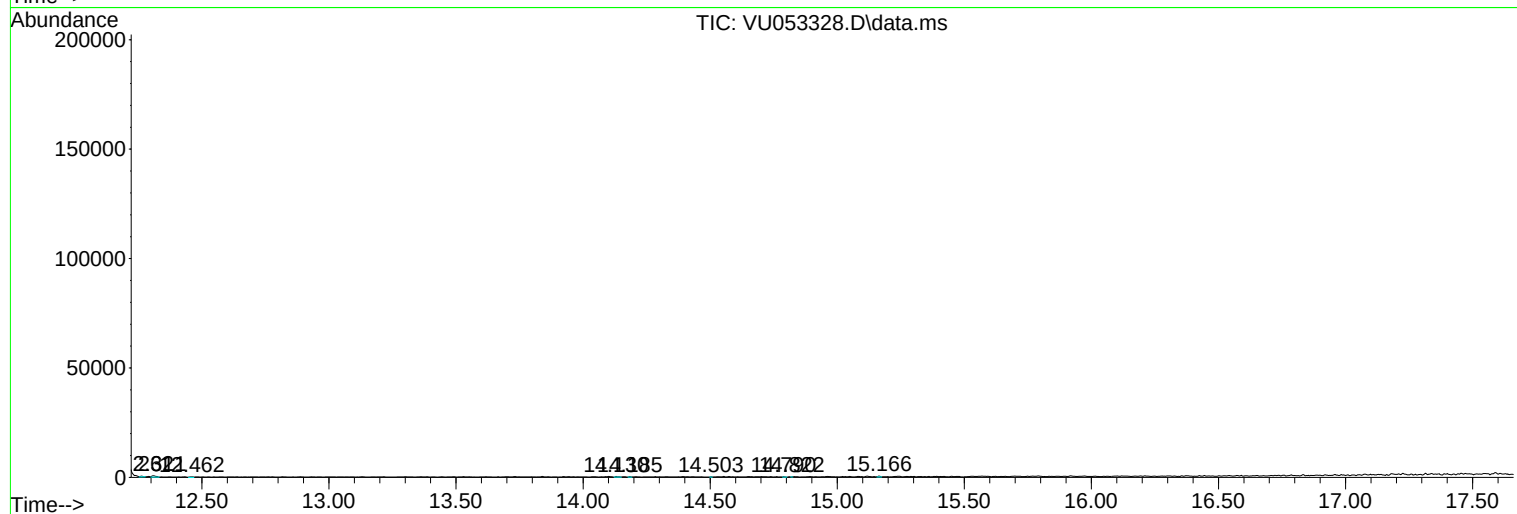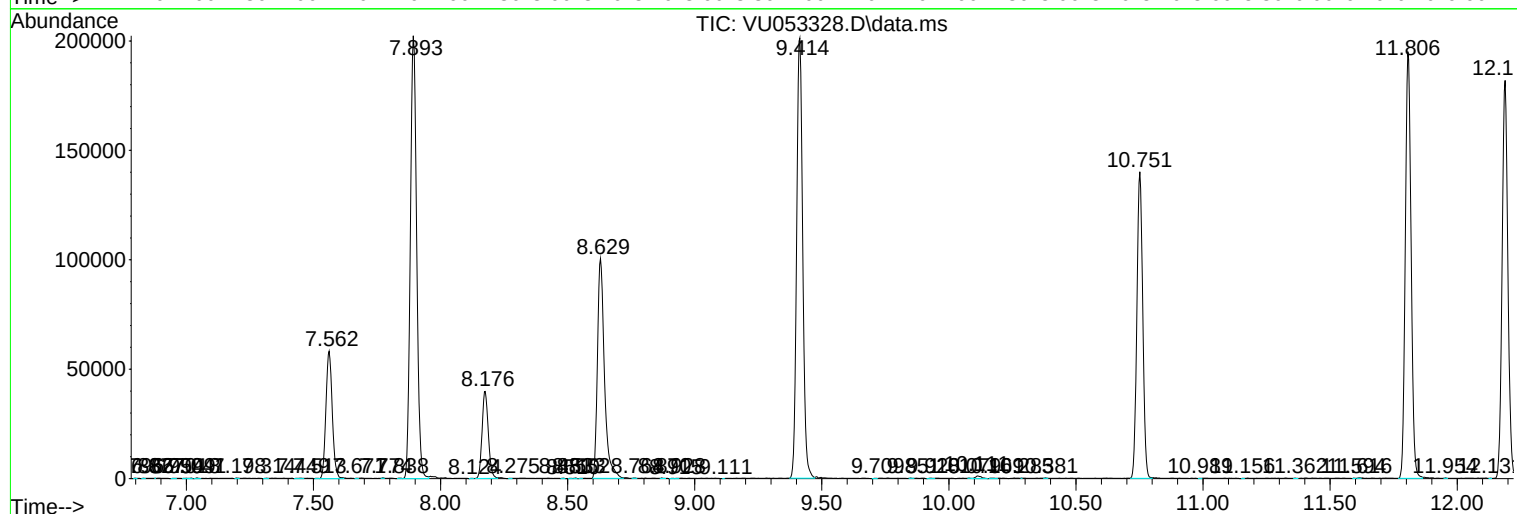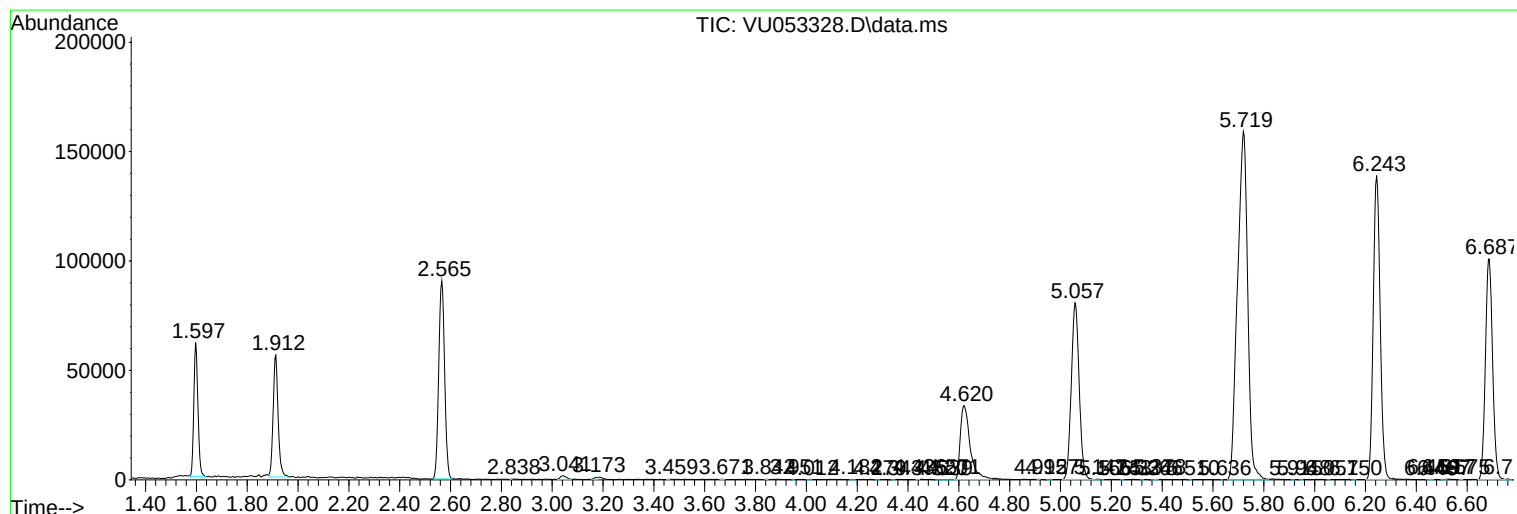

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053328.D
Acq On : 21 Mar 2023 16:45
Operator : JC/MD
Sample : 01956-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053328.D
Acq On : 21 Mar 2023 16:45
Operator : JC/MD
Sample : 01956-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------