

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053330.D
 Acq On : 21 Mar 2023 17:32
 Operator : JC/MD
 Sample : 01961-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	64271	73025	16.45%	2.174%
2	1.912	170	178	196	rVB	49655	67434	15.19%	2.008%
3	2.565	370	381	396	rBV	93775	149486	33.67%	4.451%
4	3.044	523	530	537	rBV3	547	786	0.18%	0.023%
5	3.076	538	540	541	rBV3	130	35	0.01%	0.001%
6	4.099	856	858	861	rBV	153	124	0.03%	0.004%
7	4.179	879	883	885	rBB	151	104	0.02%	0.003%
8	4.202	886	890	894	rBB	268	254	0.06%	0.008%
9	4.234	895	900	903	rBV	228	294	0.07%	0.009%
10	4.327	926	929	931	rBV	177	146	0.03%	0.004%
11	4.620	1009	1020	1052	rBV	31084	80242	18.07%	2.389%
12	4.867	1095	1097	1099	rBV	218	114	0.03%	0.003%
13	4.883	1099	1102	1103	rVV	153	95	0.02%	0.003%
14	5.057	1138	1156	1181	rBV2	80542	176104	39.66%	5.243%
15	5.266	1217	1221	1224	rBV	258	245	0.06%	0.007%
16	5.362	1247	1251	1254	rBV	173	213	0.05%	0.006%
17	5.555	1307	1311	1312	rBV	242	119	0.03%	0.004%
18	5.719	1341	1362	1393	rBV3	160107	444015	100.00%	13.220%
19	5.964	1433	1438	1440	rBV	212	244	0.05%	0.007%
20	6.054	1464	1466	1467	rBV	140	75	0.02%	0.002%
21	6.176	1500	1504	1508	rBV	188	235	0.05%	0.007%
22	6.243	1511	1525	1545	rVV	147936	275083	61.95%	8.190%
23	6.382	1565	1568	1573	rBV	270	253	0.06%	0.008%
24	6.459	1588	1592	1596	rBB	202	219	0.05%	0.007%
25	6.481	1597	1599	1600	rBV	110	60	0.01%	0.002%
26	6.613	1635	1640	1645	rBV	267	400	0.09%	0.012%
27	6.684	1649	1662	1686	rVB	101469	200065	45.06%	5.957%
28	6.780	1687	1692	1695	rBV	167	189	0.04%	0.006%
29	6.816	1702	1703	1704	rVB	112	22	0.00%	0.001%
30	6.893	1724	1727	1729	rBV	165	136	0.03%	0.004%
31	6.954	1744	1746	1747	rBV	128	71	0.02%	0.002%
32	6.983	1751	1755	1761	rBV	231	329	0.07%	0.010%
33	7.179	1812	1816	1819	rBV	398	337	0.08%	0.010%
34	7.314	1855	1858	1861	rBV	247	185	0.04%	0.006%
35	7.517	1918	1921	1922	rBV	114	84	0.02%	0.003%
36	7.559	1922	1934	1954	rVV2	56432	99923	22.50%	2.975%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053330.D
 Acq On : 21 Mar 2023 17:32
 Operator : JC/MD
 Sample : 01961-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.652	1960	1963	1964	rBV	286	169	0.04%	0.005%
38	7.710	1979	1981	1983	rBV	178	55	0.01%	0.002%
39	7.893	2025	2038	2055	rBV	205015	346450	78.03%	10.315%
40	8.047	2081	2086	2089	rBV2	284	288	0.06%	0.009%
41	8.063	2089	2091	2094	rVV	189	79	0.02%	0.002%
42	8.128	2107	2111	2113	rBV	216	224	0.05%	0.007%
43	8.173	2115	2125	2143	rVV	40200	67925	15.30%	2.022%
44	8.304	2162	2166	2168	rBV	212	197	0.04%	0.006%
45	8.337	2174	2176	2179	rVB	171	75	0.02%	0.002%
46	8.394	2190	2194	2196	rBV	181	145	0.03%	0.004%
47	8.565	2244	2247	2249	rBV	265	182	0.04%	0.005%
48	8.629	2255	2267	2294	rBV2	92116	176941	39.85%	5.268%
49	8.957	2367	2369	2370	rBV2	178	78	0.02%	0.002%
50	9.038	2391	2394	2395	rBV	215	143	0.03%	0.004%
51	9.214	2446	2449	2451	rBV	133	121	0.03%	0.004%
52	9.288	2469	2472	2475	rBV	256	233	0.05%	0.007%
53	9.359	2492	2494	2497	rBB	189	124	0.03%	0.004%
54	9.414	2498	2511	2533	rBV	206719	345015	77.70%	10.272%
55	9.542	2549	2551	2552	rBV	172	94	0.02%	0.003%
56	9.571	2558	2560	2562	rBV	178	80	0.02%	0.002%
57	9.700	2598	2600	2603	rVB2	380	212	0.05%	0.006%
58	9.722	2604	2607	2611	rBB	220	203	0.05%	0.006%
59	9.748	2612	2615	2616	rBV	134	97	0.02%	0.003%
60	9.809	2631	2634	2637	rBV	250	209	0.05%	0.006%
61	9.973	2683	2685	2686	rBV	147	80	0.02%	0.002%
62	10.115	2723	2729	2730	rBV3	938	865	0.19%	0.026%
63	10.176	2744	2748	2754	rVB2	211	155	0.03%	0.005%
64	10.372	2805	2809	2812	rBV	224	246	0.06%	0.007%
65	10.433	2824	2828	2833	rBV	209	278	0.06%	0.008%
66	10.571	2868	2871	2875	rBV	175	140	0.03%	0.004%
67	10.751	2913	2927	2947	rBV	138188	217973	49.09%	6.490%
68	10.825	2948	2950	2953	rBV	182	96	0.02%	0.003%
69	10.925	2972	2981	2985	rBV	252	467	0.11%	0.014%
70	11.806	3243	3255	3276	rBV	205742	327409	73.74%	9.748%
71	12.047	3325	3330	3332	rBV	256	282	0.06%	0.008%
72	12.144	3357	3360	3361	rBV	175	89	0.02%	0.003%
73	12.189	3362	3374	3389	rVV	182274	296983	66.89%	8.842%
74	12.308	3404	3411	3418	rBV3	629	947	0.21%	0.028%
75	12.722	3537	3540	3542	rBV	195	80	0.02%	0.002%
76	12.816	3563	3569	3571	rBV	199	276	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053330.D
 Acq On : 21 Mar 2023 17:32
 Operator : JC/MD
 Sample : 01961-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	12.957	3607	3613	3615	rBV	279	353	0.08%	0.011%
78	13.288	3714	3716	3722	rVB2	265	181	0.04%	0.005%
79	13.523	3786	3789	3797	rBV	227	253	0.06%	0.008%
80	13.680	3836	3838	3841	rBV2	190	121	0.03%	0.004%
81	14.587	4117	4120	4123	rBV	159	89	0.02%	0.003%
82	14.632	4131	4134	4137	rBV	257	145	0.03%	0.004%
83	14.857	4202	4204	4208	rBV2	205	135	0.03%	0.004%
84	14.880	4208	4211	4217	rVV2	234	226	0.05%	0.007%
85	15.095	4276	4278	4285	rBV2	219	252	0.06%	0.008%
86	15.684	4455	4461	4465	rBV	332	491	0.11%	0.015%




Sum of corrected areas: 3358696

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053330.D
Acq On : 21 Mar 2023 17:32
Operator : JC/MD
Sample : 01961-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

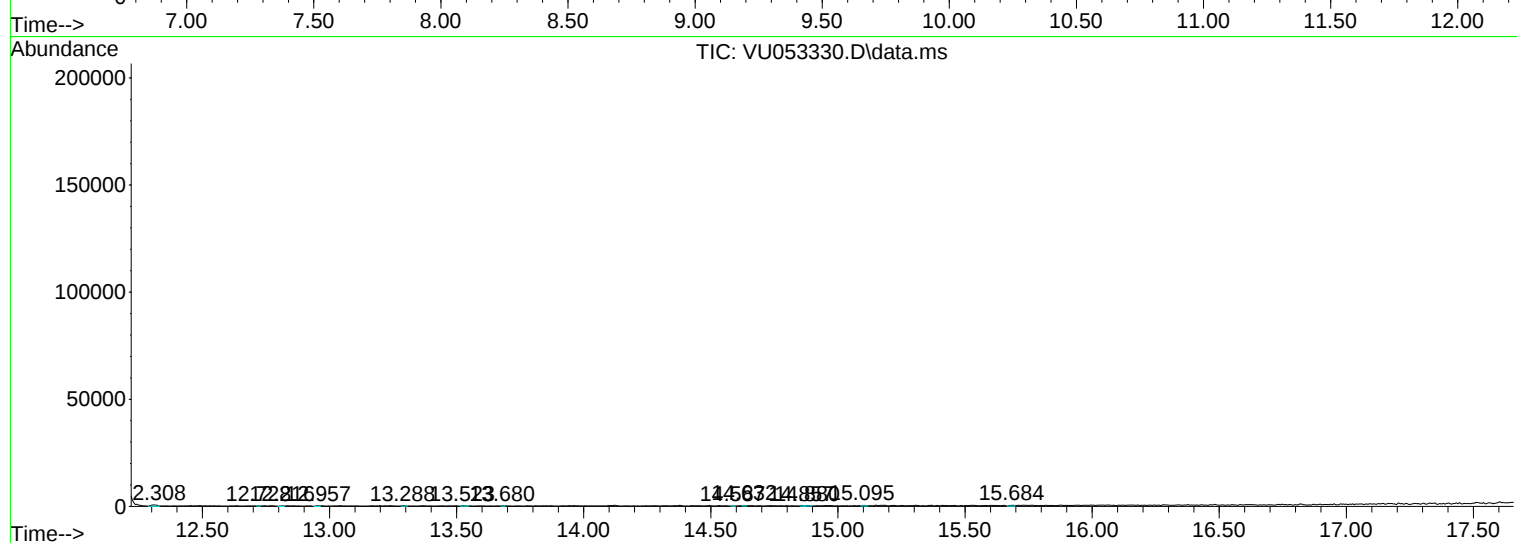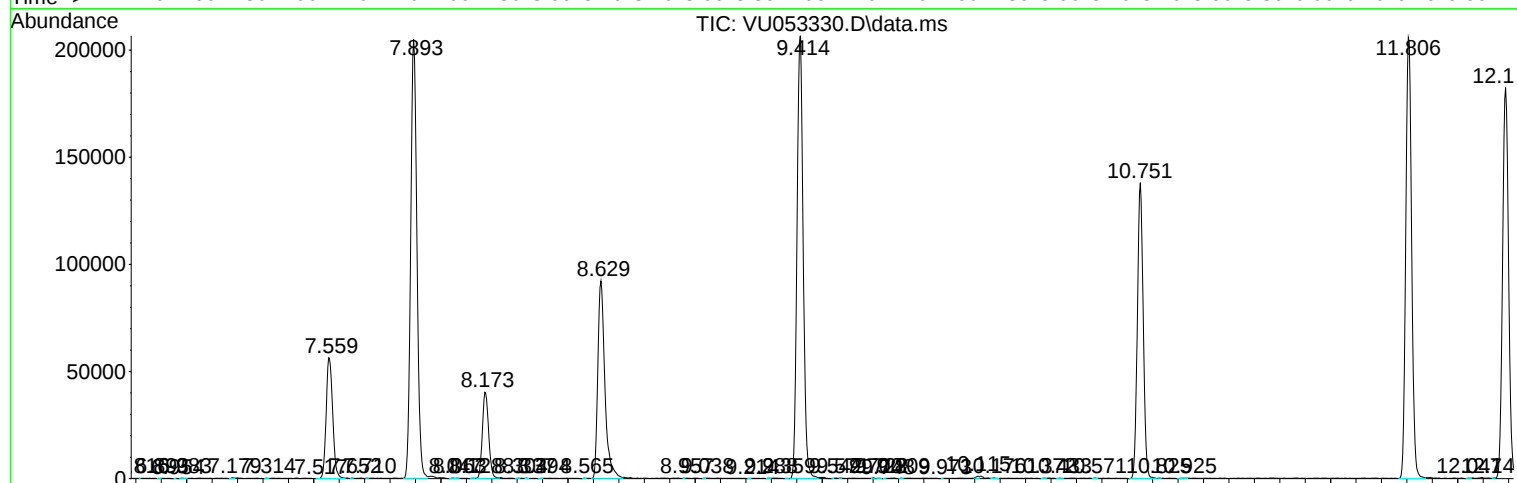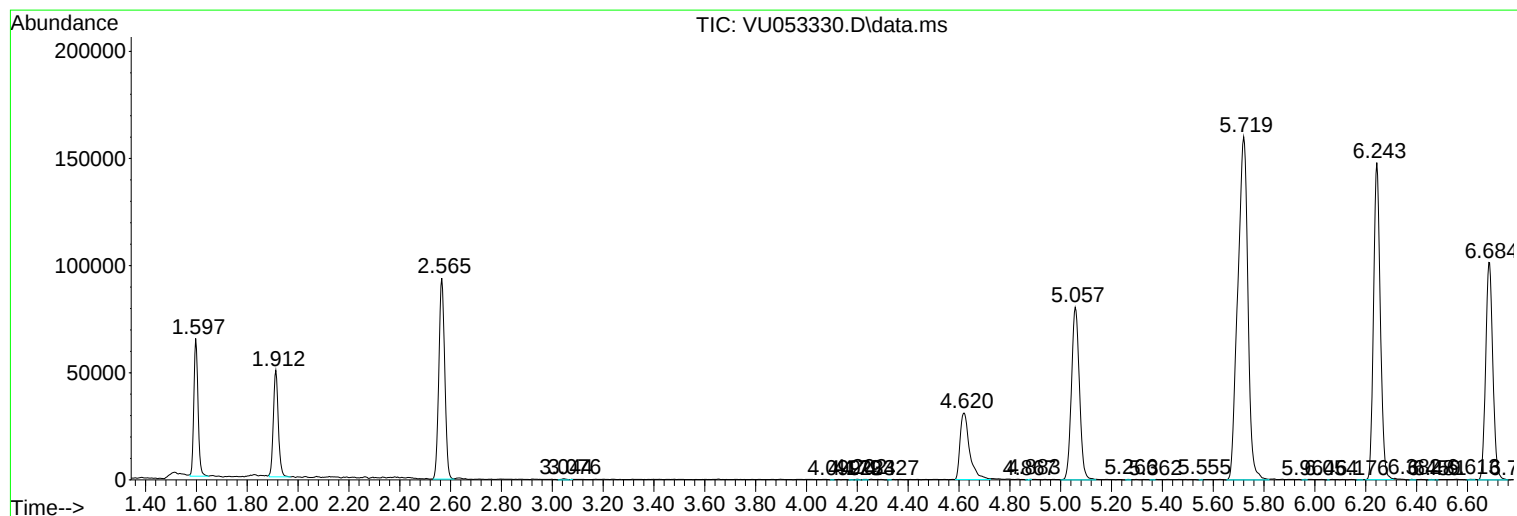

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053330.D
Acq On : 21 Mar 2023 17:32
Operator : JC/MD
Sample : 01961-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053330.D
Acq On : 21 Mar 2023 17:32
Operator : JC/MD
Sample : 01961-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------