

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053331.D
 Acq On : 21 Mar 2023 17:56
 Operator : JC/MD
 Sample : 01961-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	98	rVB2	350992	425141	12.38%	5.659%
2	1.912	170	178	195	rVB	50980	69424	2.02%	0.924%
3	2.568	369	382	402	rBV4	114179	214886	6.26%	2.861%
4	2.800	452	454	457	rBV	313	202	0.01%	0.003%
5	3.356	615	627	639	rVB4	4087	7770	0.23%	0.103%
6	3.498	668	671	674	rBV	168	127	0.00%	0.002%
7	3.668	722	724	725	rBV	163	56	0.00%	0.001%
8	3.999	825	827	833	rBV	147	102	0.00%	0.001%
9	4.115	858	863	869	rBV	254	383	0.01%	0.005%
10	4.221	895	896	897	rBV	104	25	0.00%	0.000%
11	4.250	903	905	907	rBB	115	63	0.00%	0.001%
12	4.272	907	912	917	rBB	162	250	0.01%	0.003%
13	4.295	917	919	923	rBV	237	184	0.01%	0.002%
14	4.449	966	967	969	rBV	125	36	0.00%	0.000%
15	4.658	1009	1032	1083	rBV	1509990	3434050	100.00%	45.714%
16	5.057	1142	1156	1177	rVB3	78531	172769	5.03%	2.300%
17	5.189	1196	1197	1199	rVB3	117	43	0.00%	0.001%
18	5.205	1199	1202	1205	rVB2	285	158	0.00%	0.002%
19	5.227	1205	1209	1213	rBV	174	164	0.00%	0.002%
20	5.279	1222	1225	1227	rBV	216	133	0.00%	0.002%
21	5.330	1239	1241	1243	rBV	157	112	0.00%	0.001%
22	5.539	1304	1306	1310	rBB	164	129	0.00%	0.002%
23	5.575	1311	1317	1321	rBV	207	297	0.01%	0.004%
24	5.616	1326	1330	1336	rBB	220	263	0.01%	0.004%
25	5.649	1336	1340	1342	rBV	211	217	0.01%	0.003%
26	5.719	1342	1362	1388	rBV3	160676	441574	12.86%	5.878%
27	5.970	1436	1440	1442	rBV	149	130	0.00%	0.002%
28	6.009	1449	1452	1456	rBV	172	192	0.01%	0.003%
29	6.243	1512	1525	1551	rBV	147162	274294	7.99%	3.651%
30	6.382	1566	1568	1570	rBV	150	63	0.00%	0.001%
31	6.427	1578	1582	1583	rBV	181	153	0.00%	0.002%
32	6.494	1599	1603	1604	rBV	171	142	0.00%	0.002%
33	6.536	1604	1616	1637	rVV	206806	383603	11.17%	5.107%
34	6.684	1649	1662	1689	rVB	102900	196454	5.72%	2.615%
35	6.800	1695	1698	1703	rVB2	213	237	0.01%	0.003%
36	6.909	1730	1732	1736	rBV	152	162	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053331.D
 Acq On : 21 Mar 2023 17:56
 Operator : JC/MD
 Sample : 01961-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.980	1752	1754	1757	rBV	271	170	0.00%	0.002%
38	7.047	1773	1775	1777	rVB	259	123	0.00%	0.002%
39	7.070	1778	1782	1784	rBB	129	110	0.00%	0.001%
40	7.086	1784	1787	1794	rBV	234	350	0.01%	0.005%
41	7.160	1805	1810	1811	rBV	142	154	0.00%	0.002%
42	7.372	1871	1876	1880	rBB	226	278	0.01%	0.004%
43	7.394	1880	1883	1885	rBV	156	128	0.00%	0.002%
44	7.481	1908	1910	1912	rBB	135	68	0.00%	0.001%
45	7.562	1923	1935	1954	rBV2	58505	100877	2.94%	1.343%
46	7.693	1973	1976	1980	rBV	289	137	0.00%	0.002%
47	7.812	2010	2013	2015	rBV	186	153	0.00%	0.002%
48	7.893	2024	2038	2055	rBV	204218	347661	10.12%	4.628%
49	8.057	2087	2089	2092	rBV	174	107	0.00%	0.001%
50	8.176	2115	2126	2141	rBV2	40165	66371	1.93%	0.884%
51	8.546	2237	2241	2244	rBV	200	226	0.01%	0.003%
52	8.581	2251	2252	2253	rBV	239	79	0.00%	0.001%
53	8.629	2256	2267	2299	rVV2	93616	180714	5.26%	2.406%
54	8.742	2299	2302	2305	rBV2	255	145	0.00%	0.002%
55	8.864	2336	2340	2344	rBB	214	211	0.01%	0.003%
56	8.886	2344	2347	2350	rBV	312	245	0.01%	0.003%
57	8.931	2358	2361	2363	rBV	194	156	0.00%	0.002%
58	9.218	2447	2450	2452	rBV	212	171	0.00%	0.002%
59	9.269	2463	2466	2468	rBV	167	140	0.00%	0.002%
60	9.320	2478	2482	2485	rBB	206	185	0.01%	0.002%
61	9.340	2485	2488	2492	rBB	139	142	0.00%	0.002%
62	9.365	2493	2496	2498	rBV	169	141	0.00%	0.002%
63	9.414	2498	2511	2534	rBV	207648	345663	10.07%	4.601%
64	9.565	2554	2558	2561	rBV	405	353	0.01%	0.005%
65	9.687	2595	2596	2597	rBV	110	22	0.00%	0.000%
66	9.700	2598	2600	2602	rBV	177	80	0.00%	0.001%
67	10.118	2725	2730	2737	rVB4	1147	1321	0.04%	0.018%
68	10.221	2758	2762	2768	rBB	209	301	0.01%	0.004%
69	10.250	2769	2771	2773	rBV	163	113	0.00%	0.002%
70	10.449	2829	2833	2836	rBB	143	143	0.00%	0.002%
71	10.481	2840	2843	2844	rBV	131	97	0.00%	0.001%
72	10.751	2915	2927	2944	rBV	137599	217692	6.34%	2.898%
73	10.832	2951	2952	2954	rVB	249	49	0.00%	0.001%
74	10.893	2969	2971	2973	rBV	192	131	0.00%	0.002%
75	10.954	2986	2990	2999	rBV	238	401	0.01%	0.005%
76	11.439	3139	3141	3142	rBV	217	60	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053331.D
 Acq On : 21 Mar 2023 17:56
 Operator : JC/MD
 Sample : 01961-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

77	11.526	3163	3168	3174	rBV	239	374	0.01%	0.005%
78	11.716	3224	3227	3230	rBV	224	206	0.01%	0.003%
79	11.806	3244	3255	3283	rBV	205224	325579	9.48%	4.334%
80	11.970	3301	3306	3308	rBV	232	257	0.01%	0.003%
81	12.076	3337	3339	3342	rVB	197	111	0.00%	0.001%
82	12.188	3362	3374	3393	rBV	183794	293862	8.56%	3.912%
83	13.015	3629	3631	3634	rBV2	211	142	0.00%	0.002%
84	13.989	3932	3934	3937	rVB	159	50	0.00%	0.001%
85	14.050	3949	3953	3955	rBV	196	158	0.00%	0.002%
86	14.246	4012	4014	4015	rBV	130	31	0.00%	0.000%
87	14.626	4130	4132	4135	rBV	142	55	0.00%	0.001%
88	14.780	4178	4180	4182	rBV	234	103	0.00%	0.001%
89	14.973	4237	4240	4243	rBV2	204	174	0.01%	0.002%
90	16.786	4800	4804	4809	rBV4	635	710	0.02%	0.009%
91	17.095	4898	4900	4904	rBV2	715	560	0.02%	0.007%




Sum of corrected areas: 7512028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053331.D
Acq On : 21 Mar 2023 17:56
Operator : JC/MD
Sample : 01961-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

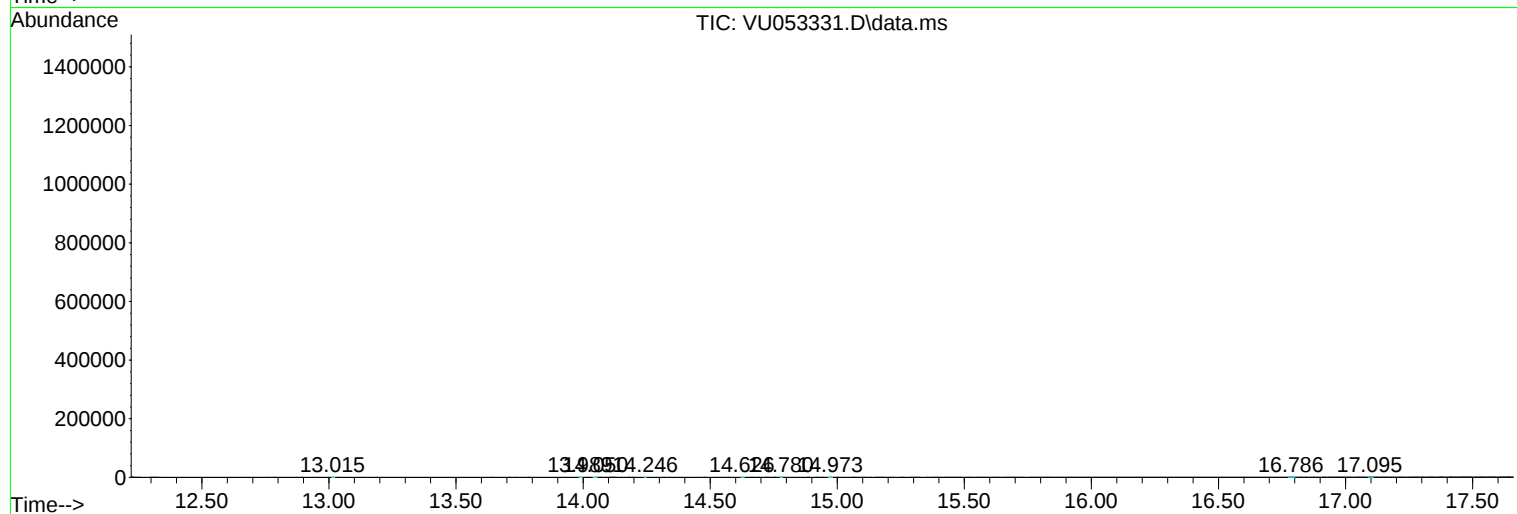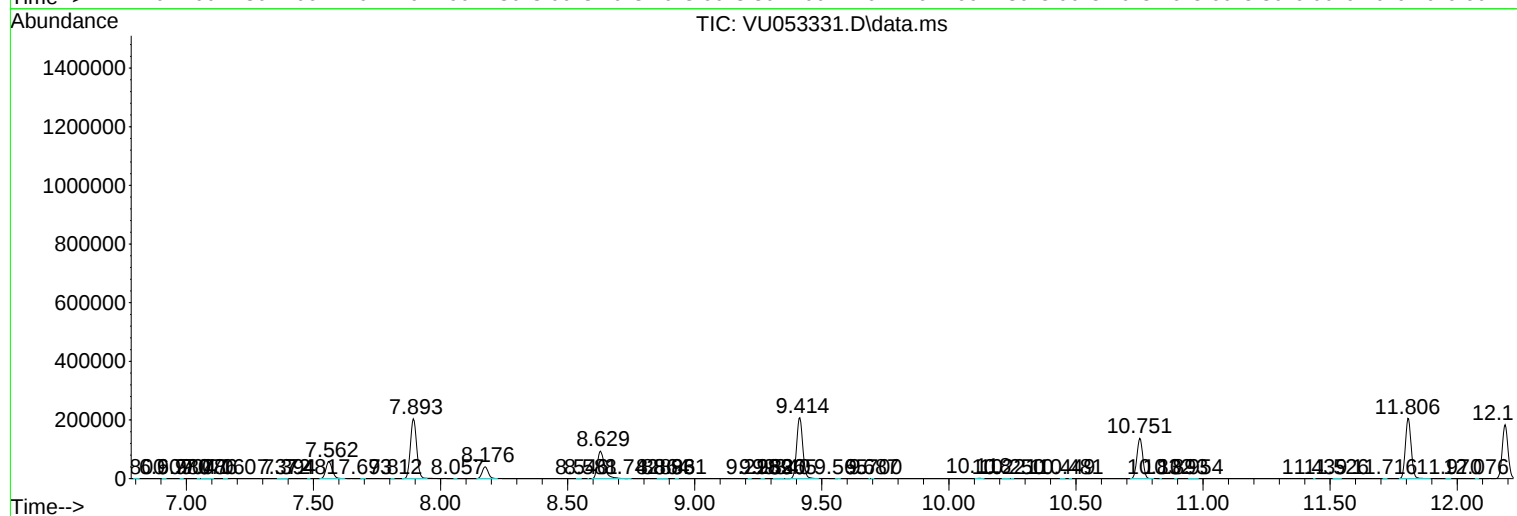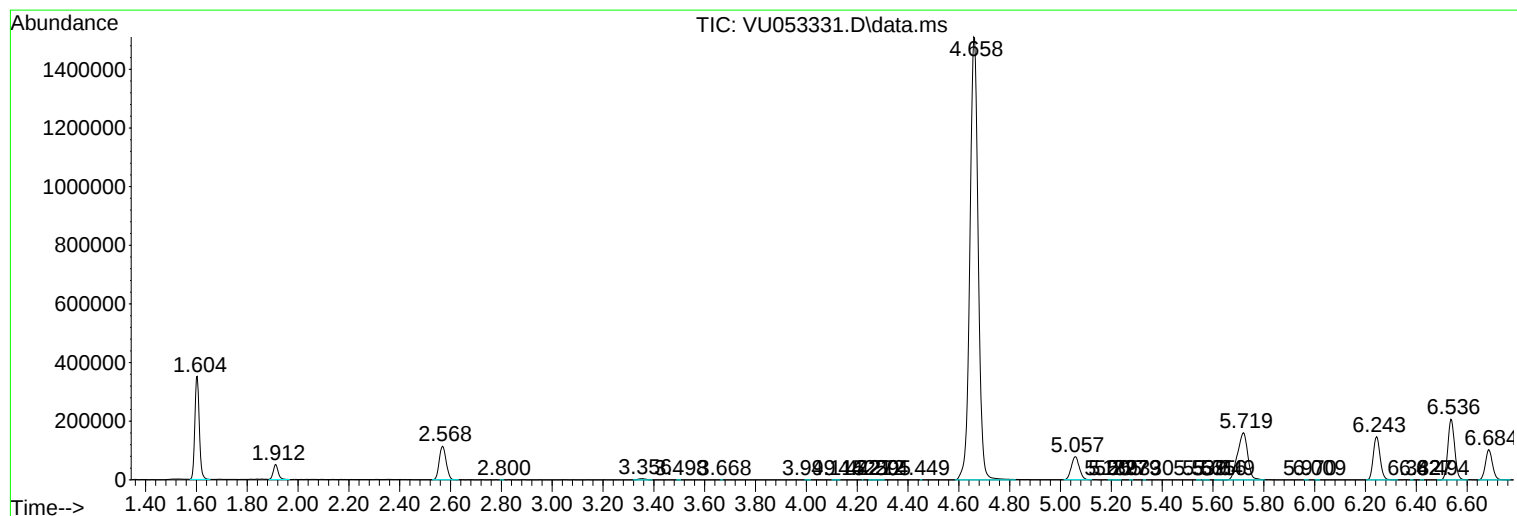

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053331.D
Acq On : 21 Mar 2023 17:56
Operator : JC/MD
Sample : 01961-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053331.D
Acq On : 21 Mar 2023 17:56
Operator : JC/MD
Sample : 01961-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------