

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053332.D
 Acq On : 21 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	66349	76618	17.66%	2.361%
2	1.912	170	178	197	rVB	49205	66881	15.41%	2.061%
3	2.565	370	381	397	rVB	92140	146852	33.84%	4.526%
4	3.623	708	710	714	rVB	175	65	0.01%	0.002%
5	3.893	791	794	799	rBV	138	119	0.03%	0.004%
6	4.041	835	840	843	rBB	178	203	0.05%	0.006%
7	4.070	844	849	851	rBV	220	250	0.06%	0.008%
8	4.166	871	879	884	rBV	267	502	0.12%	0.015%
9	4.420	955	958	960	rBV	191	155	0.04%	0.005%
10	4.481	972	977	980	rBV	170	244	0.06%	0.008%
11	4.617	1009	1019	1028	rBV	30354	69203	15.95%	2.133%
12	4.813	1077	1080	1085	rVB	172	175	0.04%	0.005%
13	4.877	1098	1100	1104	rBV	170	87	0.02%	0.003%
14	4.951	1119	1123	1125	rBV	191	188	0.04%	0.006%
15	5.057	1141	1156	1178	rBV2	78300	170431	39.28%	5.253%
16	5.282	1225	1226	1228	rBV	114	65	0.01%	0.002%
17	5.526	1300	1302	1305	rBV	167	144	0.03%	0.004%
18	5.539	1305	1306	1309	rVB	145	50	0.01%	0.002%
19	5.607	1324	1327	1335	rBB	195	280	0.06%	0.009%
20	5.645	1335	1339	1342	rBV	165	182	0.04%	0.006%
21	5.719	1342	1362	1392	rVV2	158253	433904	100.00%	13.374%
22	5.822	1392	1394	1397	rVV	219	184	0.04%	0.006%
23	5.851	1400	1403	1406	rBV	314	167	0.04%	0.005%
24	5.916	1422	1423	1426	rBV	124	33	0.01%	0.001%
25	5.977	1440	1442	1445	rBV	211	158	0.04%	0.005%
26	6.022	1452	1456	1461	rBV	181	245	0.06%	0.008%
27	6.086	1473	1476	1479	rBB	211	156	0.04%	0.005%
28	6.105	1480	1482	1485	rBV	175	148	0.03%	0.005%
29	6.163	1497	1500	1501	rBV	156	107	0.02%	0.003%
30	6.243	1512	1525	1549	rBV	136055	255859	58.97%	7.886%
31	6.459	1589	1592	1593	rBV	150	66	0.02%	0.002%
32	6.491	1598	1602	1604	rBV	225	188	0.04%	0.006%
33	6.543	1608	1618	1626	rVB4	2698	4221	0.97%	0.130%
34	6.578	1627	1629	1632	rBB	134	92	0.02%	0.003%
35	6.604	1633	1637	1639	rBV	215	204	0.05%	0.006%
36	6.684	1649	1662	1679	rBV2	100150	194671	44.86%	6.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053332.D
 Acq On : 21 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.809	1697	1701	1702	rBV	281	203	0.05%	0.006%
38	6.854	1713	1715	1718	rVB	276	144	0.03%	0.004%
39	6.883	1719	1724	1727	rBV	159	208	0.05%	0.006%
40	6.906	1729	1731	1736	rVB	209	116	0.03%	0.004%
41	7.038	1770	1772	1775	rBV	119	61	0.01%	0.002%
42	7.176	1813	1815	1817	rBV	129	37	0.01%	0.001%
43	7.301	1850	1854	1855	rBV	230	109	0.03%	0.003%
44	7.395	1878	1883	1885	rBV	245	268	0.06%	0.008%
45	7.514	1917	1920	1922	rBV	147	128	0.03%	0.004%
46	7.562	1922	1935	1951	rVV	56915	98358	22.67%	3.032%
47	7.751	1989	1994	1996	rBV	194	202	0.05%	0.006%
48	7.793	2004	2007	2009	rBV	208	180	0.04%	0.006%
49	7.893	2025	2038	2057	rBV	199972	344573	79.41%	10.620%
50	8.041	2081	2084	2085	rBV	239	129	0.03%	0.004%
51	8.176	2116	2126	2141	rBV2	38956	64490	14.86%	1.988%
52	8.259	2147	2152	2157	rBV	185	277	0.06%	0.009%
53	8.337	2173	2176	2180	rBV	120	90	0.02%	0.003%
54	8.423	2200	2203	2206	rBB	193	151	0.03%	0.005%
55	8.443	2207	2209	2210	rBV	114	63	0.01%	0.002%
56	8.591	2251	2255	2256	rBV	179	147	0.03%	0.005%
57	8.629	2256	2267	2292	rVV2	91118	173665	40.02%	5.353%
58	8.751	2303	2305	2306	rBV	176	75	0.02%	0.002%
59	8.870	2339	2342	2344	rBV	135	116	0.03%	0.004%
60	8.964	2368	2371	2375	rBV	189	212	0.05%	0.007%
61	9.076	2403	2406	2409	rBB	216	153	0.04%	0.005%
62	9.099	2410	2413	2416	rBV	230	209	0.05%	0.006%
63	9.163	2428	2433	2437	rBV	267	349	0.08%	0.011%
64	9.202	2442	2445	2447	rBV	157	111	0.03%	0.003%
65	9.285	2465	2471	2475	rBV	186	287	0.07%	0.009%
66	9.330	2482	2485	2488	rBV	213	211	0.05%	0.007%
67	9.414	2498	2511	2533	rBV	193210	323968	74.66%	9.985%
68	9.568	2557	2559	2561	rVB	129	29	0.01%	0.001%
69	9.703	2599	2601	2604	rBV2	164	103	0.02%	0.003%
70	9.806	2629	2633	2638	rBV	235	270	0.06%	0.008%
71	10.115	2724	2729	2737	rVB2	1361	1830	0.42%	0.056%
72	10.147	2737	2739	2740	rBV2	130	36	0.01%	0.001%
73	10.237	2764	2767	2768	rBV	154	111	0.03%	0.003%
74	10.620	2885	2886	2890	rVB	153	54	0.01%	0.002%
75	10.751	2915	2927	2942	rBV	135090	210461	48.50%	6.487%
76	10.919	2976	2979	2982	rBV	226	224	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053332.D
 Acq On : 21 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.992	2999	3002	3005	rBV	191	187	0.04%	0.006%
78	11.079	3027	3029	3032	rVB	152	43	0.01%	0.001%
79	11.160	3052	3054	3060	rBV	225	185	0.04%	0.006%
80	11.369	3115	3119	3122	rBV	238	238	0.05%	0.007%
81	11.472	3149	3151	3155	rBV	149	120	0.03%	0.004%
82	11.806	3244	3255	3271	rBV	191487	305262	70.35%	9.409%
83	12.054	3330	3332	3336	rVB	209	96	0.02%	0.003%
84	12.189	3362	3374	3395	rBV	181448	290714	67.00%	8.960%
85	12.308	3408	3411	3413	rBV	408	303	0.07%	0.009%
86	12.494	3467	3469	3470	rBV	161	50	0.01%	0.002%
87	12.706	3534	3535	3540	rBV	143	121	0.03%	0.004%
88	12.774	3554	3556	3559	rBV	223	95	0.02%	0.003%
89	12.883	3587	3590	3594	rBV	111	114	0.03%	0.004%
90	12.935	3605	3606	3607	rBV	160	37	0.01%	0.001%
91	13.111	3659	3661	3664	rVB2	220	126	0.03%	0.004%
92	14.513	4094	4097	4101	rBV	219	210	0.05%	0.006%
93	14.610	4124	4127	4130	rVB	197	94	0.02%	0.003%
94	14.931	4224	4227	4230	rBV	196	99	0.02%	0.003%
95	15.208	4310	4313	4315	rBV	223	120	0.03%	0.004%
96	15.224	4315	4318	4320	rBV	223	160	0.04%	0.005%
97	15.487	4397	4400	4403	rBV	377	328	0.08%	0.010%
98	16.092	4584	4588	4591	rBV2	336	286	0.07%	0.009%




Sum of corrected areas: 3244493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053332.D
Acq On : 21 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

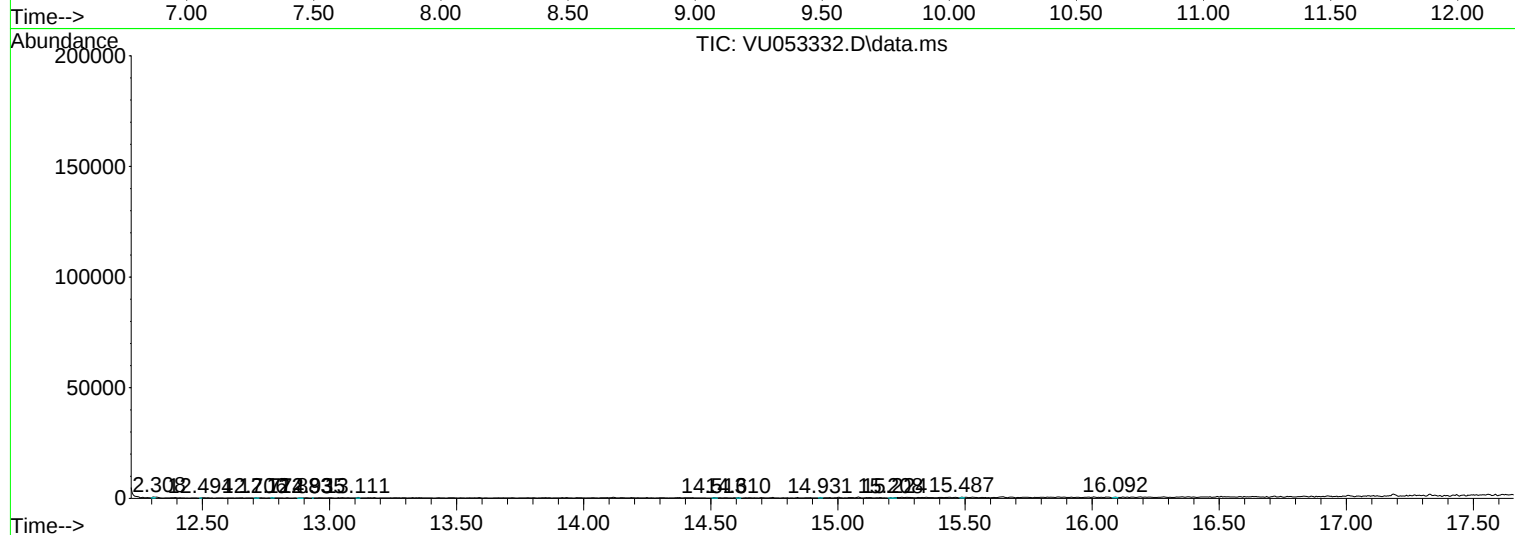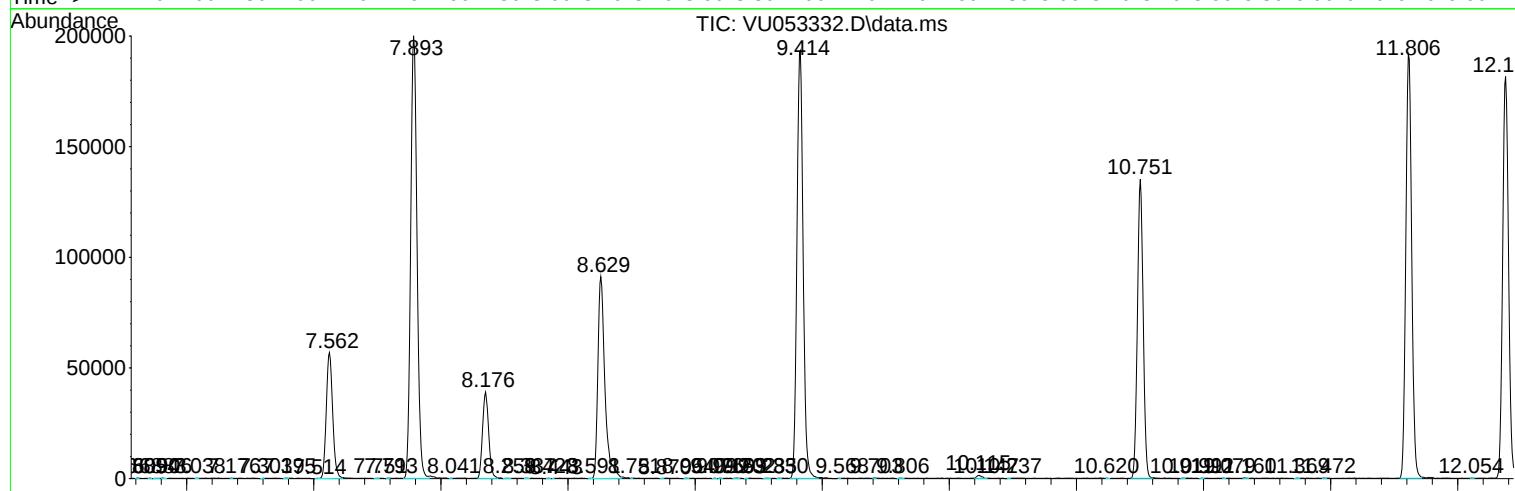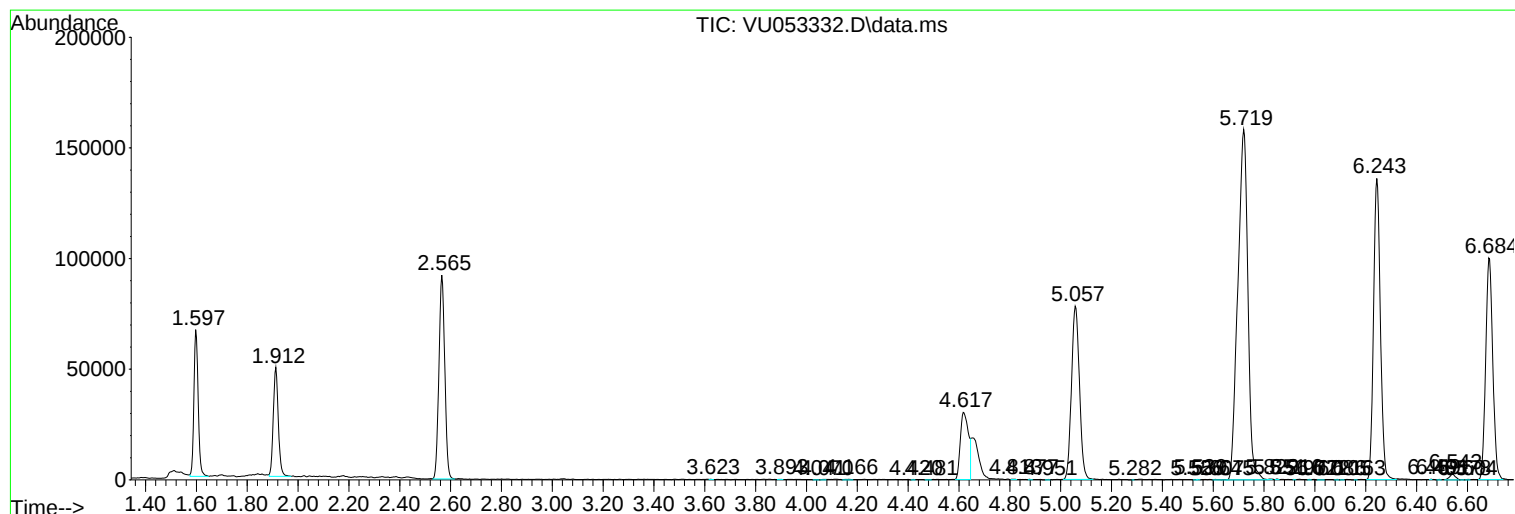

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053332.D
Acq On : 21 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053332.D
Acq On : 21 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------