

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053334.D
 Acq On : 21 Mar 2023 19:07
 Operator : JC/MD
 Sample : 01995-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB2	77150	93499	17.14%	2.393%
2	1.912	170	178	197	rVB	54769	74779	13.71%	1.914%
3	2.565	370	381	397	rVB	97422	155102	28.44%	3.969%
4	3.350	618	625	635	rVB5	2106	3586	0.66%	0.092%
5	4.115	858	863	866	rBV	230	287	0.05%	0.007%
6	4.192	885	887	889	rBV	181	120	0.02%	0.003%
7	4.288	915	917	919	rVB	135	35	0.01%	0.001%
8	4.333	929	931	932	rBV	221	85	0.02%	0.002%
9	4.661	1009	1033	1061	rBV2	206215	545444	100.00%	13.959%
10	4.867	1094	1097	1100	rBV	308	265	0.05%	0.007%
11	4.887	1100	1103	1104	rBV	172	88	0.02%	0.002%
12	5.057	1135	1156	1172	rBV	83723	181057	33.19%	4.634%
13	5.157	1185	1187	1192	rVB2	307	145	0.03%	0.004%
14	5.240	1210	1213	1215	rBV	195	150	0.03%	0.004%
15	5.279	1223	1225	1227	rBV	263	163	0.03%	0.004%
16	5.346	1242	1246	1249	rBB	198	181	0.03%	0.005%
17	5.372	1251	1254	1257	rBV	170	160	0.03%	0.004%
18	5.443	1274	1276	1279	rBV	138	118	0.02%	0.003%
19	5.504	1291	1295	1300	rBV	200	267	0.05%	0.007%
20	5.578	1316	1318	1320	rBB	113	42	0.01%	0.001%
21	5.591	1321	1322	1323	rBV	116	45	0.01%	0.001%
22	5.632	1333	1335	1339	rVB	170	74	0.01%	0.002%
23	5.719	1341	1362	1388	rBV3	166106	454513	83.33%	11.632%
24	5.928	1423	1427	1430	rBV	187	209	0.04%	0.005%
25	6.022	1452	1456	1463	rBV	231	349	0.06%	0.009%
26	6.073	1470	1472	1474	rBB	126	68	0.01%	0.002%
27	6.095	1477	1479	1482	rBB	115	63	0.01%	0.002%
28	6.118	1483	1486	1493	rBB	205	287	0.05%	0.007%
29	6.160	1494	1499	1505	rBV	200	273	0.05%	0.007%
30	6.243	1512	1525	1546	rBV	144631	273663	50.17%	7.004%
31	6.433	1582	1584	1585	rBB	114	43	0.01%	0.001%
32	6.446	1586	1588	1590	rBB	123	64	0.01%	0.002%
33	6.462	1590	1593	1595	rBV	159	130	0.02%	0.003%
34	6.472	1595	1596	1598	rVB	112	29	0.01%	0.001%
35	6.542	1609	1618	1626	rBV6	2397	4099	0.75%	0.105%
36	6.684	1648	1662	1682	rBV	106464	203148	37.24%	5.199%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053334.D
 Acq On : 21 Mar 2023 19:07
 Operator : JC/MD
 Sample : 01995-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.825	1703	1706	1708	rBV	242	166	0.03%	0.004%
38	6.883	1721	1724	1727	rBV	143	155	0.03%	0.004%
39	6.915	1733	1734	1736	rVB	131	48	0.01%	0.001%
40	6.983	1750	1755	1761	rBB	189	238	0.04%	0.006%
41	7.018	1762	1766	1768	rBV	188	180	0.03%	0.005%
42	7.157	1807	1809	1815	rVB	331	242	0.04%	0.006%
43	7.192	1816	1820	1822	rBV	418	313	0.06%	0.008%
44	7.205	1822	1824	1827	rVV	182	77	0.01%	0.002%
45	7.292	1848	1851	1852	rBV	258	151	0.03%	0.004%
46	7.330	1860	1863	1869	rBB	194	233	0.04%	0.006%
47	7.362	1869	1873	1874	rBV	150	124	0.02%	0.003%
48	7.459	1902	1903	1904	rBV	117	28	0.01%	0.001%
49	7.504	1915	1917	1921	rBV	233	191	0.04%	0.005%
50	7.562	1923	1935	1951	rVV2	61101	103612	19.00%	2.652%
51	7.632	1955	1957	1963	rVB2	385	290	0.05%	0.007%
52	7.693	1974	1976	1977	rBV2	123	35	0.01%	0.001%
53	7.719	1981	1984	1988	rBB	160	147	0.03%	0.004%
54	7.745	1988	1992	1994	rBV	233	203	0.04%	0.005%
55	7.893	2025	2038	2056	rBV	204522	354365	64.97%	9.069%
56	8.047	2080	2086	2089	rBV	199	286	0.05%	0.007%
57	8.176	2114	2126	2144	rBV	41116	69601	12.76%	1.781%
58	8.250	2145	2149	2153	rVV2	197	154	0.03%	0.004%
59	8.343	2172	2178	2180	rBV	244	278	0.05%	0.007%
60	8.475	2215	2219	2220	rBV	281	214	0.04%	0.005%
61	8.629	2256	2267	2297	rVB3	96635	183859	33.71%	4.705%
62	8.732	2297	2299	2302	rBV	241	195	0.04%	0.005%
63	8.980	2373	2376	2378	rBV	233	156	0.03%	0.004%
64	9.034	2392	2393	2394	rVB	110	21	0.00%	0.001%
65	9.079	2400	2407	2413	rBV	190	370	0.07%	0.009%
66	9.128	2419	2422	2426	rBV	222	230	0.04%	0.006%
67	9.214	2446	2449	2453	rBV	197	162	0.03%	0.004%
68	9.414	2499	2511	2531	rBV	206178	341605	62.63%	8.743%
69	9.536	2545	2549	2553	rVB2	285	322	0.06%	0.008%
70	9.562	2554	2557	2561	rBV	158	193	0.04%	0.005%
71	9.771	2617	2622	2624	rBV	200	229	0.04%	0.006%
72	9.861	2646	2650	2656	rBV	188	268	0.05%	0.007%
73	9.922	2666	2669	2674	rVB	226	153	0.03%	0.004%
74	10.005	2693	2695	2699	rBB	152	130	0.02%	0.003%
75	10.037	2699	2705	2710	rBV	231	399	0.07%	0.010%
76	10.060	2710	2712	2719	rVV	282	232	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053334.D
 Acq On : 21 Mar 2023 19:07
 Operator : JC/MD
 Sample : 01995-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.121	2723	2731	2739	rBV3	1103	1816	0.33%	0.046%
78	10.272	2775	2778	2786	rBB	232	341	0.06%	0.009%
79	10.320	2789	2793	2795	rBV	245	229	0.04%	0.006%
80	10.555	2863	2866	2867	rBV	229	141	0.03%	0.004%
81	10.693	2905	2909	2913	rBV	194	263	0.05%	0.007%
82	10.751	2915	2927	2943	rVV	142708	224628	41.18%	5.749%
83	10.861	2958	2961	2965	rBV	265	257	0.05%	0.007%
84	11.082	3028	3030	3032	rBV	181	119	0.02%	0.003%
85	11.529	3164	3169	3171	rBV	243	293	0.05%	0.007%
86	11.806	3244	3255	3272	rBV	204136	323394	59.29%	8.277%
87	11.915	3287	3289	3294	rVB	241	151	0.03%	0.004%
88	12.188	3362	3374	3390	rBV	186806	302237	55.41%	7.735%
89	12.311	3405	3412	3413	rBV3	434	462	0.08%	0.012%
90	14.893	4211	4215	4217	rBV	220	185	0.03%	0.005%
91	15.208	4307	4313	4317	rBV2	248	375	0.07%	0.010%


Sum of corrected areas: 3907376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053334.D
Acq On : 21 Mar 2023 19:07
Operator : JC/MD
Sample : 01995-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

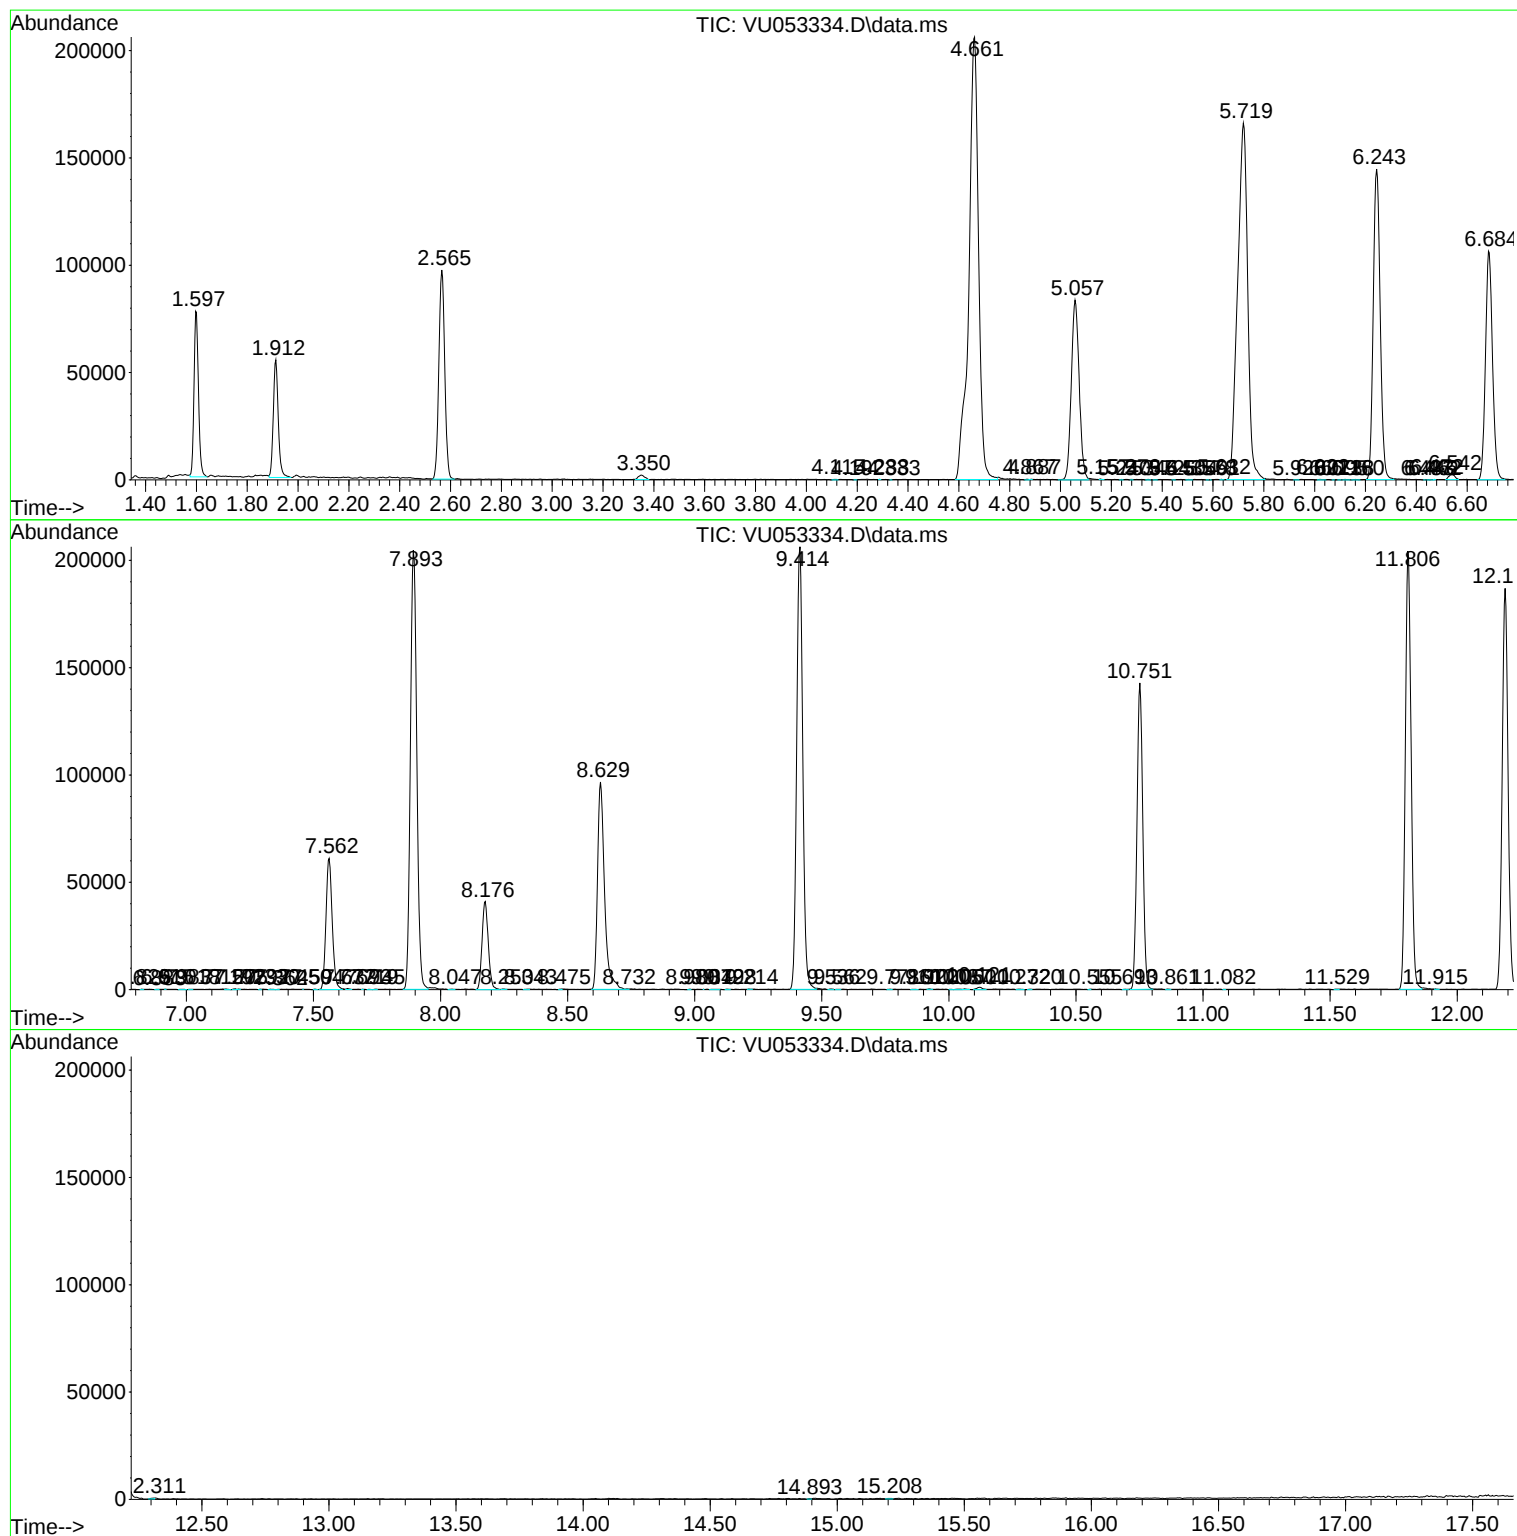

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053334.D
Acq On : 21 Mar 2023 19:07
Operator : JC/MD
Sample : 01995-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053334.D
Acq On : 21 Mar 2023 19:07
Operator : JC/MD
Sample : 01995-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------