

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053337.D
 Acq On : 21 Mar 2023 20:17
 Operator : JC/MD
 Sample : 01995-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	62903	71663	16.40%	2.159%
2	1.912	170	178	197	rVB	49603	69054	15.80%	2.080%
3	2.565	370	381	395	rVB2	91360	146235	33.46%	4.406%
4	3.035	525	527	529	rBV	274	139	0.03%	0.004%
5	3.379	633	634	636	rBV	115	45	0.01%	0.001%
6	3.523	676	679	683	rBV	155	111	0.03%	0.003%
7	3.652	713	719	723	rBV	216	334	0.08%	0.010%
8	4.350	933	936	937	rBV	122	53	0.01%	0.002%
9	4.469	965	973	976	rBV	216	350	0.08%	0.011%
10	4.546	991	997	1001	rBV	262	332	0.08%	0.010%
11	4.616	1008	1019	1051	rBV2	30797	82269	18.82%	2.478%
12	4.851	1088	1092	1094	rBV	301	233	0.05%	0.007%
13	4.922	1110	1114	1117	rBV	227	236	0.05%	0.007%
14	4.967	1126	1128	1130	rBB	112	43	0.01%	0.001%
15	4.989	1131	1135	1139	rBB	197	209	0.05%	0.006%
16	5.057	1139	1156	1177	rBV2	80686	176624	40.42%	5.321%
17	5.182	1194	1195	1197	rVB2	327	85	0.02%	0.003%
18	5.208	1200	1203	1205	rBV	184	147	0.03%	0.004%
19	5.472	1278	1285	1286	rBV	278	273	0.06%	0.008%
20	5.587	1318	1321	1323	rBV	185	150	0.03%	0.005%
21	5.719	1342	1362	1388	rBV2	157432	437022	100.00%	13.166%
22	5.858	1403	1405	1408	rVB	206	126	0.03%	0.004%
23	5.967	1435	1439	1441	rVB	268	213	0.05%	0.006%
24	6.005	1447	1451	1452	rBV	155	131	0.03%	0.004%
25	6.041	1457	1462	1465	rBV	307	271	0.06%	0.008%
26	6.243	1511	1525	1542	rBV	144704	273608	62.61%	8.243%
27	6.382	1566	1568	1569	rBV	154	46	0.01%	0.001%
28	6.391	1569	1571	1573	rVB	158	47	0.01%	0.001%
29	6.449	1585	1589	1592	rBV	229	234	0.05%	0.007%
30	6.504	1603	1606	1610	rBB	178	162	0.04%	0.005%
31	6.536	1611	1616	1618	rBV2	1092	892	0.20%	0.027%
32	6.613	1638	1640	1642	rBV	151	103	0.02%	0.003%
33	6.687	1649	1663	1682	rBV	101125	196487	44.96%	5.919%
34	6.825	1701	1706	1710	rBV	201	282	0.06%	0.008%
35	6.976	1751	1753	1759	rBV	192	229	0.05%	0.007%
36	7.050	1774	1776	1780	rVB	254	135	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053337.D
 Acq On : 21 Mar 2023 20:17
 Operator : JC/MD
 Sample : 01995-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.153	1805	1808	1809	rBV	161	113	0.03%	0.003%
38	7.189	1815	1819	1825	rVB	404	497	0.11%	0.015%
39	7.214	1825	1827	1829	rBV	152	108	0.02%	0.003%
40	7.275	1842	1846	1848	rBV	190	172	0.04%	0.005%
41	7.292	1848	1851	1855	rVV	159	121	0.03%	0.004%
42	7.369	1870	1875	1876	rBV	262	226	0.05%	0.007%
43	7.388	1879	1881	1882	rBV	132	56	0.01%	0.002%
44	7.439	1894	1897	1900	rBV	193	192	0.04%	0.006%
45	7.478	1904	1909	1911	rBV	217	244	0.06%	0.007%
46	7.517	1917	1921	1922	rBV	262	196	0.04%	0.006%
47	7.562	1924	1935	1953	rVB	56458	97255	22.25%	2.930%
48	7.661	1963	1966	1968	rBV	194	159	0.04%	0.005%
49	7.700	1975	1978	1979	rBV	178	120	0.03%	0.004%
50	7.735	1984	1989	1991	rBV	146	173	0.04%	0.005%
51	7.796	2005	2008	2012	rBV	151	185	0.04%	0.006%
52	7.816	2012	2014	2017	rVV	162	85	0.02%	0.003%
53	7.893	2025	2038	2055	rBV	201128	344656	78.86%	10.383%
54	8.028	2076	2080	2084	rBV2	307	223	0.05%	0.007%
55	8.073	2092	2094	2096	rBV	169	112	0.03%	0.003%
56	8.134	2109	2113	2115	rBV	162	160	0.04%	0.005%
57	8.176	2115	2126	2139	rVV	39051	65348	14.95%	1.969%
58	8.275	2154	2157	2161	rVB	192	103	0.02%	0.003%
59	8.427	2200	2204	2206	rBV	171	142	0.03%	0.004%
60	8.513	2229	2231	2234	rVB	142	61	0.01%	0.002%
61	8.552	2238	2243	2248	rVB2	1153	1300	0.30%	0.039%
62	8.629	2253	2267	2293	rBV2	91423	175186	40.09%	5.278%
63	8.832	2322	2330	2333	rBV	236	346	0.08%	0.010%
64	8.951	2364	2367	2370	rBV	171	164	0.04%	0.005%
65	9.066	2401	2403	2404	rBV	125	72	0.02%	0.002%
66	9.156	2429	2431	2434	rVB	143	63	0.01%	0.002%
67	9.346	2486	2490	2492	rBV	168	176	0.04%	0.005%
68	9.414	2499	2511	2530	rBV	204734	338792	77.52%	10.207%
69	9.536	2547	2549	2550	rVB	324	107	0.02%	0.003%
70	9.558	2553	2556	2559	rBV	189	178	0.04%	0.005%
71	9.783	2625	2626	2627	rBV	118	44	0.01%	0.001%
72	9.841	2641	2644	2645	rBV	181	119	0.03%	0.004%
73	9.867	2650	2652	2653	rBV	163	86	0.02%	0.003%
74	9.954	2675	2679	2683	rBV	240	280	0.06%	0.008%
75	10.070	2711	2715	2717	rBV	137	147	0.03%	0.004%
76	10.111	2725	2728	2729	rBV2	618	329	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
 Data File : VU053337.D
 Acq On : 21 Mar 2023 20:17
 Operator : JC/MD
 Sample : 01995-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.246	2767	2770	2772	rBV	147	127	0.03%	0.004%
78	10.443	2826	2831	2836	rBV	245	346	0.08%	0.010%
79	10.684	2900	2906	2910	rBV	242	307	0.07%	0.009%
80	10.751	2914	2927	2943	rVV	134767	212628	48.65%	6.406%
81	10.828	2948	2951	2953	rBV	182	87	0.02%	0.003%
82	11.172	3055	3058	3060	rBV	227	117	0.03%	0.004%
83	11.314	3100	3102	3105	rBV	256	188	0.04%	0.006%
84	11.806	3244	3255	3280	rVB	204968	323387	74.00%	9.742%
85	11.918	3288	3290	3291	rBV	173	58	0.01%	0.002%
86	12.188	3361	3374	3393	rBV	183185	292320	66.89%	8.806%
87	12.317	3407	3414	3417	rVB2	641	807	0.18%	0.024%
88	12.336	3417	3420	3422	rBV	149	106	0.02%	0.003%
89	12.446	3452	3454	3457	rBV	155	63	0.01%	0.002%
90	12.626	3506	3510	3515	rBV	279	355	0.08%	0.011%
91	12.758	3548	3551	3556	rBV2	212	215	0.05%	0.006%
92	13.343	3730	3733	3735	rBV	165	122	0.03%	0.004%
93	13.883	3898	3901	3904	rBV	210	149	0.03%	0.004%
94	14.031	3945	3947	3949	rVB	158	44	0.01%	0.001%
95	14.105	3967	3970	3974	rVB	406	214	0.05%	0.006%
96	14.372	4046	4053	4058	rBV	346	515	0.12%	0.016%
97	14.970	4235	4239	4241	rBV2	330	227	0.05%	0.007%
98	15.031	4256	4258	4259	rBV2	150	37	0.01%	0.001%
99	15.253	4325	4327	4332	rBV2	202	187	0.04%	0.006%
100	15.539	4413	4416	4418	rBV	208	97	0.02%	0.003%




Sum of corrected areas: 3319372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053337.D
Acq On : 21 Mar 2023 20:17
Operator : JC/MD
Sample : 01995-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

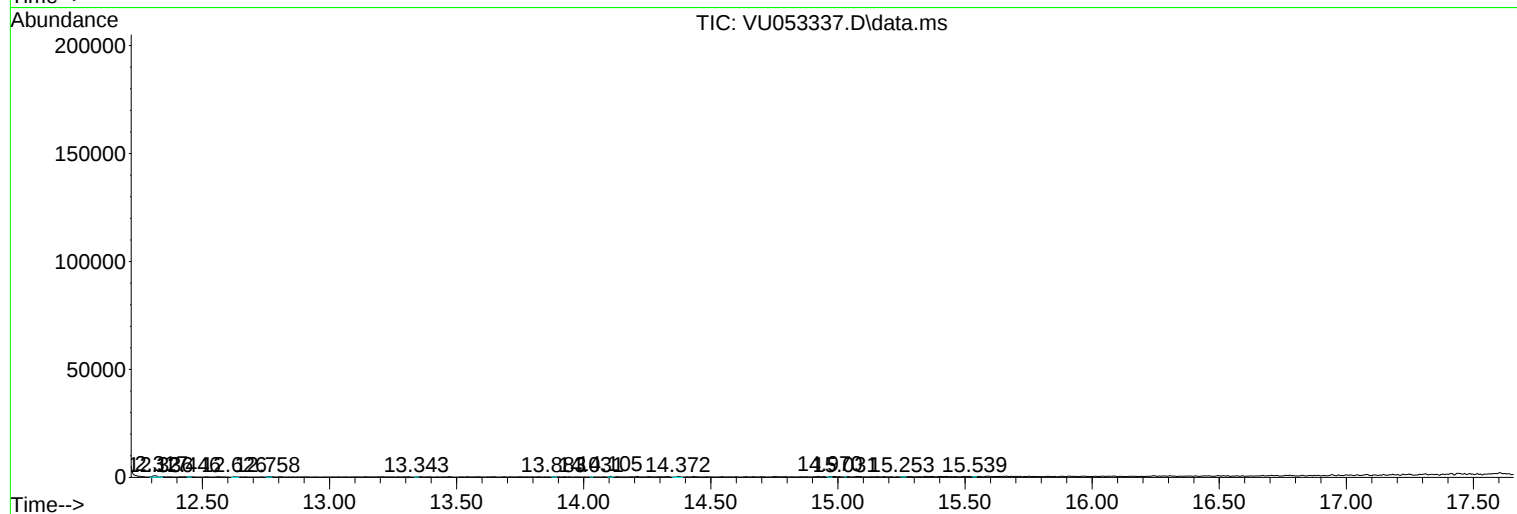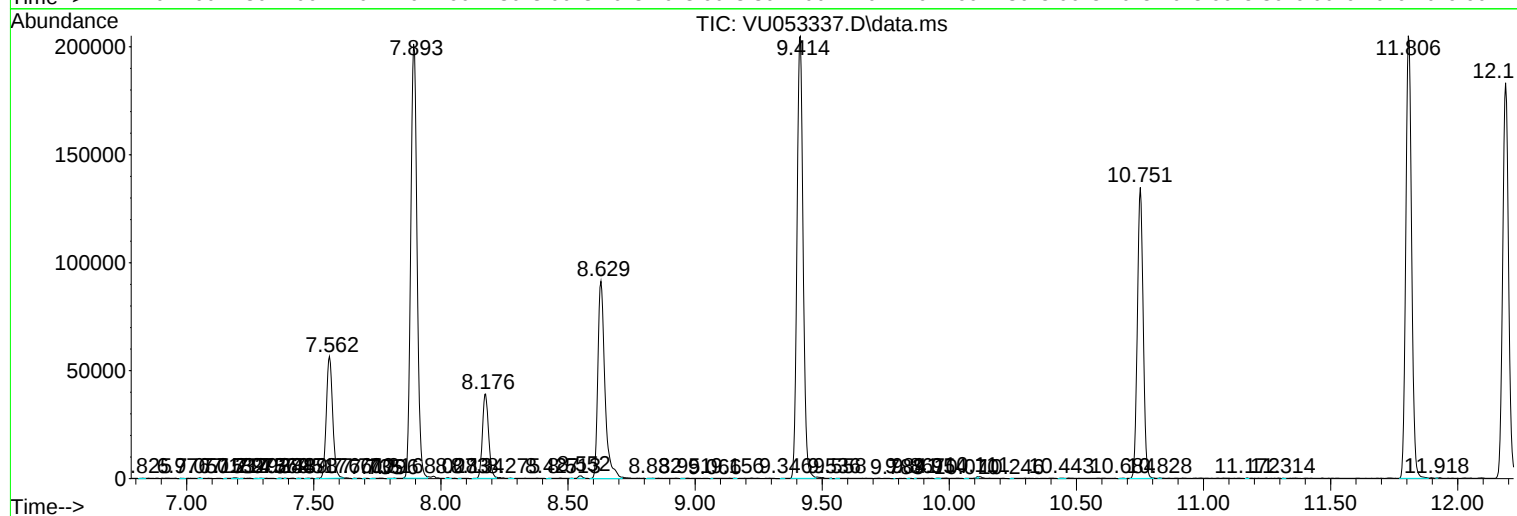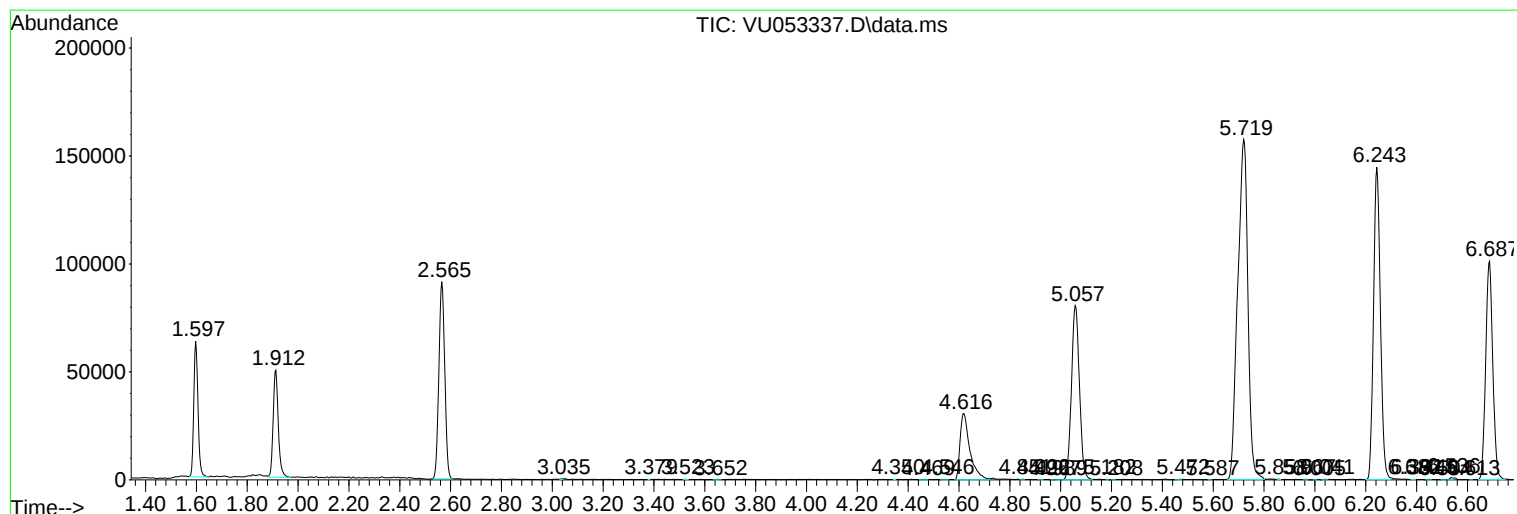

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053337.D
Acq On : 21 Mar 2023 20:17
Operator : JC/MD
Sample : 01995-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053337.D
Acq On : 21 Mar 2023 20:17
Operator : JC/MD
Sample : 01995-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc