
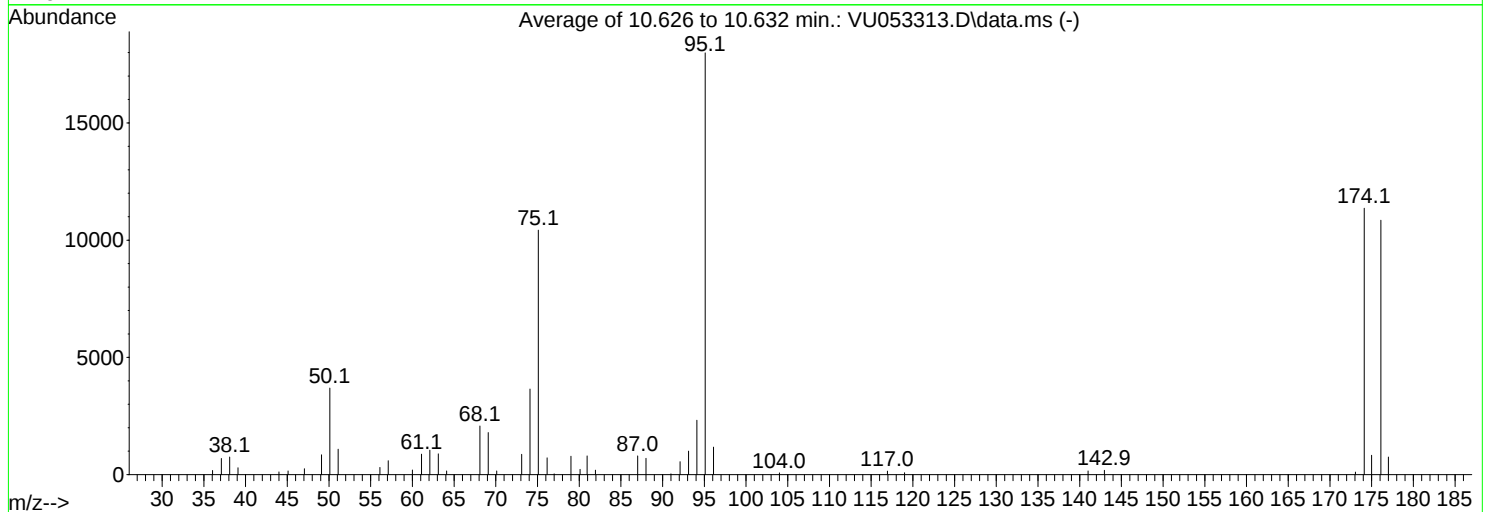


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032123\
Data File : VU053313.D
Acq On : 21 Mar 2023 09:48
Operator : JC/MD
Sample : BFB167
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB167

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Thu Mar 23 02:41:20 2023

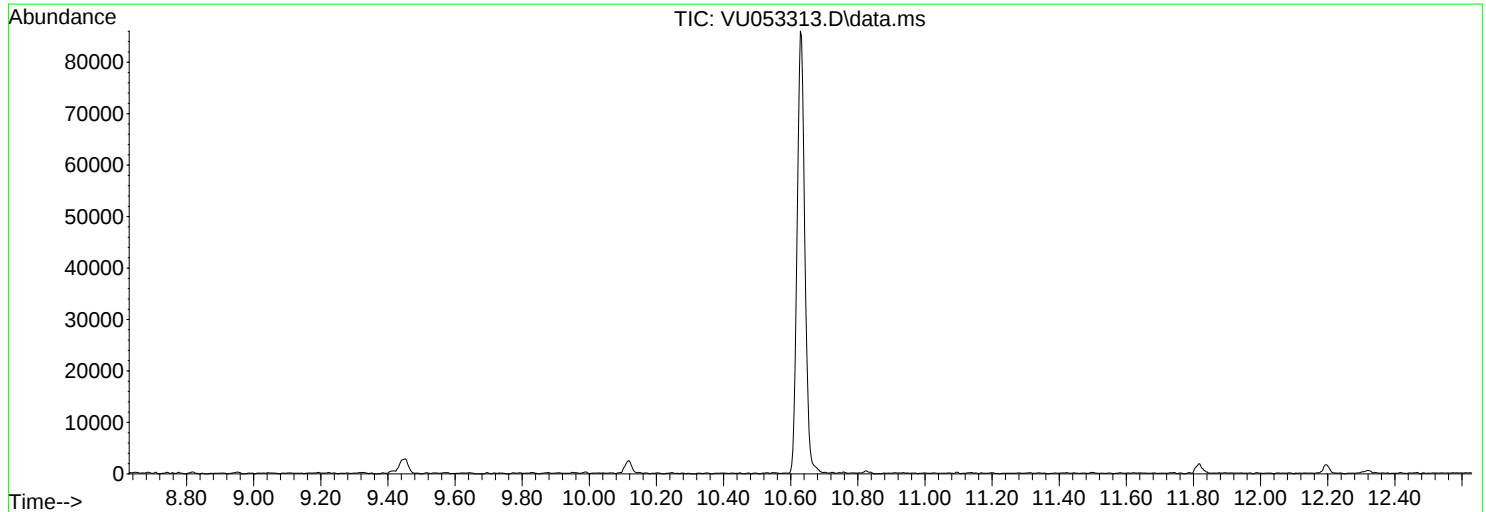

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	3693	PASS
75	95	30	80	58.0	10426	PASS
95	95	100	100	100.0	17989	PASS
96	95	5	9	6.5	1173	PASS
173	174	0.00	2	0.9	107	PASS
174	95	50	120	63.1	11359	PASS
175	174	5	9	7.3	824	PASS
176	174	95	101	95.5	10848	PASS
177	176	5	9	6.9	752	PASS

m/z	Abundance
44.10	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.00	202.0
37.10	603.0
38.10	699.0
39.10	297.0
44.00	211.0
45.10	155.0
47.00	259.0
49.10	888.0
50.10	3587.0
51.10	1124.0
56.10	298.0
57.10	606.0
60.10	152.0
61.10	852.0
62.10	1032.0
63.10	854.0
64.10	118.0
68.10	1981.0
69.10	1752.0
70.10	154.0
73.10	826.0
74.10	3407.0
75.10	9694.0
76.20	614.0
79.00	667.0
80.10	187.0
80.90	693.0
82.00	178.0
87.00	742.0
88.00	537.0
92.10	476.0
93.10	900.0
94.10	2271.0
95.10	17400.0
96.10	1197.0
116.90	105.0
141.00	175.0
142.90	177.0
173.00	100.0
174.10	10728.0
175.00	713.0
176.10	9867.0
177.00	772.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.10	190.0
37.10	723.0
38.10	785.0
39.10	305.0
44.00	268.0
45.10	171.0
47.00	266.0
49.10	887.0
50.10	3801.0
51.10	1111.0
56.10	325.0
57.10	618.0
60.00	208.0
61.10	894.0
62.10	1074.0
63.10	926.0
64.10	175.0
68.10	2146.0
69.10	1857.0
70.10	153.0
73.10	883.0
74.10	3794.0
75.10	10874.0
76.10	710.0
79.00	801.0
80.10	230.0
81.00	815.0
82.00	195.0
87.00	835.0
88.00	687.0
91.00	101.0
92.10	581.0
93.10	1051.0
94.10	2438.0
95.10	18544.0
96.10	1225.0
104.00	112.0
116.90	150.0
119.00	120.0
141.00	150.0
142.90	195.0
173.00	114.0
174.10	11723.0
175.00	834.0
176.10	11223.0
177.00	773.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.10	146.0
37.10	737.0
38.10	763.0
39.10	270.0
44.00	311.0
45.10	146.0
47.10	240.0
49.10	765.0
50.10	3692.0
51.10	1025.0
56.10	300.0
57.10	548.0
59.90	230.0
61.10	869.0
62.10	1024.0
63.10	877.0
64.10	188.0
68.10	2101.0
69.10	1773.0
70.10	160.0
73.10	893.0
74.10	3759.0
75.10	10710.0
76.10	817.0
77.00	101.0
79.00	878.0
80.10	254.0
81.00	892.0
81.90	195.0
87.00	815.0
88.00	865.0
92.10	597.0
93.10	1056.0
94.10	2251.0
95.10	18024.0
96.10	1098.0
104.00	122.0
117.00	189.0
119.00	124.0
141.00	145.0
143.00	188.0
173.10	107.0
174.10	11626.0
175.00	924.0
176.10	11454.0
177.00	711.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167