

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030296.D
 Acq On : 22 Mar 2019 10:33
 Operator : JC/SP
 Sample : VU0322WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	38	rVB	12235	11800	0.66%	0.082%
2	1.399	89	96	111	rBV	257743	261421	14.54%	1.809%
3	1.679	175	183	202	rVB	191103	242728	13.50%	1.680%
4	2.270	356	367	381	rBV	427399	643768	35.82%	4.456%
5	2.466	423	428	429	rBV	2547	1937	0.11%	0.013%
6	2.614	470	474	479	rBV	1177	1534	0.09%	0.011%
7	2.868	549	553	558	rVB	1546	1416	0.08%	0.010%
8	2.897	558	562	564	rBV	1377	1170	0.07%	0.008%
9	2.984	585	589	592	rBV3	1236	1228	0.07%	0.008%
10	3.148	637	640	644	rBV	1402	1184	0.07%	0.008%
11	3.293	682	685	687	rBV	1502	953	0.05%	0.007%
12	3.325	692	695	698	rBV	1237	1071	0.06%	0.007%
13	3.424	721	726	729	rVB	1550	1330	0.07%	0.009%
14	3.643	790	794	800	rBV	958	1061	0.06%	0.007%
15	3.707	811	814	819	rVB	1054	903	0.05%	0.006%
16	3.868	858	864	870	rVB	1540	1845	0.10%	0.013%
17	4.067	921	926	929	rVB2	1263	972	0.05%	0.007%
18	4.174	947	959	989	rVV	171115	449941	25.03%	3.114%
19	4.373	1018	1021	1026	rVB3	1873	1957	0.11%	0.014%
20	4.466	1047	1050	1055	rBV2	1188	1073	0.06%	0.007%
21	4.643	1089	1105	1130	rBV	292999	704430	39.19%	4.876%
22	4.987	1204	1212	1215	rBV2	1748	2220	0.12%	0.015%
23	5.100	1237	1247	1254	rBV2	1285	2722	0.15%	0.019%
24	5.154	1260	1264	1269	rVB	1992	1533	0.09%	0.011%
25	5.180	1269	1272	1278	rBV3	1012	1039	0.06%	0.007%
26	5.338	1298	1321	1349	rBV2	609094	1797407	100.00%	12.440%
27	5.884	1478	1491	1517	rVV	543324	1102819	61.36%	7.633%
28	6.103	1557	1559	1565	rVB3	2105	2098	0.12%	0.015%
29	6.328	1614	1629	1654	rBV	388730	798753	44.44%	5.528%
30	6.505	1681	1684	1686	rBV	1705	1234	0.07%	0.009%
31	6.575	1703	1706	1711	rBV2	1185	989	0.06%	0.007%
32	6.752	1758	1761	1767	rBV	882	928	0.05%	0.006%
33	6.891	1801	1804	1812	rVB2	1344	1583	0.09%	0.011%
34	6.926	1812	1815	1818	rBV	1627	1150	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030296.D
 Acq On : 22 Mar 2019 10:33
 Operator : JC/SP
 Sample : VU0322WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.022	1840	1845	1849	rVB	1604	1676	0.09%	0.012%
36	7.128	1872	1878	1880	rBV2	1394	1125	0.06%	0.008%
37	7.173	1885	1892	1894	rBV	1650	1985	0.11%	0.014%
38	7.225	1896	1908	1936	rBV	218303	406718	22.63%	2.815%
39	7.466	1975	1983	1997	rVB6	5282	11899	0.66%	0.082%
40	7.563	1998	2013	2047	rBV	813183	1467713	81.66%	10.158%
41	7.849	2091	2102	2126	rBV	147871	268895	14.96%	1.861%
42	8.026	2154	2157	2162	rBV	1467	1211	0.07%	0.008%
43	8.077	2170	2173	2177	rVB2	1848	1427	0.08%	0.010%
44	8.096	2177	2179	2185	rBV2	1207	1031	0.06%	0.007%
45	8.135	2185	2191	2193	rBV	1155	1117	0.06%	0.008%
46	8.308	2229	2245	2284	rBV	571707	1058153	58.87%	7.324%
47	8.588	2329	2332	2341	rVB3	2189	2449	0.14%	0.017%
48	8.717	2370	2372	2378	rVB	1115	979	0.05%	0.007%
49	8.894	2422	2427	2435	rBV2	968	1448	0.08%	0.010%
50	9.087	2474	2487	2527	rVV	798701	1368719	76.15%	9.473%
51	9.334	2557	2564	2569	rBV	1411	1799	0.10%	0.012%
52	9.376	2573	2577	2585	rVV4	1794	2178	0.12%	0.015%
53	9.437	2594	2596	2602	rVB	1292	968	0.05%	0.007%
54	9.476	2602	2608	2609	rBV	1082	1021	0.06%	0.007%
55	9.585	2640	2642	2649	rVB	1034	980	0.05%	0.007%
56	9.624	2650	2654	2657	rBV	1792	1471	0.08%	0.010%
57	9.665	2664	2667	2673	rVB2	1095	1025	0.06%	0.007%
58	9.736	2684	2689	2691	rBV2	1036	945	0.05%	0.007%
59	9.878	2728	2733	2738	rBV2	1368	1561	0.09%	0.011%
60	9.971	2758	2762	2765	rBV3	1203	1163	0.06%	0.008%
61	9.987	2765	2767	2770	rVV	1581	1127	0.06%	0.008%
62	10.029	2775	2780	2785	rVV	1986	2571	0.14%	0.018%
63	10.087	2794	2798	2803	rVB2	1813	1697	0.09%	0.012%
64	10.122	2803	2809	2817	rBV	2267	3894	0.22%	0.027%
65	10.173	2817	2825	2833	rVV4	3242	4855	0.27%	0.034%
66	10.260	2848	2852	2855	rBV	2203	1815	0.10%	0.013%
67	10.315	2860	2869	2871	rBV3	1744	2100	0.12%	0.015%
68	10.427	2889	2904	2920	rBV	603620	985545	54.83%	6.821%
69	10.607	2957	2960	2963	rVB2	1806	1040	0.06%	0.007%
70	10.665	2975	2978	2981	rBV	1338	1204	0.07%	0.008%
71	10.717	2990	2994	2997	rBV	1113	974	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030296.D
 Acq On : 22 Mar 2019 10:33
 Operator : JC/SP
 Sample : VU0322WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.816	3023	3025	3028	rVB	2035	1177	0.07%	0.008%
73	10.852	3033	3036	3039	rBV	1659	1269	0.07%	0.009%
74	11.003	3080	3083	3088	rBV2	1156	1348	0.07%	0.009%
75	11.096	3106	3112	3115	rBV	1947	2109	0.12%	0.015%
76	11.119	3115	3119	3125	rVB	1764	1882	0.10%	0.013%
77	11.283	3165	3170	3173	rBV	2029	1838	0.10%	0.013%
78	11.363	3191	3195	3200	rBV	1250	1169	0.07%	0.008%
79	11.421	3208	3213	3220	rBV5	5122	6449	0.36%	0.045%
80	11.482	3220	3232	3257	rBV	780305	1286048	71.55%	8.901%
81	11.627	3275	3277	3281	rVB	1584	1035	0.06%	0.007%
82	11.858	3336	3349	3372	rBV	790276	1337740	74.43%	9.259%
83	12.045	3404	3407	3414	rVB2	1874	1924	0.11%	0.013%
84	12.894	3662	3671	3688	rBV3	8062	16836	0.94%	0.117%
85	12.967	3688	3694	3697	rBV2	1728	1716	0.10%	0.012%
86	13.299	3792	3797	3800	rBV2	1139	1273	0.07%	0.009%
87	13.376	3817	3821	3824	rBV	1543	1403	0.08%	0.010%
88	13.466	3842	3849	3850	rBV	1345	1520	0.08%	0.011%
89	13.511	3855	3863	3873	rBV5	10608	18823	1.05%	0.130%
90	13.672	3910	3913	3917	rBV	1319	1060	0.06%	0.007%
91	13.749	3927	3937	3953	rBV	24216	57842	3.22%	0.400%
92	13.993	4004	4013	4033	rVB7	12678	27892	1.55%	0.193%
93	14.212	4078	4081	4084	rBV2	1303	1126	0.06%	0.008%
94	14.279	4096	4102	4105	rBV3	1811	1939	0.11%	0.013%
95	14.398	4133	4139	4143	rVB2	1509	2050	0.11%	0.014%
96	14.450	4153	4155	4161	rBV2	1032	1125	0.06%	0.008%
97	14.508	4170	4173	4181	rVB2	1498	1560	0.09%	0.011%
98	14.556	4185	4188	4191	rBV	1343	923	0.05%	0.006%
99	15.057	4341	4344	4346	rBV	1453	1175	0.07%	0.008%
100	15.762	4559	4563	4565	rBV3	1587	1372	0.08%	0.009%


Sum of corrected areas: 14448298

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030296.D
Acq On : 22 Mar 2019 10:33
Operator : JC/SP
Sample : VU0322WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

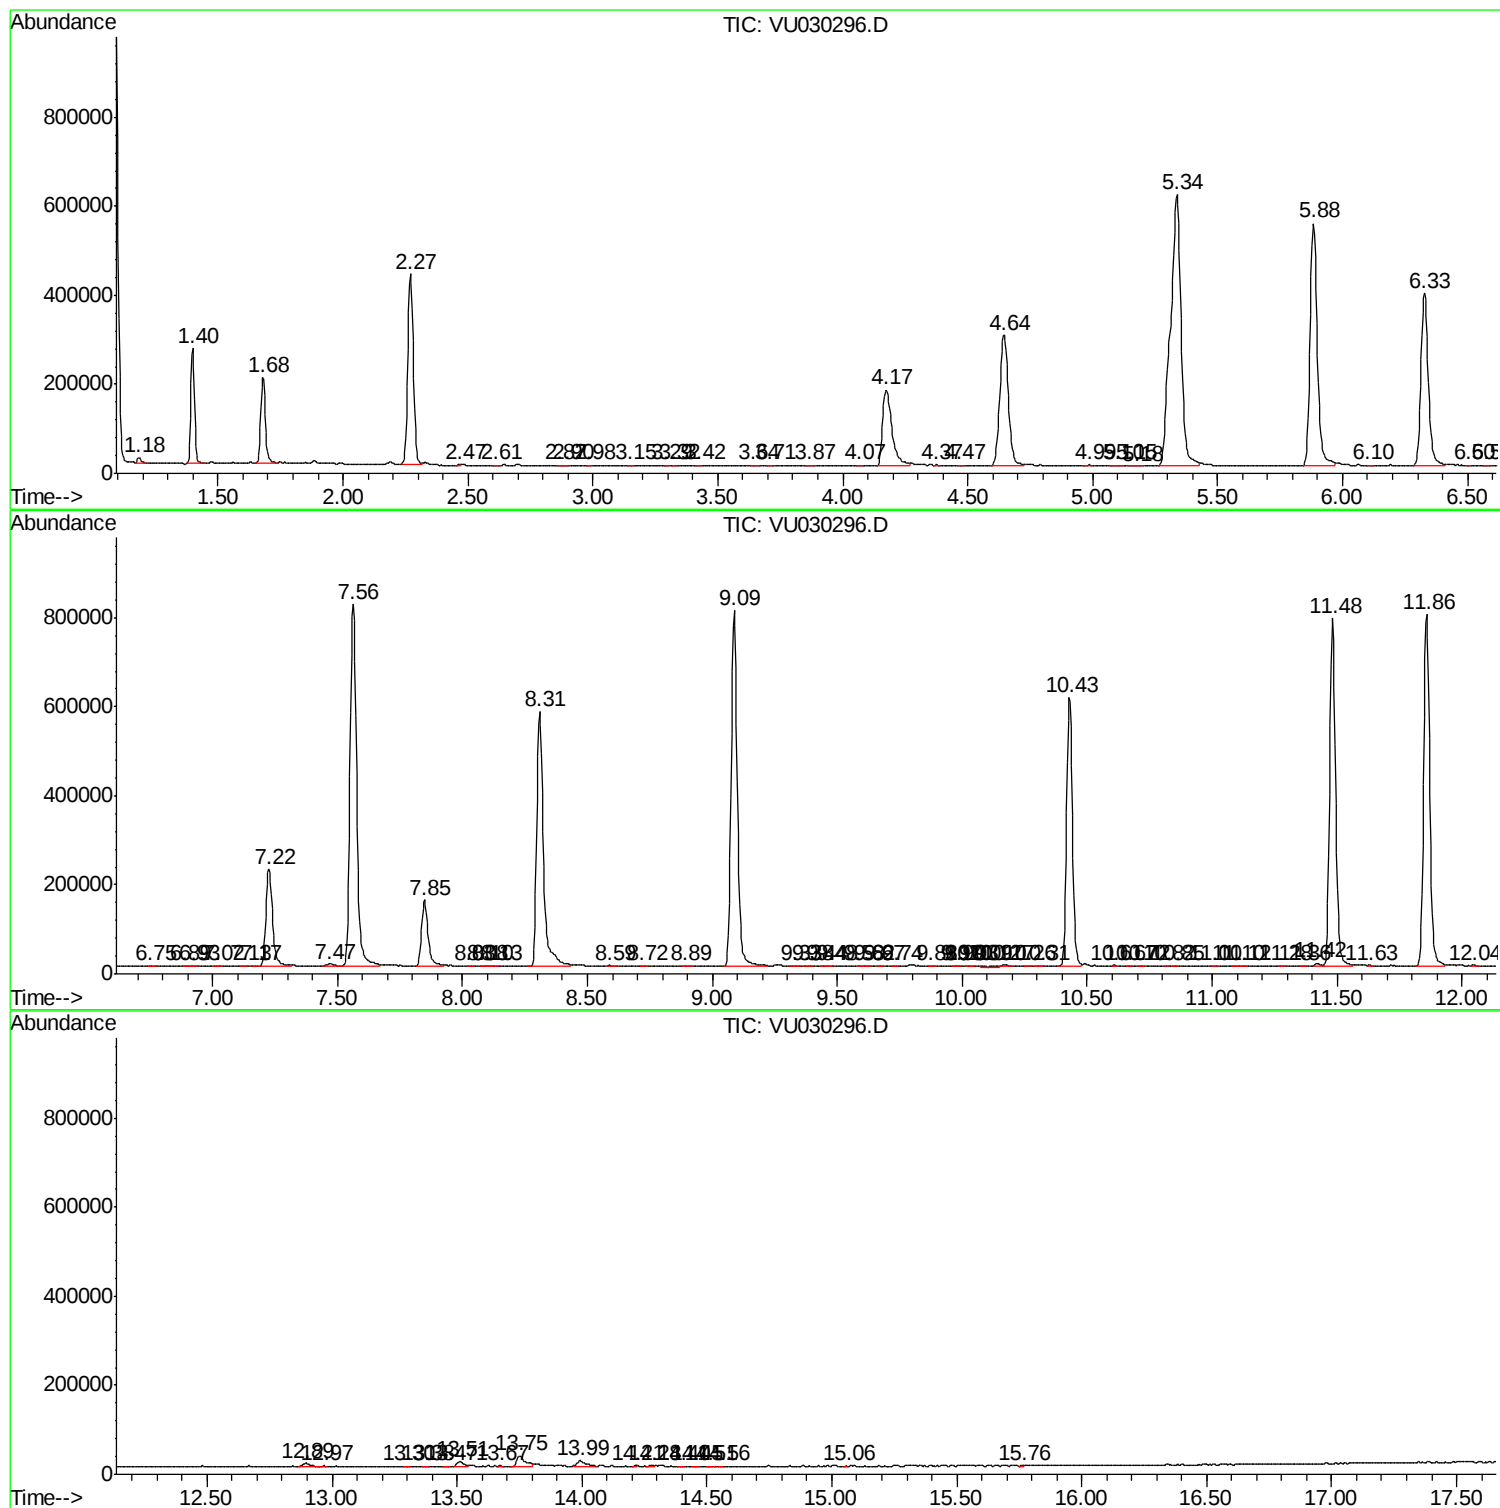

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030296.D
Acq On : 22 Mar 2019 10:33
Operator : JC/SP
Sample : VU0322WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030296.D
Acq On : 22 Mar 2019 10:33
Operator : JC/SP
Sample : VU0322WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc