

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030300.D
 Acq On : 22 Mar 2019 12:04
 Operator : JC/SP
 Sample : K2022-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0992

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rBV2	12020	11226	0.66%	0.081%
2	1.399	89	96	111	rVB	238645	233628	13.82%	1.680%
3	1.679	175	183	199	rBV	179822	229643	13.59%	1.651%
4	2.058	298	301	307	rBV4	2136	2557	0.15%	0.018%
5	2.106	313	316	318	rBV2	2050	1365	0.08%	0.010%
6	2.270	356	367	378	rBV	392139	592566	35.06%	4.260%
7	2.447	413	422	438	rVB2	18771	35777	2.12%	0.257%
8	2.527	444	447	451	rBV2	1252	1057	0.06%	0.008%
9	2.556	451	456	461	rBV	1321	1475	0.09%	0.011%
10	2.617	470	475	478	rBV	1313	1455	0.09%	0.010%
11	2.675	490	493	497	rBV	1133	1077	0.06%	0.008%
12	2.701	497	501	506	rVB3	1544	1481	0.09%	0.011%
13	2.727	506	509	514	rVB	1396	1046	0.06%	0.008%
14	2.756	514	518	521	rBV	1379	1088	0.06%	0.008%
15	2.952	576	579	585	rVB	1611	1317	0.08%	0.009%
16	3.035	601	605	612	rVB	2230	2080	0.12%	0.015%
17	3.084	617	620	623	rVV	1623	968	0.06%	0.007%
18	3.103	624	626	632	rVB2	1048	1056	0.06%	0.008%
19	3.280	679	681	685	rVB	1460	1032	0.06%	0.007%
20	3.379	708	712	717	rBV2	1171	1063	0.06%	0.008%
21	3.408	718	721	726	rVB	1800	1561	0.09%	0.011%
22	3.437	726	730	732	rBV	1635	1110	0.07%	0.008%
23	3.650	792	796	800	rBV	1960	2046	0.12%	0.015%
24	3.794	834	841	848	rVB2	1428	1928	0.11%	0.014%
25	3.952	883	890	893	rBV2	1371	1565	0.09%	0.011%
26	4.113	934	940	947	rBV2	1588	2663	0.16%	0.019%
27	4.177	947	960	989	rBV	166773	445873	26.38%	3.205%
28	4.646	1088	1106	1130	rBV	286775	680025	40.23%	4.889%
29	4.977	1206	1209	1215	rVV	1097	1124	0.07%	0.008%
30	5.167	1264	1268	1272	rBV2	1176	1105	0.07%	0.008%
31	5.338	1298	1321	1341	rBV2	579058	1690375	100.00%	12.152%
32	5.614	1404	1407	1410	rBV	1614	1221	0.07%	0.009%
33	5.884	1478	1491	1520	rBV	557556	1124834	66.54%	8.086%
34	6.100	1554	1558	1560	rBV	1641	1079	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030300.D
 Acq On : 22 Mar 2019 12:04
 Operator : JC/SP
 Sample : K2022-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0992

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1615	1629	1655	rBV	374046	763463	45.17%	5.488%
36	6.659	1725	1732	1734	rBV	1691	1794	0.11%	0.013%
37	6.707	1744	1747	1750	rVB	1743	1144	0.07%	0.008%
38	6.743	1755	1758	1765	rBV	1908	1846	0.11%	0.013%
39	6.900	1801	1807	1812	rVB	1337	1669	0.10%	0.012%
40	7.225	1894	1908	1934	rBV	202945	387361	22.92%	2.785%
41	7.479	1982	1987	1991	rVB2	1472	1505	0.09%	0.011%
42	7.563	2000	2013	2037	rBV	775889	1375141	81.35%	9.886%
43	7.736	2062	2067	2069	rBV3	1024	1055	0.06%	0.008%
44	7.849	2087	2102	2123	rBV2	142494	263493	15.59%	1.894%
45	7.974	2139	2141	2149	rVB	2314	2391	0.14%	0.017%
46	8.010	2149	2152	2156	rBV	1991	1829	0.11%	0.013%
47	8.135	2186	2191	2195	rBV2	1613	1865	0.11%	0.013%
48	8.174	2196	2203	2217	rVB4	5047	9854	0.58%	0.071%
49	8.309	2234	2245	2278	rBV	556477	1025984	60.70%	7.376%
50	8.556	2320	2322	2328	rVB2	1549	1140	0.07%	0.008%
51	8.588	2329	2332	2335	rVB	1354	961	0.06%	0.007%
52	8.627	2340	2344	2347	rVB	1228	957	0.06%	0.007%
53	8.720	2368	2373	2377	rVB2	1204	1126	0.07%	0.008%
54	8.752	2377	2383	2385	rBV2	1248	1253	0.07%	0.009%
55	8.839	2407	2410	2414	rVB	1853	1185	0.07%	0.009%
56	8.903	2425	2430	2433	rBV2	990	991	0.06%	0.007%
57	9.087	2474	2487	2518	rBV	824051	1392980	82.41%	10.014%
58	9.292	2548	2551	2554	rBV	1507	1121	0.07%	0.008%
59	9.382	2575	2579	2582	rBV	1738	1360	0.08%	0.010%
60	9.444	2596	2598	2603	rVB	1194	1018	0.06%	0.007%
61	9.665	2663	2667	2671	rBV2	1537	1655	0.10%	0.012%
62	9.743	2687	2691	2694	rVV	1459	1217	0.07%	0.009%
63	9.765	2694	2698	2702	rVB	987	957	0.06%	0.007%
64	9.849	2718	2724	2729	rBV3	1461	1753	0.10%	0.013%
65	9.890	2729	2737	2740	rBV	1138	1599	0.09%	0.011%
66	10.122	2803	2809	2813	rBV	1967	2273	0.13%	0.016%
67	10.328	2868	2873	2882	rBV	1950	3148	0.19%	0.023%
68	10.370	2883	2886	2892	rVB2	1289	1019	0.06%	0.007%
69	10.427	2892	2904	2925	rBV	585645	953745	56.42%	6.856%
70	10.601	2952	2958	2966	rVV3	3144	5567	0.33%	0.040%
71	10.691	2982	2986	2991	rBV	913	1044	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030300.D
 Acq On : 22 Mar 2019 12:04
 Operator : JC/SP
 Sample : K2022-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0992

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.746	2997	3003	3009	rBV	2341	2655	0.16%	0.019%
73	10.855	3030	3037	3044	rBV2	1596	2346	0.14%	0.017%
74	11.016	3080	3087	3090	rBV	1153	1651	0.10%	0.012%
75	11.154	3128	3130	3135	rVB	1844	1286	0.08%	0.009%
76	11.180	3135	3138	3140	rBV	1661	1183	0.07%	0.009%
77	11.299	3168	3175	3178	rBV3	1492	1398	0.08%	0.010%
78	11.347	3187	3190	3195	rBV	1238	963	0.06%	0.007%
79	11.482	3219	3232	3253	rBV	786462	1295151	76.62%	9.311%
80	11.672	3287	3291	3296	rVB2	1740	1668	0.10%	0.012%
81	11.701	3296	3300	3304	rBV	2149	1861	0.11%	0.013%
82	11.858	3336	3349	3371	rBV	756773	1272208	75.26%	9.146%
83	12.003	3391	3394	3398	rVB2	1419	957	0.06%	0.007%
84	12.119	3427	3430	3433	rVB	1483	968	0.06%	0.007%
85	12.267	3471	3476	3478	rBV	1220	1093	0.06%	0.008%
86	12.357	3501	3504	3508	rVV2	1032	943	0.06%	0.007%
87	12.521	3552	3555	3559	rVB	2072	1578	0.09%	0.011%
88	12.550	3560	3564	3567	rBV	1270	1005	0.06%	0.007%
89	12.623	3583	3587	3591	rBV2	1312	1201	0.07%	0.009%
90	12.948	3685	3688	3692	rVB	1495	1055	0.06%	0.008%
91	13.148	3745	3750	3753	rBV2	1215	1153	0.07%	0.008%
92	13.193	3761	3764	3767	rVB	1708	1133	0.07%	0.008%
93	13.222	3767	3773	3777	rBV2	1407	2113	0.13%	0.015%
94	13.263	3781	3786	3795	rBV	1827	2662	0.16%	0.019%
95	13.437	3837	3840	3845	rBV2	1282	1079	0.06%	0.008%
96	13.521	3860	3866	3871	rBV3	2214	3275	0.19%	0.024%
97	13.688	3913	3918	3921	rBV2	1459	1254	0.07%	0.009%
98	14.128	4047	4055	4057	rBV2	1481	2041	0.12%	0.015%
99	14.276	4097	4101	4111	rVB3	3044	4696	0.28%	0.034%
100	14.424	4142	4147	4154	rBV2	1251	1930	0.11%	0.014%


Sum of corrected areas: 13910435

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030300.D
Acq On : 22 Mar 2019 12:04
Operator : JC/SP
Sample : K2022-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0992

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

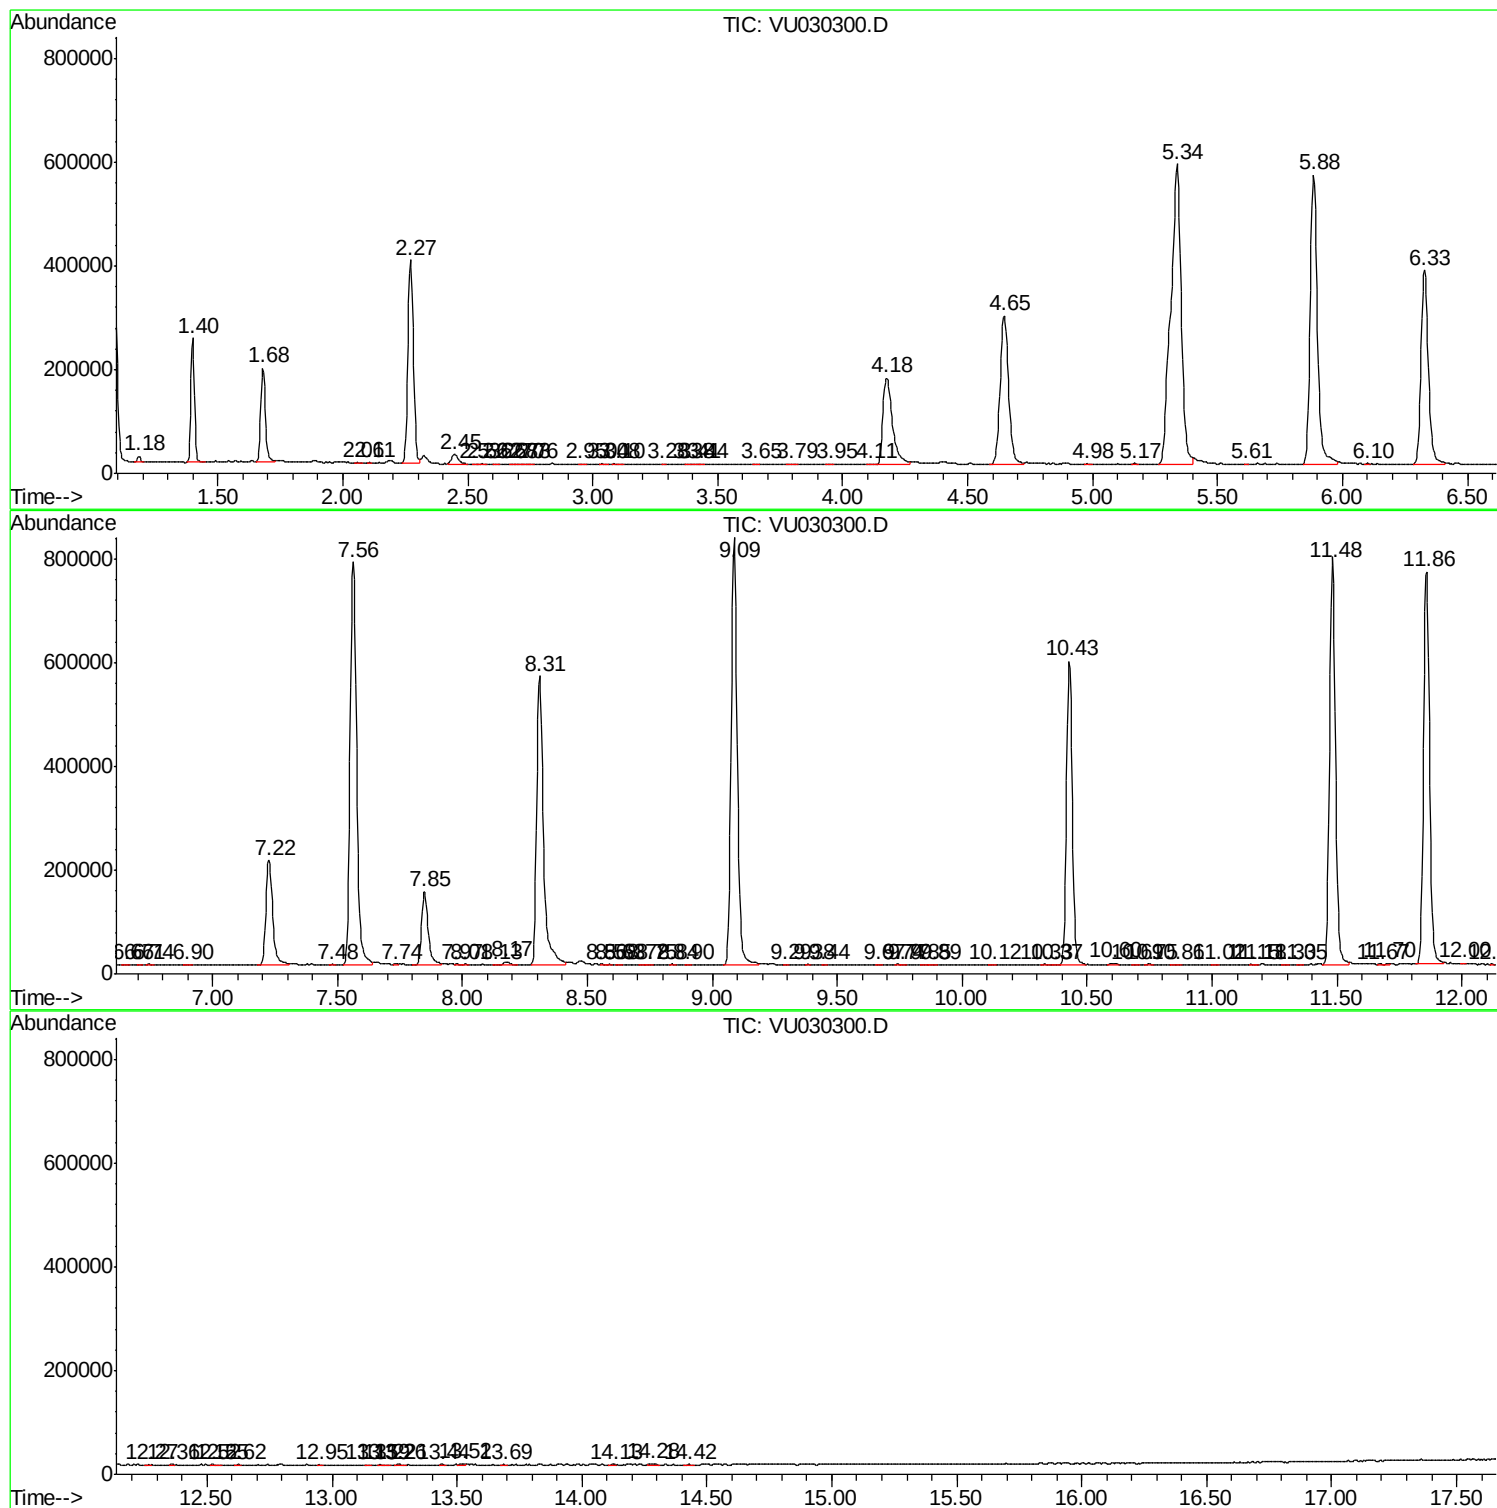

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030300.D
Acq On : 22 Mar 2019 12:04
Operator : JC/SP
Sample : K2022-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0992

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030300.D
Acq On : 22 Mar 2019 12:04
Operator : JC/SP
Sample : K2022-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0992

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc