

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030301.D
 Acq On : 22 Mar 2019 12:27
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	11689	10147	0.60%	0.072%
2	1.399	89	96	109	rVB	242392	236085	13.89%	1.680%
3	1.678	176	183	198	rVB	180128	229079	13.48%	1.630%
4	2.186	336	341	348	rVB6	4983	6907	0.41%	0.049%
5	2.270	356	367	379	rBV	389905	597356	35.14%	4.251%
6	2.447	413	422	437	rVB2	6652	13201	0.78%	0.094%
7	2.592	463	467	473	rVB	2071	2195	0.13%	0.016%
8	2.675	487	493	495	rBV2	1537	1237	0.07%	0.009%
9	2.727	506	509	513	rVB	1414	964	0.06%	0.007%
10	2.839	528	544	561	rVB	33683	76335	4.49%	0.543%
11	2.910	561	566	569	rVB2	964	958	0.06%	0.007%
12	3.019	596	600	604	rVB	1281	1161	0.07%	0.008%
13	3.344	695	701	705	rVB2	1310	1421	0.08%	0.010%
14	3.440	725	731	739	rVB	1494	2090	0.12%	0.015%
15	3.476	739	742	749	rBV	1997	2506	0.15%	0.018%
16	3.572	769	772	776	rBV	1173	1179	0.07%	0.008%
17	3.630	787	790	798	rVB	843	1113	0.07%	0.008%
18	3.997	899	904	907	rVB	1554	1431	0.08%	0.010%
19	4.019	907	911	915	rBV	1647	1743	0.10%	0.012%
20	4.087	926	932	937	rBV	1492	2082	0.12%	0.015%
21	4.177	944	960	985	rBV2	183187	521386	30.67%	3.710%
22	4.556	1074	1078	1082	rBV	2055	1579	0.09%	0.011%
23	4.646	1088	1106	1130	rBV	281869	675246	39.73%	4.805%
24	4.929	1190	1194	1197	rBV	1138	1177	0.07%	0.008%
25	4.987	1209	1212	1218	rBV2	1547	1272	0.07%	0.009%
26	5.029	1222	1225	1231	rVB	1446	1330	0.08%	0.009%
27	5.170	1265	1269	1271	rBV	1713	1451	0.09%	0.010%
28	5.337	1298	1321	1344	rBV2	585398	1699719	100.00%	12.095%
29	5.826	1468	1473	1477	rBV	942	1076	0.06%	0.008%
30	5.884	1477	1491	1528	rVV	557488	1142388	67.21%	8.129%
31	6.148	1570	1573	1577	rBV2	1186	992	0.06%	0.007%
32	6.328	1612	1629	1652	rBV	376394	764260	44.96%	5.438%
33	6.534	1691	1693	1700	rVB	1050	983	0.06%	0.007%
34	6.714	1746	1749	1757	rVB3	1236	1601	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030301.D
 Acq On : 22 Mar 2019 12:27
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.749	1757	1760	1764	rBV	1265	1206	0.07%	0.009%
36	6.768	1764	1766	1773	rVB	1204	1138	0.07%	0.008%
37	6.855	1789	1793	1796	rVB	1060	926	0.05%	0.007%
38	6.878	1796	1800	1804	rBV	1425	1624	0.10%	0.012%
39	6.939	1816	1819	1822	rBV	1084	867	0.05%	0.006%
40	6.974	1827	1830	1835	rVB2	1398	1154	0.07%	0.008%
41	7.087	1862	1865	1868	rBV	1467	924	0.05%	0.007%
42	7.225	1896	1908	1930	rBV	206152	382744	22.52%	2.723%
43	7.434	1970	1973	1982	rBV3	1460	1633	0.10%	0.012%
44	7.562	2000	2013	2045	rBV	781008	1397677	82.23%	9.945%
45	7.736	2064	2067	2071	rBV	1842	1194	0.07%	0.008%
46	7.849	2089	2102	2122	rBV	141437	255174	15.01%	1.816%
47	7.984	2140	2144	2146	rBV	1454	1345	0.08%	0.010%
48	8.177	2191	2204	2215	rVV2	13555	23223	1.37%	0.165%
49	8.231	2218	2221	2226	rVB2	1425	921	0.05%	0.007%
50	8.308	2231	2245	2280	rBV	533080	985595	57.99%	7.013%
51	8.636	2343	2347	2352	rVB2	1284	1330	0.08%	0.009%
52	8.704	2364	2368	2373	rVB	1132	943	0.06%	0.007%
53	8.733	2373	2377	2381	rVB2	1227	889	0.05%	0.006%
54	8.775	2386	2390	2393	rBV	1128	955	0.06%	0.007%
55	8.919	2430	2435	2439	rVB	1655	1867	0.11%	0.013%
56	8.945	2439	2443	2447	rBV	1903	1767	0.10%	0.013%
57	8.984	2448	2455	2460	rVB	1567	1710	0.10%	0.012%
58	9.086	2470	2487	2517	rBV	840693	1415359	83.27%	10.071%
59	9.450	2597	2600	2605	rVB	1590	1333	0.08%	0.009%
60	9.543	2626	2629	2633	rVB	1509	1172	0.07%	0.008%
61	9.762	2691	2697	2702	rVB	914	1025	0.06%	0.007%
62	9.807	2708	2711	2715	rVB	1301	877	0.05%	0.006%
63	9.910	2739	2743	2747	rVB2	1336	989	0.06%	0.007%
64	9.993	2765	2769	2776	rBV2	1360	1900	0.11%	0.014%
65	10.106	2800	2804	2811	rBV	1284	1626	0.10%	0.012%
66	10.141	2811	2815	2818	rBV2	1311	1074	0.06%	0.008%
67	10.170	2818	2824	2829	rBV3	1639	1809	0.11%	0.013%
68	10.385	2887	2891	2893	rBV	1249	1024	0.06%	0.007%
69	10.427	2893	2904	2931	rVB	582611	948195	55.79%	6.747%
70	10.527	2931	2935	2937	rBV2	1290	985	0.06%	0.007%
71	10.607	2946	2960	2977	rBV3	12271	24984	1.47%	0.178%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030301.D
 Acq On : 22 Mar 2019 12:27
 Operator : JC/SP
 Sample : K2022-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0995

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.820	3022	3026	3031	rVB2	1054	1148	0.07%	0.008%
73	10.845	3031	3034	3037	rBV2	1346	910	0.05%	0.006%
74	10.865	3037	3040	3045	rVB	1488	1227	0.07%	0.009%
75	10.926	3057	3059	3064	rVB	1483	1042	0.06%	0.007%
76	10.961	3064	3070	3072	rBV	1217	1488	0.09%	0.011%
77	11.051	3095	3098	3103	rVV	964	965	0.06%	0.007%
78	11.128	3118	3122	3125	rBV	1212	1244	0.07%	0.009%
79	11.209	3143	3147	3151	rVV2	1010	873	0.05%	0.006%
80	11.414	3208	3211	3213	rBV	1780	1432	0.08%	0.010%
81	11.482	3219	3232	3250	rBV	789647	1286437	75.69%	9.154%
82	11.791	3325	3328	3332	rBV	1236	1051	0.06%	0.007%
83	11.858	3336	3349	3373	rBV	764842	1259101	74.08%	8.959%
84	12.138	3431	3436	3439	rBV2	2005	1903	0.11%	0.014%
85	12.273	3474	3478	3481	rVB	1300	996	0.06%	0.007%
86	12.405	3516	3519	3522	rBV	1239	896	0.05%	0.006%
87	12.443	3525	3531	3533	rBV3	979	1001	0.06%	0.007%
88	12.707	3609	3613	3615	rBV2	1538	1184	0.07%	0.008%
89	12.948	3684	3688	3693	rBV	1249	1289	0.08%	0.009%
90	13.189	3759	3763	3767	rBV2	1416	1121	0.07%	0.008%
91	13.282	3789	3792	3801	rVB3	2051	2183	0.13%	0.016%
92	13.321	3801	3804	3807	rBV	2102	1431	0.08%	0.010%
93	13.623	3895	3898	3903	rBV2	982	904	0.05%	0.006%
94	14.421	4143	4146	4152	rVB	2101	1733	0.10%	0.012%
95	14.450	4152	4155	4160	rVB2	2246	1612	0.09%	0.011%
96	14.662	4218	4221	4225	rBV3	1238	998	0.06%	0.007%
97	14.716	4230	4238	4243	rBV2	1949	3155	0.19%	0.022%
98	14.864	4281	4284	4287	rBV	1134	1145	0.07%	0.008%
99	15.038	4335	4338	4345	rVB2	993	1091	0.06%	0.008%
100	15.479	4472	4475	4476	rBV	1999	1159	0.07%	0.008%


Sum of corrected areas: 14053527

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030301.D
Acq On : 22 Mar 2019 12:27
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

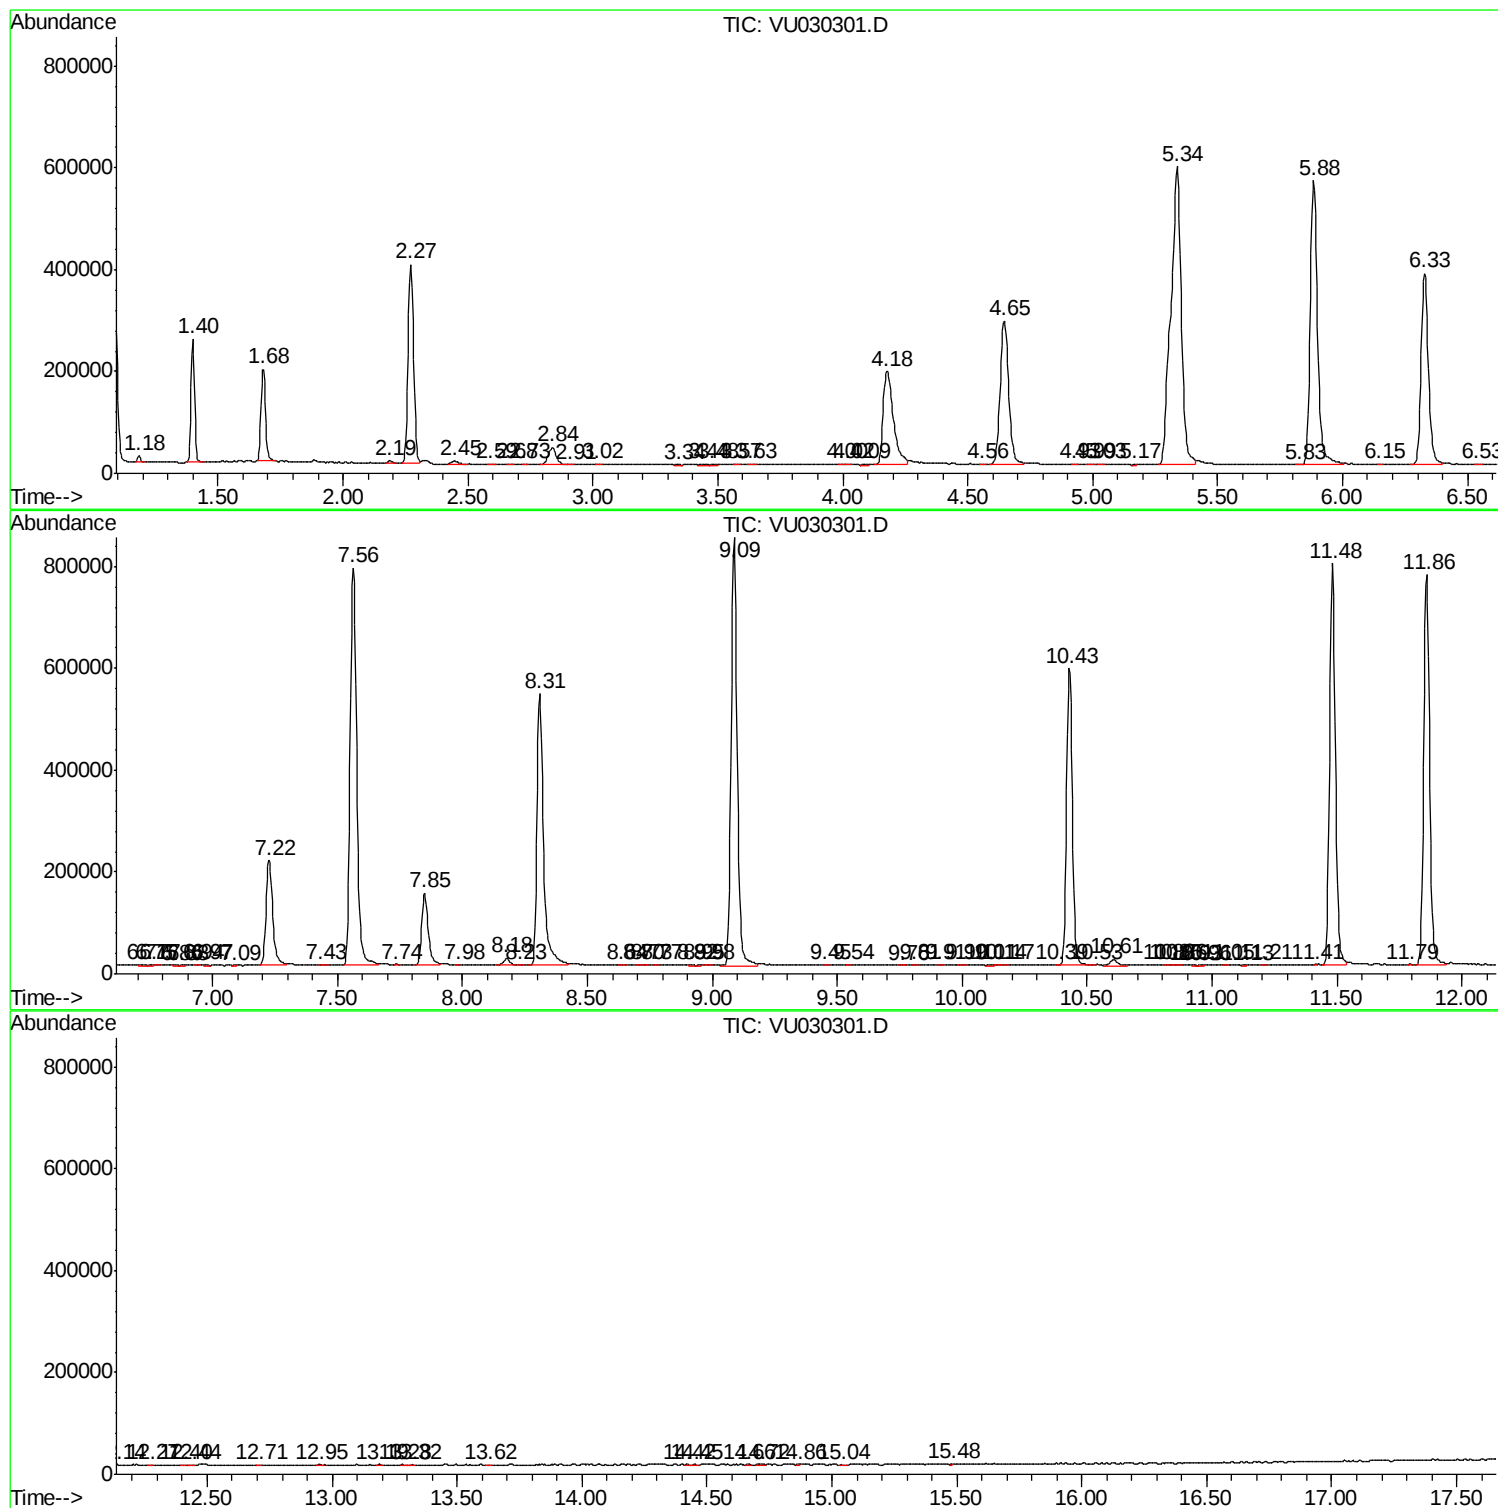

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030301.D
Acq On : 22 Mar 2019 12:27
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030301.D
Acq On : 22 Mar 2019 12:27
Operator : JC/SP
Sample : K2022-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0995

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc