

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032219\
 Data File : VU030302.D
 Acq On : 22 Mar 2019 12:50
 Operator : JC/SP
 Sample : K2022-08DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	35	rVB2	10913	9917	0.34%	0.058%
2	1.399	89	96	105	rBV	226874	225703	7.81%	1.320%
3	1.678	176	183	201	rVB	177202	224328	7.76%	1.312%
4	2.270	356	367	380	rBV	369469	572029	19.80%	3.345%
5	2.411	407	411	416	rBV2	1350	1160	0.04%	0.007%
6	2.447	416	422	429	rBV3	1816	3309	0.11%	0.019%
7	2.691	494	498	499	rBV	1513	1031	0.04%	0.006%
8	2.829	536	541	543	rBV3	1666	1539	0.05%	0.009%
9	3.202	654	657	662	rVV2	1109	1083	0.04%	0.006%
10	3.254	669	673	676	rBV	1506	1245	0.04%	0.007%
11	3.421	721	725	727	rVV	1118	929	0.03%	0.005%
12	3.482	739	744	746	rBV	1473	1560	0.05%	0.009%
13	3.553	763	766	770	rBV3	1246	1022	0.04%	0.006%
14	3.858	855	861	866	rBV	976	1398	0.05%	0.008%
15	3.942	879	887	892	rVB	1393	1927	0.07%	0.011%
16	3.968	892	895	899	rBV	1383	1022	0.04%	0.006%
17	4.096	929	935	940	rBV	1448	2337	0.08%	0.014%
18	4.177	948	960	996	rBV	157788	426977	14.78%	2.496%
19	4.489	1053	1057	1061	rBV2	1200	1208	0.04%	0.007%
20	4.546	1071	1075	1080	rBV	1306	1328	0.05%	0.008%
21	4.646	1089	1106	1128	rBV	277026	656946	22.74%	3.841%
22	4.900	1182	1185	1188	rVB	2185	1489	0.05%	0.009%
23	4.997	1207	1215	1218	rVB2	1406	1833	0.06%	0.011%
24	5.016	1218	1221	1225	rVB	1304	925	0.03%	0.005%
25	5.067	1231	1237	1239	rVB3	1058	961	0.03%	0.006%
26	5.337	1293	1321	1358	rBV2	566532	1677352	58.05%	9.807%
27	5.556	1385	1389	1392	rBV	1171	941	0.03%	0.006%
28	5.749	1446	1449	1453	rBV	1330	929	0.03%	0.005%
29	5.800	1460	1465	1471	rVB	1265	1348	0.05%	0.008%
30	5.884	1477	1491	1519	rBV	562081	1140654	39.48%	6.669%
31	6.254	1603	1606	1611	rBV2	1287	1394	0.05%	0.008%
32	6.328	1614	1629	1651	rBV	368045	745201	25.79%	4.357%
33	6.669	1730	1735	1740	rBV	996	1300	0.04%	0.008%
34	6.987	1829	1834	1839	rBV	1070	1213	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032219\
 Data File : VU030302.D
 Acq On : 22 Mar 2019 12:50
 Operator : JC/SP
 Sample : K2022-08DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.109	1867	1872	1877	rBV	1416	1380	0.05%	0.008%
36	7.225	1896	1908	1932	rBV	202251	378672	13.11%	2.214%
37	7.421	1966	1969	1973	rBV3	1711	1566	0.05%	0.009%
38	7.562	2000	2013	2037	rBV	764123	1350484	46.74%	7.896%
39	7.849	2091	2102	2122	rBV	140966	251358	8.70%	1.470%
40	8.173	2197	2203	2211	rBV5	4583	7893	0.27%	0.046%
41	8.250	2221	2227	2232	rBV2	1112	1172	0.04%	0.007%
42	8.308	2234	2245	2271	rBV	538108	972493	33.66%	5.686%
43	8.852	2410	2414	2418	rBV	1618	1801	0.06%	0.011%
44	9.086	2474	2487	2517	rBV2	869589	1936073	67.01%	11.320%
45	9.260	2539	2541	2547	rVB2	1441	1134	0.04%	0.007%
46	9.450	2597	2600	2604	rBV	1572	1269	0.04%	0.007%
47	9.791	2702	2706	2710	rBV	1894	2003	0.07%	0.012%
48	10.029	2774	2780	2784	rBV	1686	1847	0.06%	0.011%
49	10.112	2803	2806	2810	rBV	1399	1213	0.04%	0.007%
50	10.193	2828	2831	2835	rVB	2050	1421	0.05%	0.008%
51	10.225	2835	2841	2844	rBV	1243	1558	0.05%	0.009%
52	10.292	2855	2862	2865	rBV2	861	1161	0.04%	0.007%
53	10.427	2893	2904	2925	rBV	581332	941195	32.57%	5.503%
54	10.607	2952	2960	2970	rVB4	5425	8932	0.31%	0.052%
55	10.688	2977	2985	2988	rBV	2130	3346	0.12%	0.020%
56	10.723	2993	2996	3001	rBV	1394	1566	0.05%	0.009%
57	10.775	3007	3012	3015	rBV	1245	1232	0.04%	0.007%
58	10.942	3058	3064	3068	rBV	1170	1566	0.05%	0.009%
59	11.048	3093	3097	3099	rBV	1171	922	0.03%	0.005%
60	11.418	3202	3212	3221	rVV	50916	81430	2.82%	0.476%
61	11.482	3221	3232	3265	rVB2	886111	1929591	66.78%	11.282%
62	11.694	3293	3298	3303	rBV	1430	1444	0.05%	0.008%
63	11.781	3320	3325	3329	rVB	1677	1766	0.06%	0.010%
64	11.871	3336	3353	3389	rVV2	1195086	2889414	100.00%	16.894%
65	12.118	3424	3430	3433	rBV	1937	2232	0.08%	0.013%
66	12.373	3505	3509	3511	rBV	1507	1103	0.04%	0.006%
67	12.475	3532	3541	3543	rBV3	1852	2024	0.07%	0.012%
68	12.488	3543	3545	3549	rVV2	2572	1816	0.06%	0.011%
69	12.517	3549	3554	3559	rVV	1047	1437	0.05%	0.008%
70	12.556	3563	3566	3569	rVB	1631	1032	0.04%	0.006%
71	12.617	3579	3585	3589	rBV2	1750	2210	0.08%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032219\
 Data File : VU030302.D
 Acq On : 22 Mar 2019 12:50
 Operator : JC/SP
 Sample : K2022-08DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	12.649	3589	3595	3602	rVV2	1875	2901	0.10%	0.017%
73	12.691	3602	3608	3613	rVB2	1594	2169	0.08%	0.013%
74	12.755	3624	3628	3630	rBV	1438	1060	0.04%	0.006%
75	12.951	3686	3689	3696	rVB2	1568	1888	0.07%	0.011%
76	12.983	3696	3699	3707	rBV	2033	2342	0.08%	0.014%
77	13.019	3707	3710	3713	rBV	1126	976	0.03%	0.006%
78	13.138	3743	3747	3750	rBV2	1342	1107	0.04%	0.006%
79	13.208	3763	3769	3773	rVB	1758	2174	0.08%	0.013%
80	13.241	3773	3779	3786	rBV	1729	2593	0.09%	0.015%
81	13.299	3791	3797	3799	rBV2	1271	1427	0.05%	0.008%
82	13.360	3810	3816	3819	rBV	1464	1658	0.06%	0.010%
83	13.405	3828	3830	3836	rVB3	1257	1128	0.04%	0.007%
84	13.437	3838	3840	3845	rVB	1510	993	0.03%	0.006%
85	13.501	3849	3860	3898	rBV	242203	475524	16.46%	2.780%
86	13.990	4003	4012	4030	rVV2	28571	55773	1.93%	0.326%
87	14.501	4167	4171	4177	rBV3	1046	1218	0.04%	0.007%
88	14.591	4195	4199	4202	rBV2	1002	1005	0.03%	0.006%
89	14.691	4224	4230	4235	rBV3	2013	2813	0.10%	0.016%
90	14.784	4256	4259	4270	rVB3	1581	2436	0.08%	0.014%
91	14.832	4270	4274	4276	rBV	1571	1353	0.05%	0.008%
92	14.916	4296	4300	4302	rBV2	1253	934	0.03%	0.005%
93	14.993	4321	4324	4328	rBV2	1546	1322	0.05%	0.008%
94	15.147	4370	4372	4377	rVB	1446	1115	0.04%	0.007%
95	15.173	4377	4380	4383	rBV2	1455	1014	0.04%	0.006%
96	15.253	4396	4405	4412	rBV3	1847	4285	0.15%	0.025%
97	15.498	4477	4481	4486	rVB3	2193	1974	0.07%	0.012%
98	15.530	4486	4491	4494	rBV3	1258	1268	0.04%	0.007%
99	15.578	4503	4506	4508	rBV	1568	1139	0.04%	0.007%
100	15.671	4525	4535	4554	rBV7	9902	25277	0.87%	0.148%


Sum of corrected areas: 17103160

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032219\
Data File : VU030302.D
Acq On : 22 Mar 2019 12:50
Operator : JC/SP
Sample : K2022-08DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09C8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

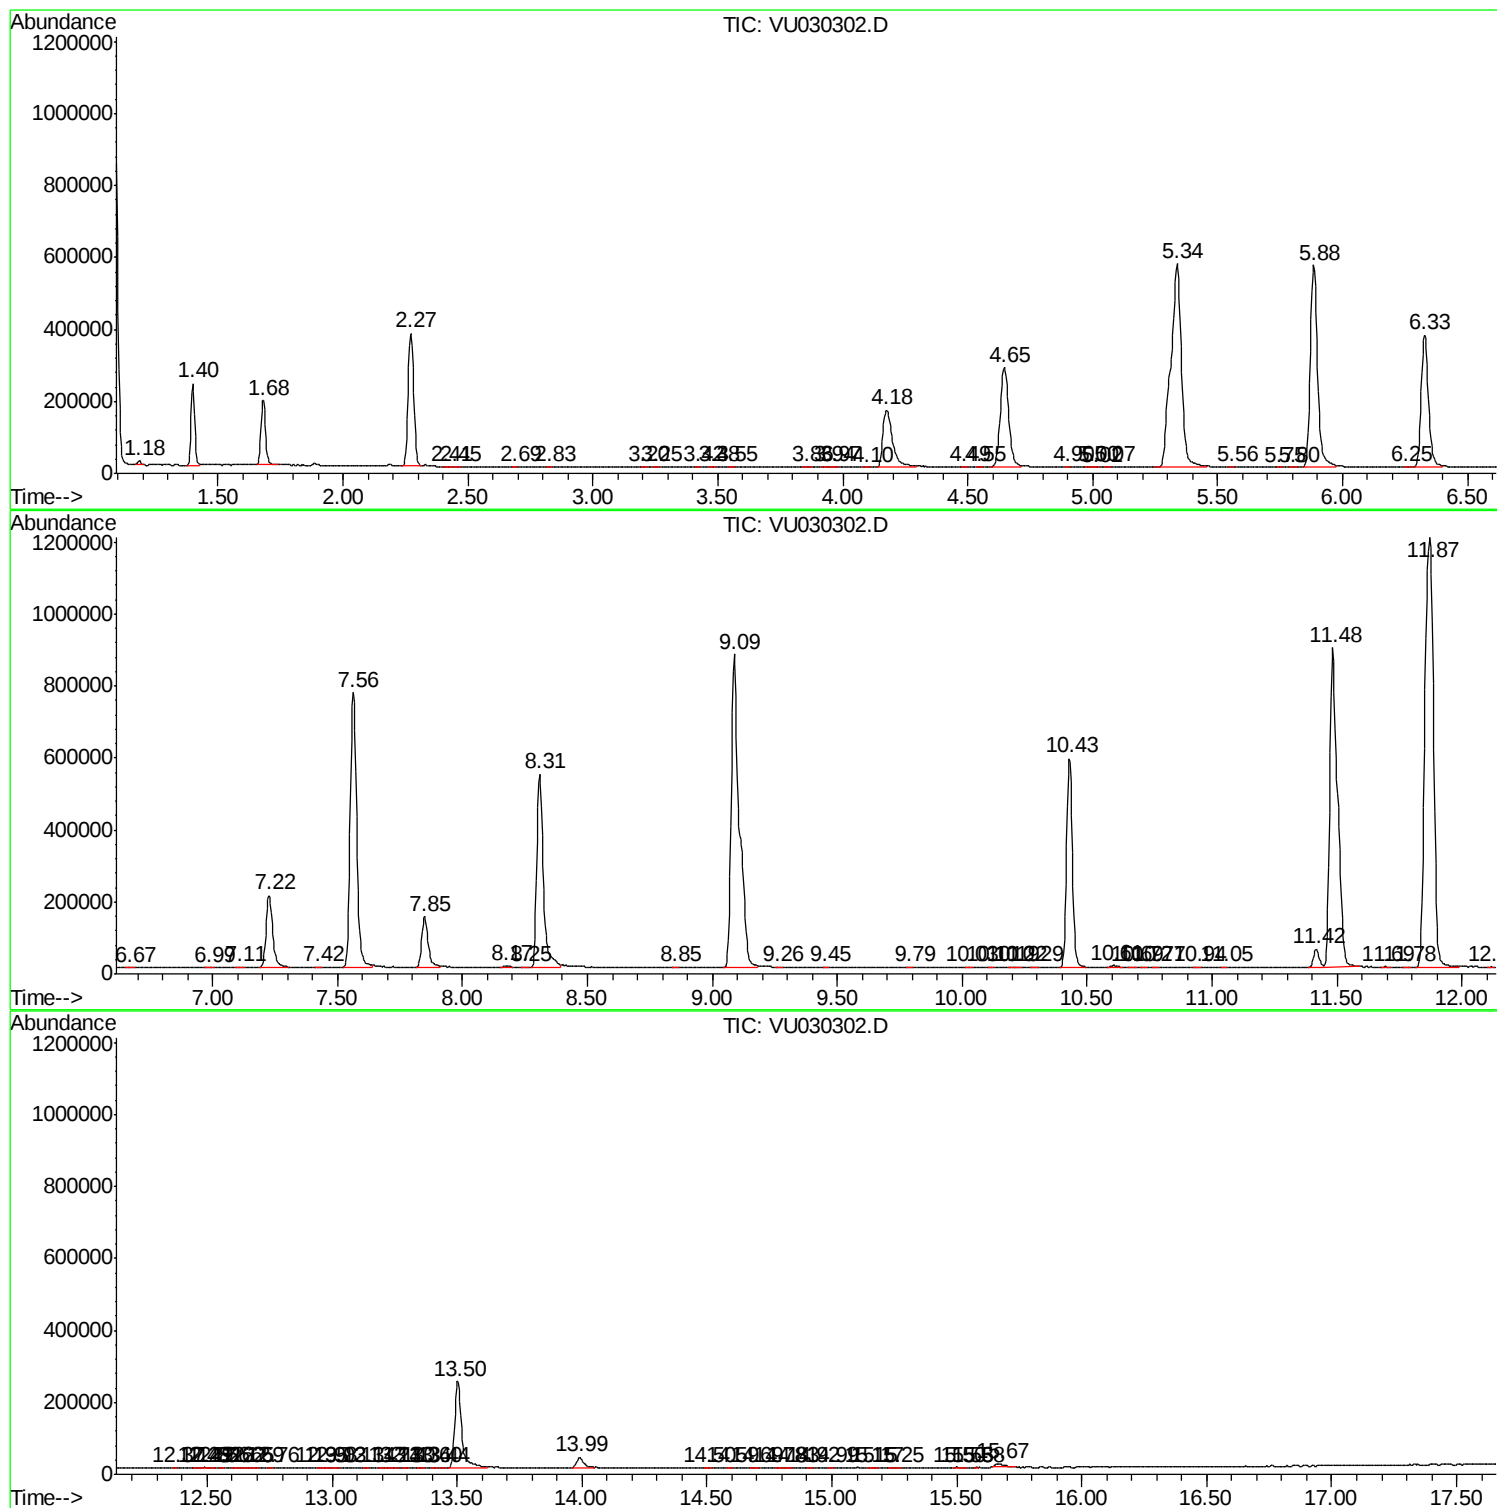

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032219\
Data File : VU030302.D
Acq On : 22 Mar 2019 12:50
Operator : JC/SP
Sample : K2022-08DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032219\
Data File : VU030302.D
Acq On : 22 Mar 2019 12:50
Operator : JC/SP
Sample : K2022-08DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc