

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030303.D
 Acq On : 22 Mar 2019 13:13
 Operator : JC/SP
 Sample : K2048-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB	12661	11392	0.65%	0.079%
2	1.399	89	96	110	rBV	247029	242144	13.88%	1.679%
3	1.678	176	183	197	rVB	180604	230887	13.24%	1.601%
4	2.270	356	367	381	rBV	389690	595003	34.12%	4.126%
5	2.813	533	536	539	rBV	1967	1590	0.09%	0.011%
6	2.923	567	570	572	rBV	1379	1081	0.06%	0.007%
7	3.871	859	865	866	rBV	1502	1415	0.08%	0.010%
8	3.913	875	878	884	rVB	1412	1247	0.07%	0.009%
9	3.942	884	887	889	rBV	1649	1073	0.06%	0.007%
10	4.128	942	945	948	rBV	1300	986	0.06%	0.007%
11	4.174	948	959	996	rVV	172303	484482	27.78%	3.360%
12	4.518	1062	1066	1069	rBV	1437	1148	0.07%	0.008%
13	4.646	1086	1106	1129	rBV	289626	689744	39.55%	4.783%
14	4.945	1195	1199	1201	rBV2	1353	1060	0.06%	0.007%
15	5.003	1215	1217	1221	rVB	1729	1025	0.06%	0.007%
16	5.157	1262	1265	1269	rBV2	1020	744	0.04%	0.005%
17	5.337	1297	1321	1354	rBV2	587285	1744015	100.00%	12.094%
18	5.559	1387	1390	1394	rBV	1344	1019	0.06%	0.007%
19	5.794	1460	1463	1466	rVB	1364	772	0.04%	0.005%
20	5.813	1466	1469	1473	rVB	1355	1029	0.06%	0.007%
21	5.884	1477	1491	1527	rBV	557302	1132642	64.94%	7.854%
22	6.096	1555	1557	1561	rVB	1344	857	0.05%	0.006%
23	6.119	1561	1564	1568	rBV	809	750	0.04%	0.005%
24	6.183	1571	1584	1610	rVV2	177784	361563	20.73%	2.507%
25	6.328	1615	1629	1653	rBV	379715	769278	44.11%	5.335%
26	6.556	1693	1700	1702	rBV3	1429	1680	0.10%	0.012%
27	6.591	1709	1711	1715	rVB	1141	696	0.04%	0.005%
28	6.636	1720	1725	1731	rVB3	1269	1420	0.08%	0.010%
29	6.694	1739	1743	1746	rBV	990	841	0.05%	0.006%
30	6.884	1799	1802	1805	rBV2	961	673	0.04%	0.005%
31	6.919	1810	1813	1815	rBV2	1208	906	0.05%	0.006%
32	6.990	1832	1835	1838	rBV	1322	963	0.06%	0.007%
33	7.074	1855	1861	1865	rVB	1186	1238	0.07%	0.009%
34	7.106	1868	1871	1874	rVB	1550	955	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030303.D
 Acq On : 22 Mar 2019 13:13
 Operator : JC/SP
 Sample : K2048-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.138	1874	1881	1885	rBV2	1870	3162	0.18%	0.022%
36	7.225	1895	1908	1933	rBV	210220	389269	22.32%	2.699%
37	7.382	1952	1957	1959	rBV	1069	1094	0.06%	0.008%
38	7.427	1966	1971	1977	rVB3	1265	1613	0.09%	0.011%
39	7.466	1977	1983	1986	rBV	1878	2035	0.12%	0.014%
40	7.492	1989	1991	1995	rVB	1586	971	0.06%	0.007%
41	7.514	1995	1998	2000	rBV	1196	775	0.04%	0.005%
42	7.562	2000	2013	2043	rBV	784951	1413101	81.03%	9.799%
43	7.849	2091	2102	2129	rBV	144686	263108	15.09%	1.825%
44	8.016	2148	2154	2161	rBV2	1574	2297	0.13%	0.016%
45	8.048	2161	2164	2171	rVB2	1489	1588	0.09%	0.011%
46	8.087	2171	2176	2179	rVB3	1120	1037	0.06%	0.007%
47	8.109	2179	2183	2187	rVB	1407	1392	0.08%	0.010%
48	8.135	2187	2191	2192	rBV	1517	1026	0.06%	0.007%
49	8.180	2196	2205	2214	rBV3	2045	3867	0.22%	0.027%
50	8.225	2215	2219	2223	rBV3	1526	1360	0.08%	0.009%
51	8.308	2234	2245	2280	rBV	566516	1050908	60.26%	7.288%
52	8.601	2332	2336	2340	rBV2	995	872	0.05%	0.006%
53	8.714	2366	2371	2377	rBV3	1335	1654	0.09%	0.011%
54	8.742	2377	2380	2384	rBV2	980	939	0.05%	0.007%
55	8.858	2410	2416	2421	rBV3	1415	1773	0.10%	0.012%
56	8.987	2453	2456	2462	rVB2	1227	1093	0.06%	0.008%
57	9.086	2473	2487	2510	rBV	818534	1388458	79.61%	9.628%
58	9.270	2539	2544	2547	rBV3	881	1001	0.06%	0.007%
59	9.373	2571	2576	2582	rBV	1446	2124	0.12%	0.015%
60	9.575	2637	2639	2643	rVB	1187	687	0.04%	0.005%
61	9.614	2643	2651	2654	rBV2	1393	1973	0.11%	0.014%
62	9.675	2666	2670	2676	rBV	1165	1258	0.07%	0.009%
63	9.971	2760	2762	2766	rVB	2369	1396	0.08%	0.010%
64	10.080	2792	2796	2798	rBV	1186	1087	0.06%	0.008%
65	10.131	2809	2812	2818	rVB	1288	1323	0.08%	0.009%
66	10.218	2836	2839	2846	rVB2	919	972	0.06%	0.007%
67	10.250	2846	2849	2859	rBV3	990	1543	0.09%	0.011%
68	10.427	2889	2904	2930	rBV	596296	974627	55.88%	6.759%
69	10.591	2951	2955	2958	rBV2	1404	1266	0.07%	0.009%
70	10.607	2958	2960	2966	rVB	1536	1350	0.08%	0.009%
71	10.723	2993	2996	3000	rVV	1171	947	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030303.D
 Acq On : 22 Mar 2019 13:13
 Operator : JC/SP
 Sample : K2048-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.791	3012	3017	3026	rVB	1573	2322	0.13%	0.016%
73	10.829	3026	3029	3036	rBV	2085	2394	0.14%	0.017%
74	10.922	3054	3058	3061	rBV	995	867	0.05%	0.006%
75	10.993	3074	3080	3082	rBV	911	966	0.06%	0.007%
76	11.006	3082	3084	3088	rVB	1511	1030	0.06%	0.007%
77	11.131	3118	3123	3125	rBV	1015	1054	0.06%	0.007%
78	11.164	3130	3133	3137	rVV	1680	1423	0.08%	0.010%
79	11.186	3137	3140	3143	rVV	1214	837	0.05%	0.006%
80	11.205	3143	3146	3148	rVV2	1043	711	0.04%	0.005%
81	11.334	3182	3186	3191	rBV	1364	1415	0.08%	0.010%
82	11.482	3220	3232	3255	rBV	776755	1280533	73.42%	8.880%
83	11.858	3337	3349	3367	rBV	771616	1292414	74.11%	8.962%
84	12.212	3456	3459	3462	rBV	1006	835	0.05%	0.006%
85	12.241	3466	3468	3470	rBV2	1236	752	0.04%	0.005%
86	12.395	3512	3516	3519	rBV	1451	1119	0.06%	0.008%
87	12.633	3586	3590	3594	rBV	1401	1342	0.08%	0.009%
88	12.678	3600	3604	3607	rBV2	1069	1066	0.06%	0.007%
89	12.746	3620	3625	3628	rBV	1376	1426	0.08%	0.010%
90	12.938	3683	3685	3689	rVV	1403	903	0.05%	0.006%
91	12.977	3693	3697	3698	rBV	1110	848	0.05%	0.006%
92	13.128	3741	3744	3753	rVB2	1641	1784	0.10%	0.012%
93	13.189	3759	3763	3766	rBV2	1475	1322	0.08%	0.009%
94	13.389	3822	3825	3828	rBV	1195	918	0.05%	0.006%
95	13.459	3843	3847	3848	rBV	1117	685	0.04%	0.005%
96	13.524	3862	3867	3872	rBV4	3155	4411	0.25%	0.031%
97	13.945	3995	3998	4002	rBV	1880	1312	0.08%	0.009%
98	14.199	4074	4077	4079	rBV2	1611	1192	0.07%	0.008%
99	14.260	4091	4096	4098	rBV2	2068	2040	0.12%	0.014%
100	14.327	4113	4117	4120	rBV2	1189	1310	0.08%	0.009%


Sum of corrected areas: 14420495

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030303.D
Acq On : 22 Mar 2019 13:13
Operator : JC/SP
Sample : K2048-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

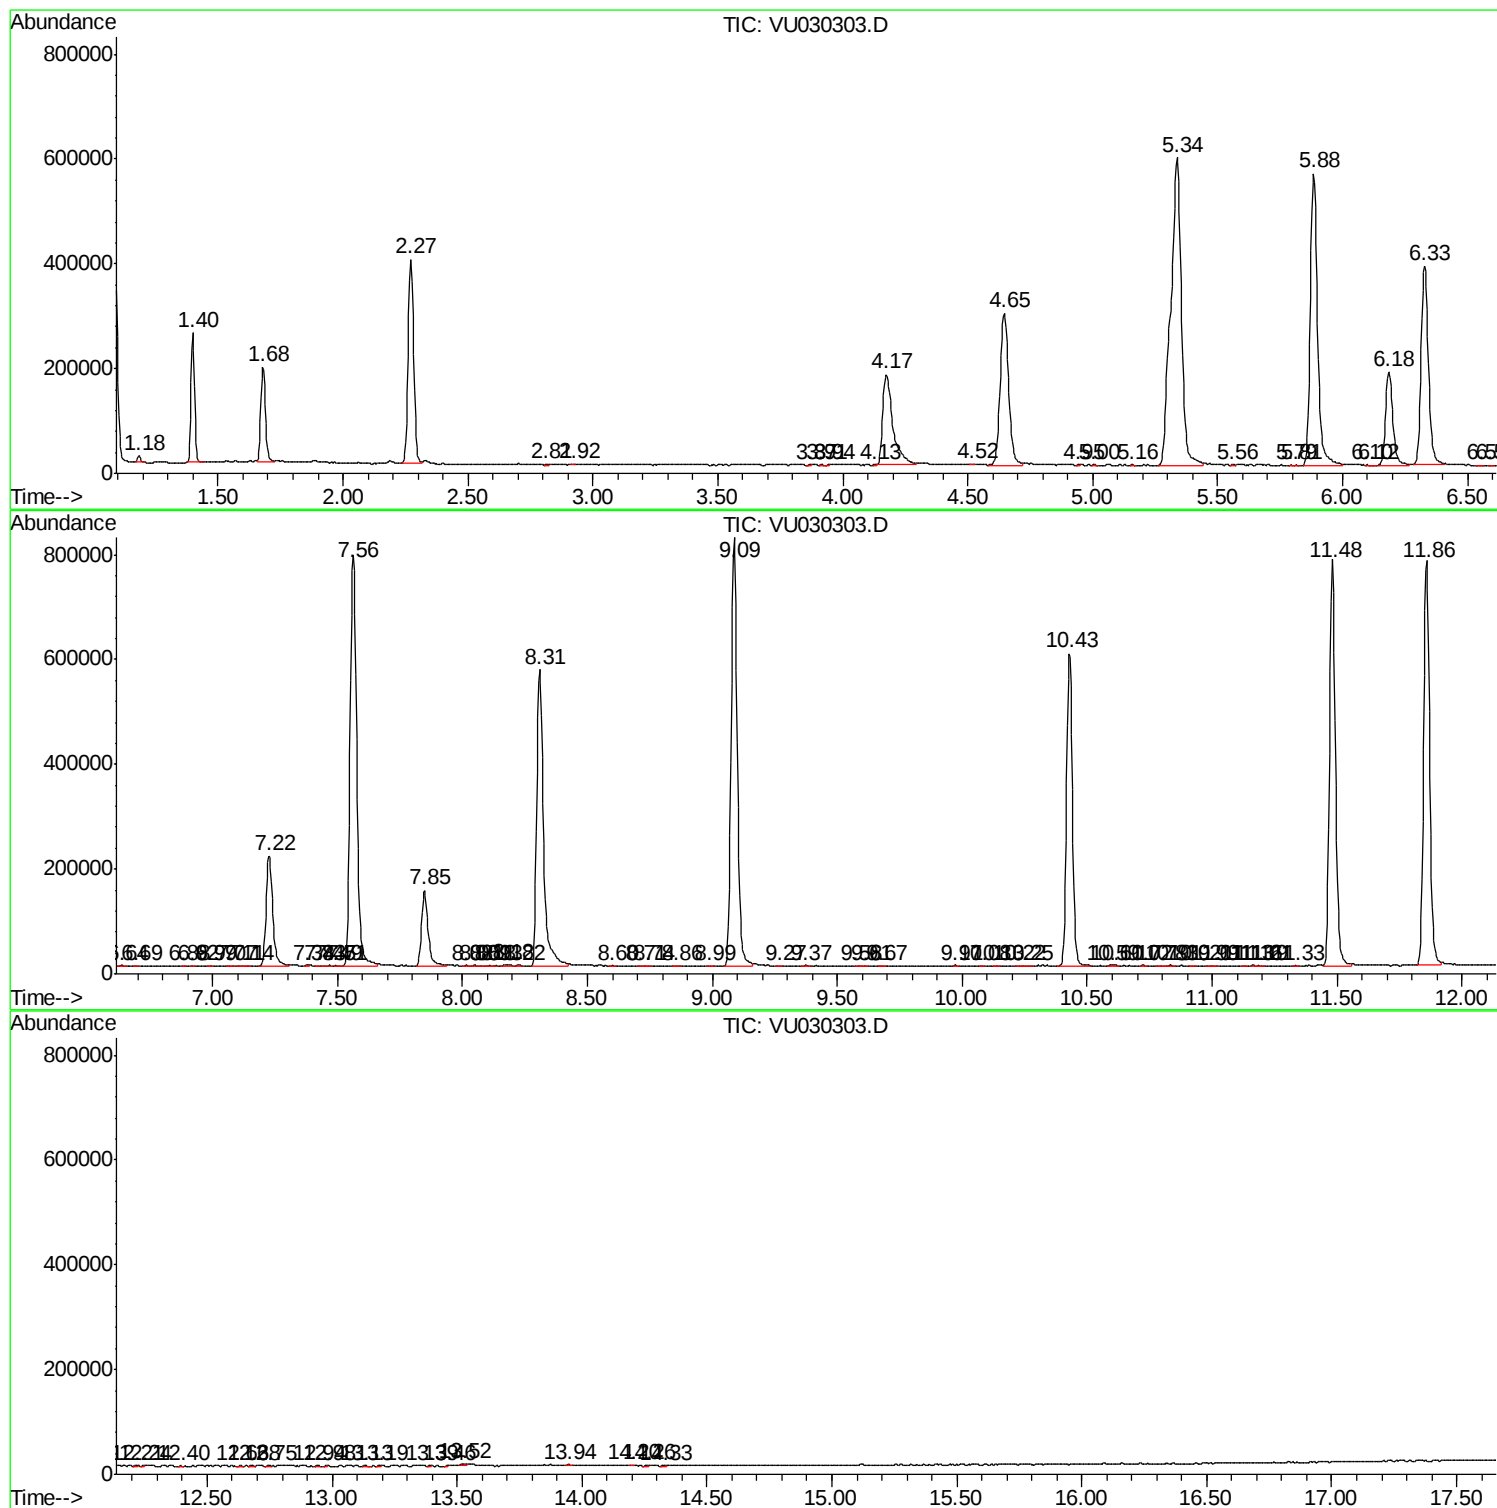

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030303.D
Acq On : 22 Mar 2019 13:13
Operator : JC/SP
Sample : K2048-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030303.D
Acq On : 22 Mar 2019 13:13
Operator : JC/SP
Sample : K2048-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc