

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030304.D
 Acq On : 22 Mar 2019 13:36
 Operator : JC/SP
 Sample : K2048-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF199

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	35	rVB2	11158	10802	0.50%	0.067%
2	1.399	89	96	107	rBV	243558	240356	11.17%	1.502%
3	1.678	176	183	203	rVB	178124	231589	10.76%	1.447%
4	2.270	357	367	382	rBV	384430	583037	27.09%	3.642%
5	2.370	396	398	401	rBV2	1443	1059	0.05%	0.007%
6	2.704	496	502	508	rVB3	2367	3705	0.17%	0.023%
7	2.791	522	529	535	rBV	1704	2526	0.12%	0.016%
8	2.845	544	546	550	rVB	1706	1122	0.05%	0.007%
9	2.903	561	564	571	rBV	1326	1703	0.08%	0.011%
10	2.971	577	585	587	rBV	1134	1661	0.08%	0.010%
11	3.032	600	604	609	rVB	1592	1553	0.07%	0.010%
12	3.235	663	667	670	rVV	1523	1199	0.06%	0.007%
13	3.469	735	740	743	rBV	1489	1596	0.07%	0.010%
14	3.733	818	822	826	rVB	1345	1165	0.05%	0.007%
15	3.829	848	852	858	rBV	1131	1121	0.05%	0.007%
16	3.955	887	891	901	rVB	1124	2040	0.09%	0.013%
17	4.173	948	959	993	rBV	164413	479542	22.28%	2.996%
18	4.421	1033	1036	1040	rVB	2369	1678	0.08%	0.010%
19	4.450	1040	1045	1047	rBV	2095	1812	0.08%	0.011%
20	4.508	1058	1063	1066	rBV	1612	1337	0.06%	0.008%
21	4.530	1066	1070	1075	rVB	1831	1660	0.08%	0.010%
22	4.646	1090	1106	1129	rBV	278355	666424	30.96%	4.163%
23	5.141	1256	1260	1265	rVB	1316	1396	0.06%	0.009%
24	5.186	1265	1274	1277	rBV	2085	2576	0.12%	0.016%
25	5.218	1281	1284	1291	rVV2	1142	1304	0.06%	0.008%
26	5.337	1297	1321	1359	rBV2	570054	1704671	79.19%	10.649%
27	5.572	1391	1394	1398	rVB	1468	1053	0.05%	0.007%
28	5.636	1408	1414	1415	rBV	1396	1240	0.06%	0.008%
29	5.749	1442	1449	1455	rBV	1907	2942	0.14%	0.018%
30	5.781	1455	1459	1466	rBV3	1082	1052	0.05%	0.007%
31	5.884	1477	1491	1528	rBV	551145	1130212	52.51%	7.060%
32	6.054	1540	1544	1551	rBV2	2055	2332	0.11%	0.015%
33	6.103	1554	1559	1564	rVB2	1188	1073	0.05%	0.007%
34	6.183	1569	1584	1615	rBV	1095790	2152521	100.00%	13.447%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030304.D
 Acq On : 22 Mar 2019 13:36
 Operator : JC/SP
 Sample : K2048-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF199

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1616	1629	1663	rVB	376029	767782	35.67%	4.796%
36	6.604	1711	1715	1719	rBV2	994	1047	0.05%	0.007%
37	6.662	1728	1733	1736	rBV2	961	1123	0.05%	0.007%
38	6.836	1781	1787	1794	rVB3	1522	2391	0.11%	0.015%
39	6.871	1794	1798	1803	rBV	1893	1730	0.08%	0.011%
40	6.923	1808	1814	1816	rBV4	1298	1549	0.07%	0.010%
41	6.955	1821	1824	1833	rVB	1337	1399	0.06%	0.009%
42	7.022	1838	1845	1850	rBV2	1376	1789	0.08%	0.011%
43	7.054	1851	1855	1863	rVB2	1310	1503	0.07%	0.009%
44	7.096	1863	1868	1871	rBV	1842	1257	0.06%	0.008%
45	7.225	1897	1908	1927	rBV	207163	381464	17.72%	2.383%
46	7.562	1997	2013	2039	rBV	770648	1383041	64.25%	8.640%
47	7.720	2058	2062	2065	rBV	1323	1121	0.05%	0.007%
48	7.849	2092	2102	2120	rBV	144052	254831	11.84%	1.592%
49	8.051	2161	2165	2167	rBV	1417	1292	0.06%	0.008%
50	8.099	2176	2180	2184	rVB3	1049	1047	0.05%	0.007%
51	8.170	2197	2202	2205	rBV3	1114	1064	0.05%	0.007%
52	8.228	2211	2220	2231	rVB5	12480	22658	1.05%	0.142%
53	8.308	2234	2245	2286	rBV	547666	1015231	47.16%	6.342%
54	8.768	2384	2388	2395	rVB2	1151	1129	0.05%	0.007%
55	8.906	2426	2431	2433	rBV2	1850	1483	0.07%	0.009%
56	9.000	2456	2460	2464	rBV	1271	1329	0.06%	0.008%
57	9.086	2475	2487	2505	rBV	824789	1373993	63.83%	8.583%
58	9.504	2613	2617	2619	rBV2	1839	1654	0.08%	0.010%
59	9.582	2637	2641	2646	rBV	1617	1764	0.08%	0.011%
60	9.672	2665	2669	2672	rBV	1184	1064	0.05%	0.007%
61	9.932	2746	2750	2754	rVV2	1369	1641	0.08%	0.010%
62	9.955	2755	2757	2763	rVB	1408	1223	0.06%	0.008%
63	10.048	2783	2786	2790	rBV	1581	1479	0.07%	0.009%
64	10.167	2816	2823	2830	rVB	1273	1710	0.08%	0.011%
65	10.257	2844	2851	2855	rBV	1172	1555	0.07%	0.010%
66	10.427	2892	2904	2929	rBV	583499	954361	44.34%	5.962%
67	10.710	2988	2992	2994	rBV	1500	1183	0.05%	0.007%
68	10.774	3008	3012	3015	rBV	1622	1055	0.05%	0.007%
69	10.839	3021	3032	3037	rBV	1906	3756	0.17%	0.023%
70	10.871	3037	3042	3046	rBV2	1217	1724	0.08%	0.011%
71	11.083	3105	3108	3116	rBV3	1667	1569	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030304.D
 Acq On : 22 Mar 2019 13:36
 Operator : JC/SP
 Sample : K2048-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF199

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.144	3123	3127	3132	rBV3	958	1090	0.05%	0.007%
73	11.254	3157	3161	3167	rVB	1848	1998	0.09%	0.012%
74	11.286	3167	3171	3182	rBV3	1345	2449	0.11%	0.015%
75	11.379	3194	3200	3204	rBV	1956	2613	0.12%	0.016%
76	11.482	3220	3232	3261	rBV	766761	1266878	58.86%	7.914%
77	11.858	3336	3349	3371	rBV	743861	1258622	58.47%	7.863%
78	12.073	3413	3416	3421	rBV3	1253	1033	0.05%	0.006%
79	12.106	3423	3426	3429	rVB	1961	1197	0.06%	0.007%
80	12.247	3467	3470	3476	rVB	1749	1598	0.07%	0.010%
81	12.276	3476	3479	3482	rVB	1611	1088	0.05%	0.007%
82	12.315	3486	3491	3494	rBV	2365	2590	0.12%	0.016%
83	12.594	3575	3578	3582	rVB	2014	1324	0.06%	0.008%
84	12.633	3582	3590	3593	rBV2	2581	3086	0.14%	0.019%
85	13.157	3748	3753	3759	rBV2	1489	1985	0.09%	0.012%
86	13.289	3789	3794	3797	rVB	1581	1564	0.07%	0.010%
87	13.498	3856	3859	3862	rVB	1721	1201	0.06%	0.008%
88	13.524	3862	3867	3870	rBV3	1646	1799	0.08%	0.011%
89	13.710	3921	3925	3929	rVB	1317	1336	0.06%	0.008%
90	13.739	3929	3934	3936	rBV2	1541	1520	0.07%	0.009%
91	13.951	3995	4000	4002	rBV	1489	1266	0.06%	0.008%
92	14.093	4040	4044	4049	rBV	1041	1182	0.05%	0.007%
93	14.343	4119	4122	4125	rBV	1630	1122	0.05%	0.007%
94	14.729	4235	4242	4245	rBV	1191	1624	0.08%	0.010%
95	14.890	4290	4292	4298	rBV2	969	1149	0.05%	0.007%
96	15.096	4353	4356	4362	rBV	2158	2075	0.10%	0.013%
97	15.173	4377	4380	4385	rVB	2669	2144	0.10%	0.013%
98	15.199	4385	4388	4391	rBV	1522	1233	0.06%	0.008%
99	15.305	4417	4421	4423	rBV	1733	1387	0.06%	0.009%
100	15.427	4455	4459	4462	rBV2	1695	1505	0.07%	0.009%


Sum of corrected areas: 16007708

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030304.D
Acq On : 22 Mar 2019 13:36
Operator : JC/SP
Sample : K2048-07 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF199

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

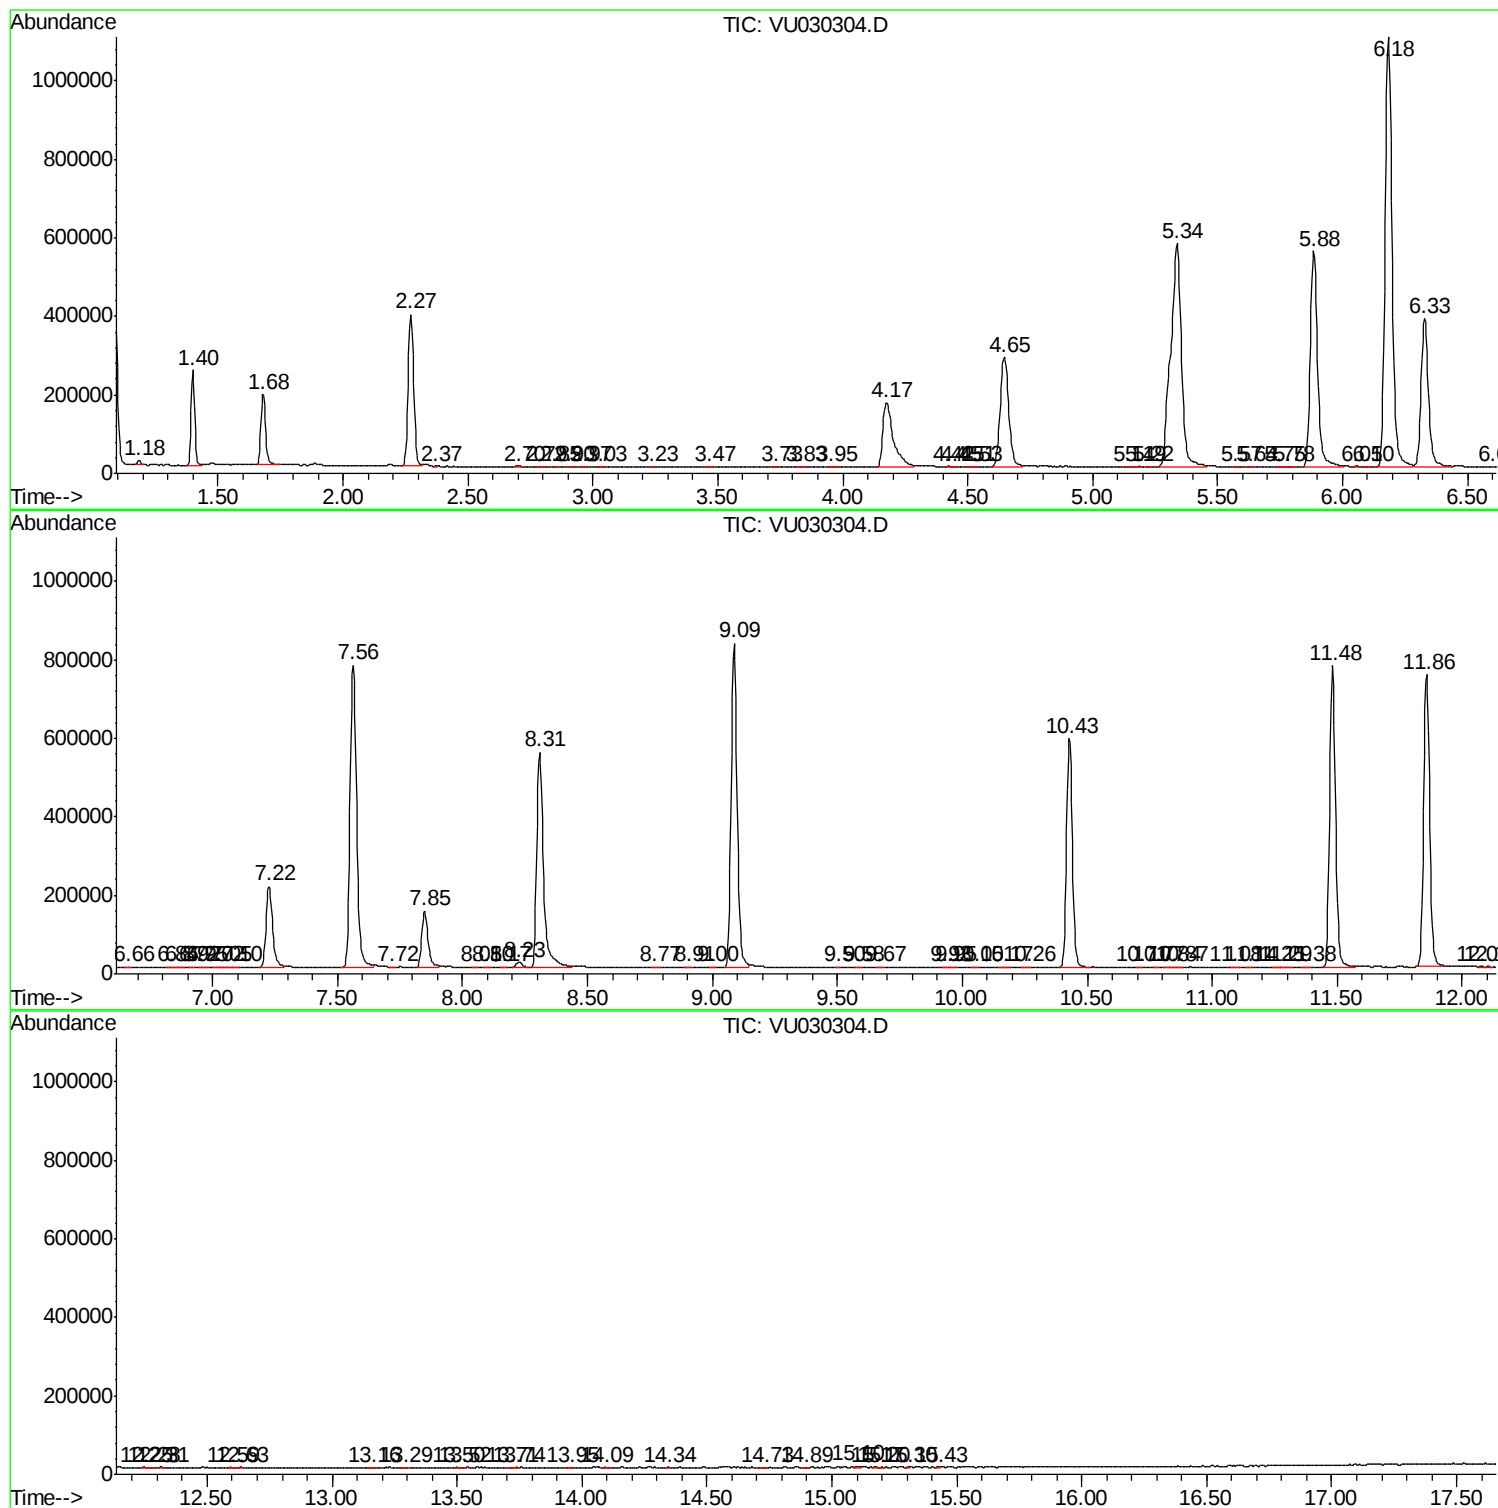

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030304.D
Acq On : 22 Mar 2019 13:36
Operator : JC/SP
Sample : K2048-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF199

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030304.D
Acq On : 22 Mar 2019 13:36
Operator : JC/SP
Sample : K2048-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF199

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc