

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030307.D
 Acq On : 22 Mar 2019 14:45
 Operator : JC/SP
 Sample : K2048-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	35	rVB	12287	10966	0.63%	0.078%
2	1.399	89	96	111	rBV	236472	241577	13.95%	1.717%
3	1.678	176	183	200	rVB	179979	227917	13.16%	1.620%
4	2.270	357	367	380	rBV	391526	594974	34.37%	4.228%
5	2.537	447	450	458	rVB	1487	1710	0.10%	0.012%
6	2.630	475	479	482	rVB	1517	1266	0.07%	0.009%
7	2.701	497	501	507	rVV3	1678	1680	0.10%	0.012%
8	2.842	539	545	550	rBV	1242	1630	0.09%	0.012%
9	3.096	621	624	628	rBV2	1137	1125	0.06%	0.008%
10	3.174	643	648	650	rBV	1552	1481	0.09%	0.011%
11	3.215	655	661	665	rBV2	1455	1570	0.09%	0.011%
12	3.473	735	741	747	rBV	1233	1966	0.11%	0.014%
13	3.505	747	751	755	rBV	1426	1271	0.07%	0.009%
14	3.675	800	804	810	rBV	813	1087	0.06%	0.008%
15	3.826	847	851	854	rBV	1277	1134	0.07%	0.008%
16	3.858	858	861	865	rVB	1429	1024	0.06%	0.007%
17	3.952	885	890	896	rBV	1859	2421	0.14%	0.017%
18	4.010	901	908	911	rBV	1648	2028	0.12%	0.014%
19	4.119	936	942	945	rBV	1116	1322	0.08%	0.009%
20	4.177	948	960	991	rBV	169900	449212	25.95%	3.192%
21	4.399	1024	1029	1032	rBV2	1526	1686	0.10%	0.012%
22	4.646	1090	1106	1133	rBV	288316	686239	39.64%	4.876%
23	4.865	1171	1174	1177	rBV	1920	1720	0.10%	0.012%
24	5.116	1249	1252	1256	rBV	1600	1240	0.07%	0.009%
25	5.337	1297	1321	1342	rBV2	591514	1731302	100.00%	12.303%
26	5.675	1422	1426	1430	rBV	1192	1431	0.08%	0.010%
27	5.797	1459	1464	1467	rBV	1132	1154	0.07%	0.008%
28	5.884	1478	1491	1517	rBV	553373	1124175	64.93%	7.989%
29	6.145	1569	1572	1574	rBV2	1251	1007	0.06%	0.007%
30	6.328	1615	1629	1660	rBV	380035	775599	44.80%	5.511%
31	6.537	1690	1694	1702	rBV2	1744	2236	0.13%	0.016%
32	6.836	1779	1787	1789	rBV	1047	1187	0.07%	0.008%
33	6.997	1833	1837	1841	rBV3	918	1034	0.06%	0.007%
34	7.225	1896	1908	1926	rVV	209161	381667	22.05%	2.712%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030307.D
 Acq On : 22 Mar 2019 14:45
 Operator : JC/SP
 Sample : K2048-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.353	1945	1948	1952	rBV	1587	1360	0.08%	0.010%
36	7.505	1993	1995	1999	rVB	1449	962	0.06%	0.007%
37	7.562	1999	2013	2039	rBV	787109	1416390	81.81%	10.065%
38	7.726	2061	2064	2069	rVB3	1367	1038	0.06%	0.007%
39	7.849	2092	2102	2117	rBV2	147016	257266	14.86%	1.828%
40	8.080	2171	2174	2177	rBV	1505	965	0.06%	0.007%
41	8.161	2194	2199	2201	rBV2	1665	1464	0.08%	0.010%
42	8.177	2201	2204	2209	rBV2	1363	1129	0.07%	0.008%
43	8.225	2209	2219	2234	rBV2	43514	77222	4.46%	0.549%
44	8.308	2234	2245	2274	rBV	565528	1040131	60.08%	7.391%
45	8.546	2312	2319	2323	rVV	2255	2708	0.16%	0.019%
46	8.569	2323	2326	2331	rVB2	1867	1375	0.08%	0.010%
47	8.601	2331	2336	2342	rBV2	1460	1796	0.10%	0.013%
48	8.633	2343	2346	2351	rVB	1788	1392	0.08%	0.010%
49	8.669	2353	2357	2360	rBV2	1146	960	0.06%	0.007%
50	8.768	2383	2388	2391	rBV	1153	1045	0.06%	0.007%
51	8.849	2405	2413	2417	rBV	1676	2376	0.14%	0.017%
52	8.919	2430	2435	2440	rBV	1294	1208	0.07%	0.009%
53	8.958	2441	2447	2450	rVB	1241	1138	0.07%	0.008%
54	9.013	2456	2464	2468	rBV2	1278	1394	0.08%	0.010%
55	9.038	2468	2472	2474	rBV	1202	1002	0.06%	0.007%
56	9.087	2475	2487	2511	rBV	834833	1394136	80.53%	9.907%
57	9.263	2538	2542	2545	rBV	1164	1077	0.06%	0.008%
58	9.299	2550	2553	2556	rVB2	1901	1324	0.08%	0.009%
59	9.488	2607	2612	2615	rBV2	1133	1127	0.07%	0.008%
60	9.604	2645	2648	2652	rBV	1492	1164	0.07%	0.008%
61	9.890	2733	2737	2743	rVB2	1328	1556	0.09%	0.011%
62	10.106	2795	2804	2807	rBV2	1817	2686	0.16%	0.019%
63	10.357	2878	2882	2885	rBV	1089	1026	0.06%	0.007%
64	10.427	2893	2904	2928	rVB	594622	973599	56.24%	6.919%
65	10.559	2943	2945	2952	rVB2	1598	1361	0.08%	0.010%
66	10.614	2957	2962	2968	rBV3	1348	1568	0.09%	0.011%
67	10.697	2983	2988	2991	rBV	979	951	0.05%	0.007%
68	10.849	3031	3035	3038	rBV	1424	1199	0.07%	0.009%
69	10.910	3049	3054	3061	rBV2	1708	2361	0.14%	0.017%
70	10.974	3071	3074	3078	rBV	2007	1895	0.11%	0.013%
71	11.247	3157	3159	3165	rVB	1475	1197	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030307.D
 Acq On : 22 Mar 2019 14:45
 Operator : JC/SP
 Sample : K2048-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.392	3202	3204	3207	rVB2	1650	996	0.06%	0.007%
73	11.482	3217	3232	3252	rBV	779691	1284242	74.18%	9.126%
74	11.781	3322	3325	3329	rVB2	1287	1074	0.06%	0.008%
75	11.858	3336	3349	3369	rBV	773353	1290672	74.55%	9.172%
76	12.543	3559	3562	3564	rBV	1474	1150	0.07%	0.008%
77	12.601	3577	3580	3584	rBV	1112	1008	0.06%	0.007%
78	12.675	3600	3603	3608	rBV	1369	1245	0.07%	0.009%
79	12.810	3638	3645	3647	rBV	1781	2063	0.12%	0.015%
80	12.852	3651	3658	3659	rBV	1264	1269	0.07%	0.009%
81	12.903	3670	3674	3679	rVB2	1178	1077	0.06%	0.008%
82	12.932	3679	3683	3686	rBV2	1250	1183	0.07%	0.008%
83	13.080	3726	3729	3732	rBV	1605	1157	0.07%	0.008%
84	13.160	3751	3754	3758	rVB	1256	1045	0.06%	0.007%
85	13.254	3777	3783	3788	rBV2	1347	1805	0.10%	0.013%
86	13.315	3796	3802	3804	rBV2	1198	1161	0.07%	0.008%
87	13.495	3855	3858	3865	rVB2	1500	1583	0.09%	0.011%
88	13.668	3906	3912	3917	rBV	1699	1728	0.10%	0.012%
89	13.723	3925	3929	3931	rBV3	1116	1008	0.06%	0.007%
90	13.832	3956	3963	3966	rBV2	1997	2522	0.15%	0.018%
91	13.971	4002	4006	4010	rBV2	1251	1361	0.08%	0.010%
92	14.038	4024	4027	4030	rBV	1585	1347	0.08%	0.010%
93	14.106	4041	4048	4050	rBV	1278	1473	0.09%	0.010%
94	14.270	4095	4099	4102	rBV2	1490	1272	0.07%	0.009%
95	14.337	4115	4120	4121	rBV	1291	1042	0.06%	0.007%
96	14.443	4149	4153	4156	rBV	1060	991	0.06%	0.007%
97	14.887	4287	4291	4295	rBV3	1415	1450	0.08%	0.010%
98	15.205	4384	4390	4392	rBV	1609	1539	0.09%	0.011%
99	15.253	4401	4405	4410	rVB2	1577	1252	0.07%	0.009%
100	15.601	4510	4513	4515	rBV2	1610	1098	0.06%	0.008%


Sum of corrected areas: 14072399

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030307.D
Acq On : 22 Mar 2019 14:45
Operator : JC/SP
Sample : K2048-10 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

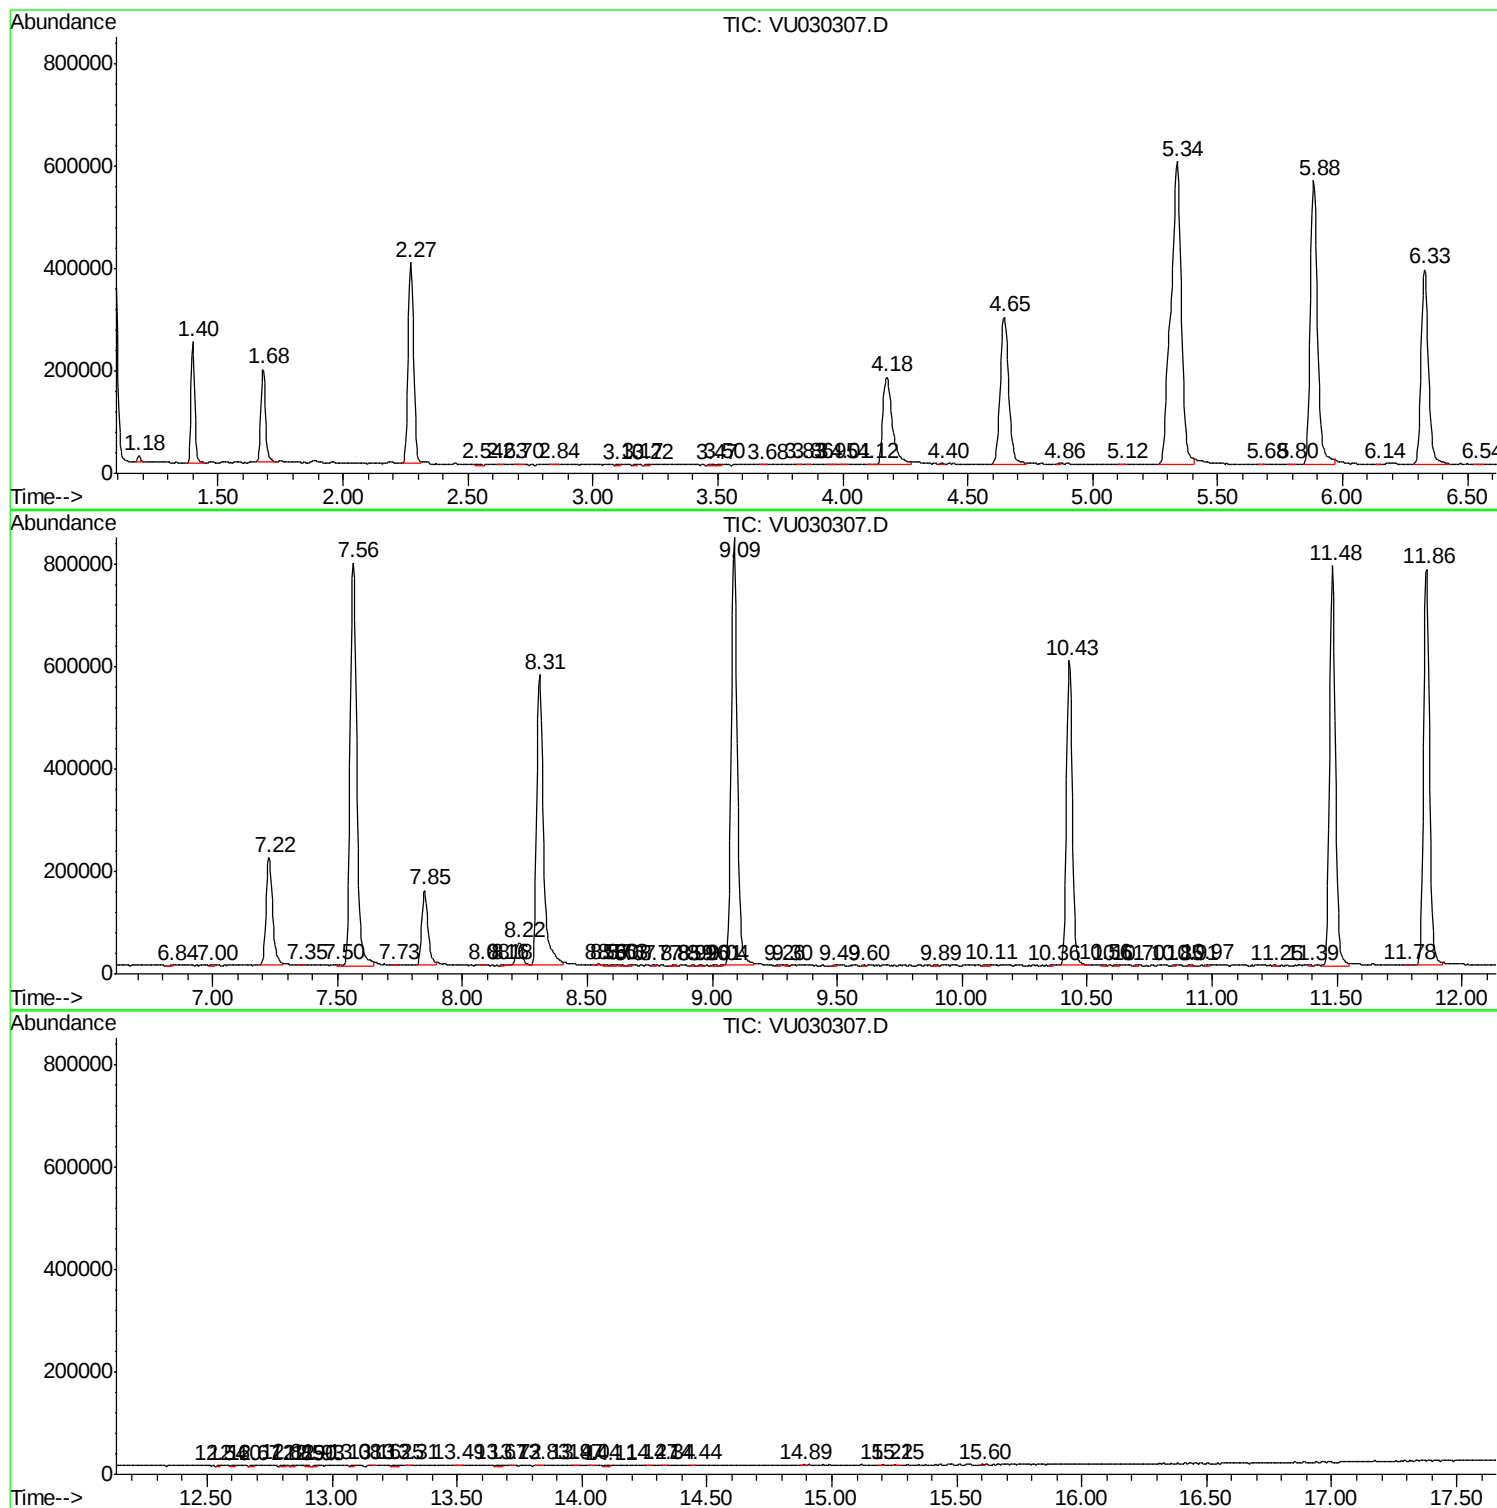

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030307.D
Acq On : 22 Mar 2019 14:45
Operator : JC/SP
Sample : K2048-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030307.D
Acq On : 22 Mar 2019 14:45
Operator : JC/SP
Sample : K2048-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc