

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030311.D
 Acq On : 22 Mar 2019 16:25
 Operator : JC/SP
 Sample : VU0322WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	38	rVB2	12281	12069	0.71%	0.088%
2	1.399	89	96	109	rVB	241829	236176	13.97%	1.727%
3	1.678	176	183	194	rBV	176935	222334	13.15%	1.626%
4	2.270	357	367	382	rBV	386874	594278	35.16%	4.345%
5	3.029	599	603	605	rBV	1973	1581	0.09%	0.012%
6	3.203	652	657	658	rBV	1117	1062	0.06%	0.008%
7	3.653	792	797	800	rBV	1301	1354	0.08%	0.010%
8	3.772	831	834	838	rBV	1823	1493	0.09%	0.011%
9	4.064	920	925	927	rBV	1565	1539	0.09%	0.011%
10	4.177	948	960	996	rVV	165535	444112	26.28%	3.247%
11	4.646	1090	1106	1132	rBV	277994	660017	39.05%	4.825%
12	5.029	1221	1225	1228	rBV	1231	1094	0.06%	0.008%
13	5.103	1243	1248	1249	rBV	1387	1087	0.06%	0.008%
14	5.186	1271	1274	1280	rVB2	1112	935	0.06%	0.007%
15	5.338	1298	1321	1345	rBV2	574573	1690156	100.00%	12.357%
16	5.585	1394	1398	1402	rBV2	1299	1095	0.06%	0.008%
17	5.755	1448	1451	1455	rBV2	1246	1000	0.06%	0.007%
18	5.884	1478	1491	1528	rBV	513302	1056838	62.53%	7.727%
19	6.177	1577	1582	1583	rBV3	1850	1546	0.09%	0.011%
20	6.328	1614	1629	1658	rBV	366368	756737	44.77%	5.533%
21	6.685	1736	1740	1746	rBV	1617	1806	0.11%	0.013%
22	6.723	1746	1752	1755	rVB2	1497	1419	0.08%	0.010%
23	6.743	1755	1758	1760	rBV2	1230	927	0.05%	0.007%
24	6.755	1760	1762	1766	rVV	1462	953	0.06%	0.007%
25	6.797	1770	1775	1779	rVB	729	892	0.05%	0.007%
26	6.907	1806	1809	1812	rBV2	1392	999	0.06%	0.007%
27	6.942	1817	1820	1824	rBV2	1172	970	0.06%	0.007%
28	6.987	1830	1834	1836	rBV	1333	937	0.06%	0.007%
29	7.029	1843	1847	1850	rVB	1371	1008	0.06%	0.007%
30	7.048	1850	1853	1858	rBV	932	955	0.06%	0.007%
31	7.132	1875	1879	1883	rBV3	817	944	0.06%	0.007%
32	7.225	1889	1908	1935	rBV	210188	390924	23.13%	2.858%
33	7.370	1948	1953	1956	rBV	1658	1481	0.09%	0.011%
34	7.563	2000	2013	2051	rBV	759520	1388405	82.15%	10.151%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030311.D
 Acq On : 22 Mar 2019 16:25
 Operator : JC/SP
 Sample : VU0322WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.781	2079	2081	2088	rVB3	1674	1565	0.09%	0.011%
36	7.849	2091	2102	2129	rBV	142627	263261	15.58%	1.925%
37	7.974	2138	2141	2144	rVB	1621	1101	0.07%	0.008%
38	8.029	2156	2158	2162	rVB	1309	868	0.05%	0.006%
39	8.093	2174	2178	2181	rVB	1363	1065	0.06%	0.008%
40	8.161	2192	2199	2200	rBV2	1297	1313	0.08%	0.010%
41	8.225	2214	2219	2227	rVB5	2742	3607	0.21%	0.026%
42	8.308	2233	2245	2283	rBV	553722	1029110	60.89%	7.524%
43	8.579	2326	2329	2334	rBV	1131	893	0.05%	0.007%
44	8.990	2454	2457	2460	rVB	1303	851	0.05%	0.006%
45	9.013	2460	2464	2468	rVB2	931	857	0.05%	0.006%
46	9.087	2468	2487	2510	rBV	780765	1321739	78.20%	9.663%
47	9.299	2549	2553	2559	rBV	1968	2410	0.14%	0.018%
48	9.382	2573	2579	2584	rVV4	1786	2708	0.16%	0.020%
49	9.421	2588	2591	2596	rVV3	1249	1206	0.07%	0.009%
50	9.460	2600	2603	2606	rVV	1044	833	0.05%	0.006%
51	9.778	2693	2702	2706	rBV	1784	3015	0.18%	0.022%
52	9.836	2718	2720	2726	rVB2	1846	1186	0.07%	0.009%
53	9.890	2734	2737	2743	rVB2	1114	908	0.05%	0.007%
54	9.980	2761	2765	2769	rVB	1362	1333	0.08%	0.010%
55	10.003	2769	2772	2775	rBV	1185	851	0.05%	0.006%
56	10.074	2789	2794	2797	rBV2	1178	1347	0.08%	0.010%
57	10.122	2802	2809	2812	rBV	1324	1594	0.09%	0.012%
58	10.241	2840	2846	2848	rBV3	1048	968	0.06%	0.007%
59	10.427	2892	2904	2925	rBV	584663	953686	56.43%	6.973%
60	10.604	2953	2959	2960	rBV2	2494	2244	0.13%	0.016%
61	10.685	2980	2984	2989	rVB	1907	1916	0.11%	0.014%
62	10.919	3049	3057	3060	rBV	1042	1226	0.07%	0.009%
63	11.003	3078	3083	3091	rVB	1472	2066	0.12%	0.015%
64	11.193	3139	3142	3146	rBV	1267	905	0.05%	0.007%
65	11.427	3204	3215	3220	rBV4	3820	5638	0.33%	0.041%
66	11.482	3220	3232	3251	rBV	761738	1250664	74.00%	9.144%
67	11.697	3296	3299	3305	rVV2	1471	1679	0.10%	0.012%
68	11.858	3336	3349	3378	rBV	763788	1282663	75.89%	9.378%
69	12.270	3470	3477	3478	rBV2	1112	1412	0.08%	0.010%
70	12.324	3490	3494	3497	rBV	1057	856	0.05%	0.006%
71	12.360	3501	3505	3511	rBV2	1422	1680	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030311.D
 Acq On : 22 Mar 2019 16:25
 Operator : JC/SP
 Sample : VU0322WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	12.414	3519	3522	3527	rBV	1593	1682	0.10%	0.012%
73	12.482	3534	3543	3544	rBV4	2352	3147	0.19%	0.023%
74	12.537	3557	3560	3564	rVB	1342	971	0.06%	0.007%
75	12.614	3581	3584	3587	rVB	1348	836	0.05%	0.006%
76	12.639	3587	3592	3596	rBV	1044	1273	0.08%	0.009%
77	12.739	3620	3623	3628	rBV	1536	1703	0.10%	0.012%
78	12.803	3638	3643	3647	rVV3	1686	2035	0.12%	0.015%
79	12.823	3647	3649	3655	rVB2	1154	982	0.06%	0.007%
80	12.897	3666	3672	3675	rBV3	1835	2147	0.13%	0.016%
81	12.993	3697	3702	3706	rBV2	1227	1303	0.08%	0.010%
82	13.032	3712	3714	3722	rVB2	1438	1172	0.07%	0.009%
83	13.080	3724	3729	3735	rVV3	1189	1203	0.07%	0.009%
84	13.144	3746	3749	3754	rBV2	1169	1006	0.06%	0.007%
85	13.170	3754	3757	3763	rVB	1393	1347	0.08%	0.010%
86	13.209	3763	3769	3770	rBV2	1035	1019	0.06%	0.007%
87	13.283	3788	3792	3796	rBV	1440	1322	0.08%	0.010%
88	13.311	3798	3801	3803	rVV	1327	1054	0.06%	0.008%
89	13.437	3835	3840	3842	rBV2	1219	1206	0.07%	0.009%
90	13.623	3895	3898	3902	rBV2	840	828	0.05%	0.006%
91	13.672	3910	3913	3922	rBV2	1011	1157	0.07%	0.008%
92	13.765	3928	3942	3946	rBV2	5344	9253	0.55%	0.068%
93	13.926	3988	3992	3996	rBV2	1257	1297	0.08%	0.009%
94	14.167	4064	4067	4070	rVB2	1448	891	0.05%	0.007%
95	14.353	4118	4125	4127	rBV	1404	1524	0.09%	0.011%
96	14.434	4146	4150	4153	rBV	1790	1462	0.09%	0.011%
97	14.967	4313	4316	4319	rBV2	1277	915	0.05%	0.007%
98	15.009	4326	4329	4331	rBV	1581	958	0.06%	0.007%
99	15.678	4530	4537	4540	rBV3	1930	2568	0.15%	0.019%
100	16.022	4641	4644	4646	rBV	2004	1125	0.07%	0.008%


Sum of corrected areas: 13677733

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030311.D
Acq On : 22 Mar 2019 16:25
Operator : JC/SP
Sample : VU0322WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

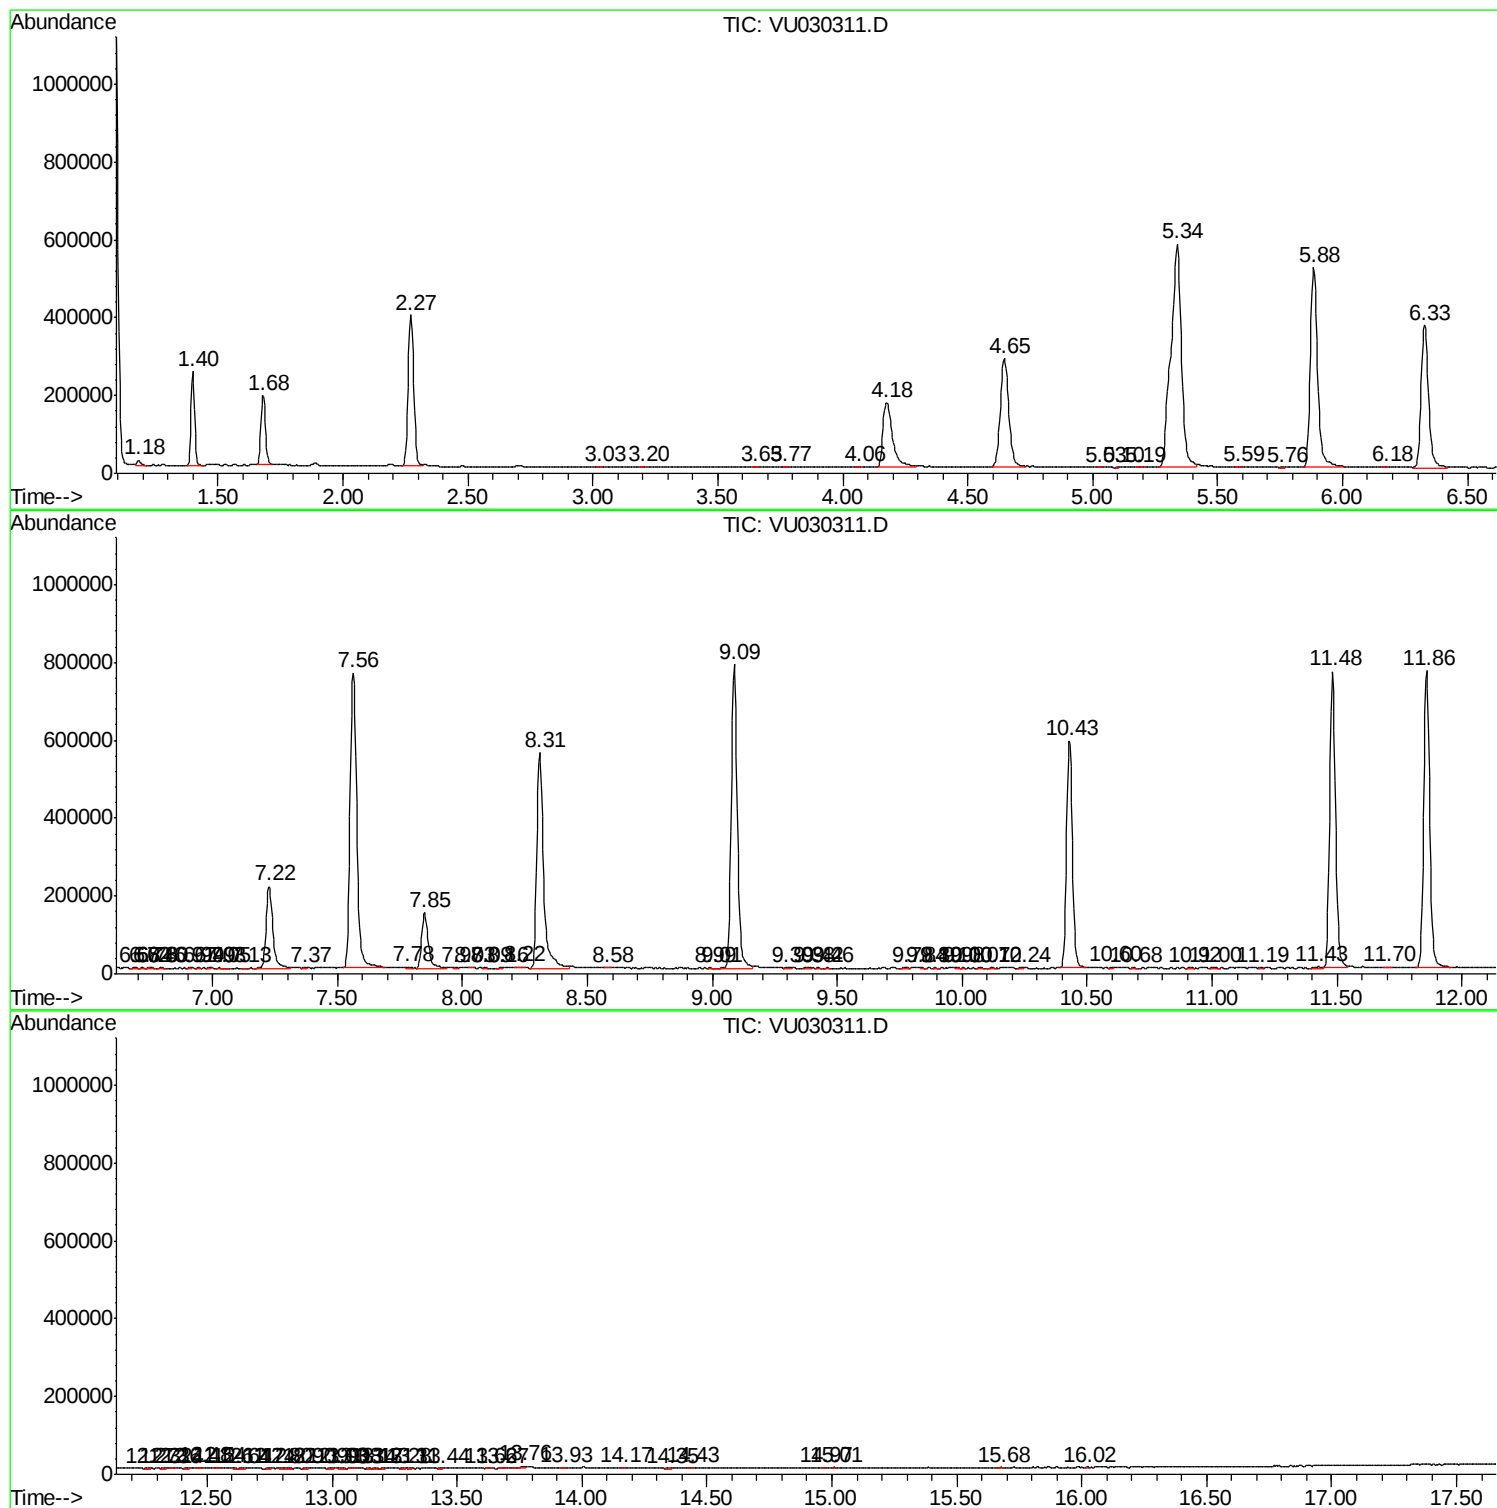

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030311.D
Acq On : 22 Mar 2019 16:25
Operator : JC/SP
Sample : VU0322WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030311.D
Acq On : 22 Mar 2019 16:25
Operator : JC/SP
Sample : VU0322WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc