

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030314.D
 Acq On : 22 Mar 2019 17:34
 Operator : JC/SP
 Sample : K2062-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB3	11599	11677	0.74%	0.088%
2	1.399	89	96	109	rBV	205194	204747	12.98%	1.545%
3	1.682	176	184	198	rVB	164498	207708	13.17%	1.567%
4	2.010	279	286	297	rVB	27262	40688	2.58%	0.307%
5	2.270	357	367	380	rBV	339265	515889	32.70%	3.892%
6	2.447	412	422	440	rVB2	25290	50840	3.22%	0.384%
7	2.566	456	459	463	rBV	1562	1465	0.09%	0.011%
8	2.698	493	500	505	rBV2	3659	4495	0.28%	0.034%
9	2.842	539	545	553	rVB3	2289	3484	0.22%	0.026%
10	2.968	581	584	588	rBV	1152	1068	0.07%	0.008%
11	3.161	639	644	646	rBV	940	1007	0.06%	0.008%
12	3.199	653	656	661	rBV	1352	1573	0.10%	0.012%
13	3.309	687	690	694	rBV	1371	1206	0.08%	0.009%
14	3.344	699	701	705	rVB	1774	1112	0.07%	0.008%
15	3.485	742	745	748	rVB2	1346	853	0.05%	0.006%
16	3.530	754	759	763	rBV	1584	1773	0.11%	0.013%
17	3.598	776	780	783	rBV	1206	906	0.06%	0.007%
18	3.672	800	803	807	rVB	1704	1313	0.08%	0.010%
19	3.784	835	838	841	rBV	1064	804	0.05%	0.006%
20	3.981	896	899	904	rVB	1653	1330	0.08%	0.010%
21	4.006	904	907	912	rBV	1738	1875	0.12%	0.014%
22	4.177	948	960	994	rBV	157052	425848	26.99%	3.213%
23	4.408	1029	1032	1037	rBV	1266	961	0.06%	0.007%
24	4.489	1052	1057	1060	rBV	1183	1161	0.07%	0.009%
25	4.646	1091	1106	1130	rBV	265457	630595	39.97%	4.757%
26	4.868	1172	1175	1179	rBV2	1137	1178	0.07%	0.009%
27	5.051	1229	1232	1236	rBV2	1241	863	0.05%	0.007%
28	5.212	1278	1282	1285	rVB	1444	1092	0.07%	0.008%
29	5.244	1285	1292	1297	rBV	1447	2151	0.14%	0.016%
30	5.337	1297	1321	1349	rBV2	527095	1577519	100.00%	11.901%
31	5.534	1379	1382	1387	rVB	2003	1480	0.09%	0.011%
32	5.778	1455	1458	1460	rBV	1466	1027	0.07%	0.008%
33	5.884	1478	1491	1526	rBV	546116	1120527	71.03%	8.454%
34	6.247	1600	1604	1612	rVB	1240	1932	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030314.D
 Acq On : 22 Mar 2019 17:34
 Operator : JC/SP
 Sample : K2062-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1612	1629	1651	rBV	350936	720918	45.70%	5.439%
36	6.691	1739	1742	1746	rVB	1079	832	0.05%	0.006%
37	6.910	1807	1810	1815	rBV	1407	1200	0.08%	0.009%
38	6.987	1831	1834	1841	rVB	2170	2309	0.15%	0.017%
39	7.019	1841	1844	1846	rBV	1589	1143	0.07%	0.009%
40	7.048	1850	1853	1859	rVB2	1634	1629	0.10%	0.012%
41	7.080	1859	1863	1868	rBV	2147	2525	0.16%	0.019%
42	7.119	1872	1875	1878	rVB	1270	935	0.06%	0.007%
43	7.154	1878	1886	1890	rBV	2389	3379	0.21%	0.025%
44	7.225	1895	1908	1935	rBV	190117	359068	22.76%	2.709%
45	7.363	1948	1951	1956	rVB	2140	1566	0.10%	0.012%
46	7.389	1956	1959	1964	rBV3	1440	1386	0.09%	0.010%
47	7.562	2000	2013	2056	rBV	678852	1258162	79.76%	9.492%
48	7.849	2087	2102	2126	rBV	128504	243259	15.42%	1.835%
49	7.987	2142	2145	2151	rVB3	1261	1013	0.06%	0.008%
50	8.176	2193	2204	2214	rBV4	11853	23502	1.49%	0.177%
51	8.222	2214	2218	2219	rBV	2195	1437	0.09%	0.011%
52	8.308	2234	2245	2286	rVV	504772	961159	60.93%	7.251%
53	8.675	2350	2359	2373	rVB6	6022	13987	0.89%	0.106%
54	8.730	2373	2376	2377	rBV	1575	954	0.06%	0.007%
55	8.775	2384	2390	2393	rBV	1197	1196	0.08%	0.009%
56	8.865	2412	2418	2423	rBV	1540	1872	0.12%	0.014%
57	8.951	2440	2445	2449	rBV2	1428	1269	0.08%	0.010%
58	9.086	2475	2487	2514	rBV	790463	1378656	87.39%	10.401%
59	9.273	2540	2545	2548	rVB	1380	1227	0.08%	0.009%
60	9.357	2566	2571	2573	rBV	1161	1096	0.07%	0.008%
61	9.463	2601	2604	2609	rVB2	1149	887	0.06%	0.007%
62	9.488	2609	2612	2614	rBV	1282	942	0.06%	0.007%
63	9.636	2654	2658	2659	rBV	1620	1135	0.07%	0.009%
64	9.713	2679	2682	2687	rVB	1494	1103	0.07%	0.008%
65	9.758	2693	2696	2703	rBV2	1727	2220	0.14%	0.017%
66	9.922	2742	2747	2752	rBV	1657	2101	0.13%	0.016%
67	10.016	2772	2776	2781	rBV2	1057	1031	0.07%	0.008%
68	10.077	2790	2795	2797	rBV	1228	1115	0.07%	0.008%
69	10.115	2803	2807	2811	rBV	1205	1219	0.08%	0.009%
70	10.170	2818	2824	2830	rVB2	1329	1406	0.09%	0.011%
71	10.279	2855	2858	2863	rBV2	1478	982	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030314.D
 Acq On : 22 Mar 2019 17:34
 Operator : JC/SP
 Sample : K2062-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.427	2892	2904	2928	rVV	554924	917910	58.19%	6.925%
73	10.604	2947	2959	2969	rBV4	13036	24650	1.56%	0.186%
74	10.691	2980	2986	2988	rBV2	859	916	0.06%	0.007%
75	10.736	2994	3000	3001	rBV	1129	1119	0.07%	0.008%
76	10.765	3005	3009	3014	rBV2	1187	1160	0.07%	0.009%
77	10.816	3021	3025	3028	rVB	1064	789	0.05%	0.006%
78	10.842	3028	3033	3036	rBV2	1161	1173	0.07%	0.009%
79	10.884	3042	3046	3050	rBV	1925	1498	0.09%	0.011%
80	10.913	3050	3055	3057	rBV2	1052	808	0.05%	0.006%
81	10.958	3066	3069	3075	rVB	1159	1133	0.07%	0.009%
82	11.032	3085	3092	3095	rBV	1454	1882	0.12%	0.014%
83	11.083	3104	3108	3114	rBV	1174	1415	0.09%	0.011%
84	11.241	3150	3157	3160	rBV	1801	1810	0.11%	0.014%
85	11.344	3186	3189	3196	rVB2	1536	1432	0.09%	0.011%
86	11.482	3219	3232	3249	rBV	782163	1265642	80.23%	9.548%
87	11.858	3337	3349	3375	rBV	710877	1191917	75.56%	8.992%
88	12.437	3526	3529	3532	rVB	1320	860	0.05%	0.006%
89	12.475	3533	3541	3542	rBV2	4384	4203	0.27%	0.032%
90	12.906	3670	3675	3676	rBV2	1500	1322	0.08%	0.010%
91	13.385	3821	3824	3828	rBV	1505	1418	0.09%	0.011%
92	13.424	3834	3836	3839	rVB	1580	875	0.06%	0.007%
93	13.729	3929	3931	3934	rBV	1430	859	0.05%	0.006%
94	13.781	3945	3947	3952	rBV2	918	846	0.05%	0.006%
95	14.800	4261	4264	4268	rVB2	1597	1196	0.08%	0.009%
96	14.922	4299	4302	4304	rBV	1423	902	0.06%	0.007%
97	14.970	4313	4317	4322	rBV2	1667	1874	0.12%	0.014%
98	15.070	4345	4348	4355	rBV2	1671	1461	0.09%	0.011%
99	15.504	4480	4483	4485	rBV2	1826	1116	0.07%	0.008%
100	15.601	4510	4513	4515	rBV	1363	854	0.05%	0.006%


Sum of corrected areas: 13255007

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030314.D
Acq On : 22 Mar 2019 17:34
Operator : JC/SP
Sample : K2062-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

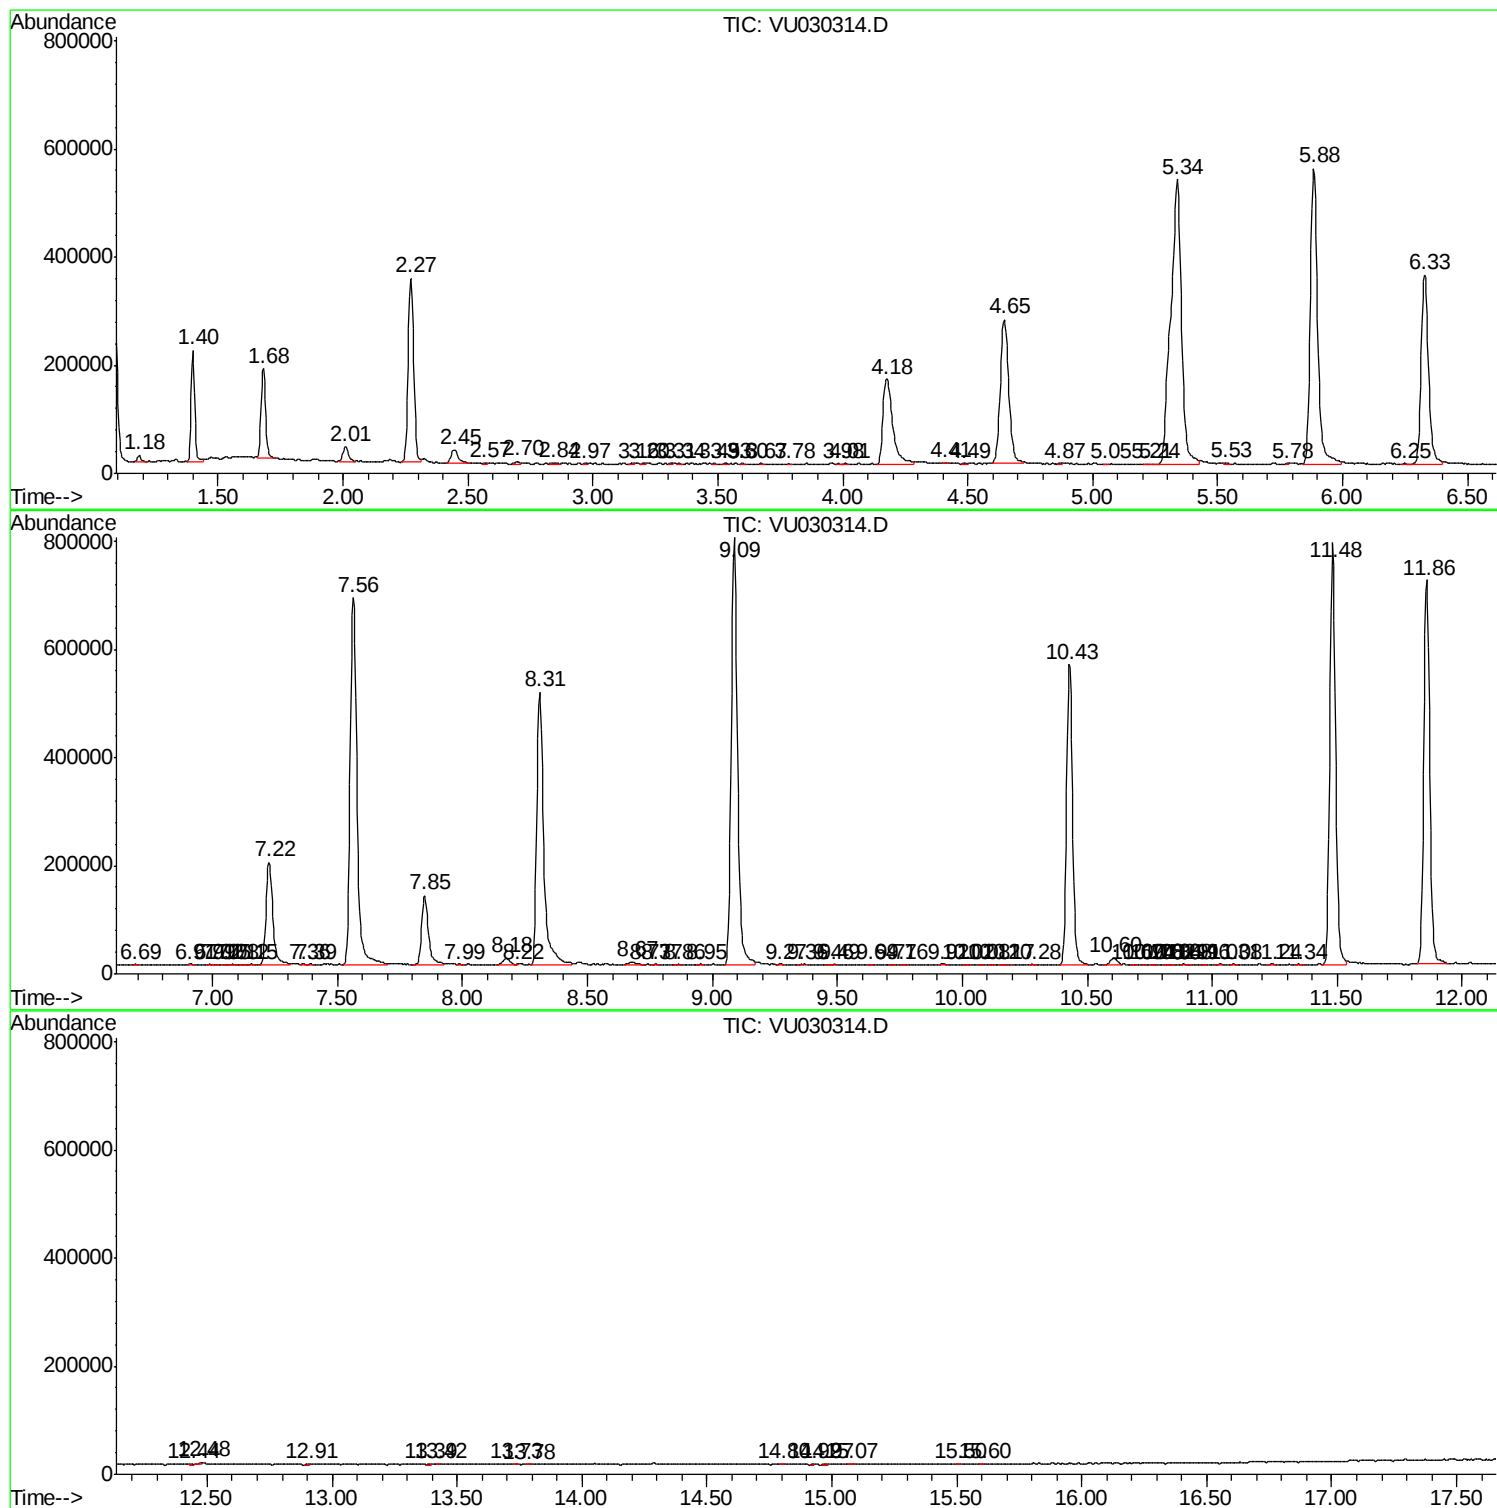

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030314.D
Acq On : 22 Mar 2019 17:34
Operator : JC/SP
Sample : K2062-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030314.D
Acq On : 22 Mar 2019 17:34
Operator : JC/SP
Sample : K2062-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc