

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030317.D
 Acq On : 22 Mar 2019 18:43
 Operator : JC/SP
 Sample : K2048-06 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	38	rBV2	14581	14609	0.82%	0.095%
2	1.399	89	96	105	rBV	225057	228115	12.76%	1.486%
3	1.678	175	183	199	rVB	160956	215129	12.04%	1.401%
4	2.270	357	367	378	rBV	364583	549026	30.72%	3.576%
5	2.807	532	534	536	rBV	1264	811	0.05%	0.005%
6	4.177	948	960	994	rBV3	164624	578277	32.36%	3.766%
7	4.646	1091	1106	1127	rBV	266119	638041	35.70%	4.155%
8	4.881	1175	1179	1185	rBV4	1624	1909	0.11%	0.012%
9	4.981	1207	1210	1213	rBV	1662	1360	0.08%	0.009%
10	5.051	1229	1232	1237	rVB	1439	1106	0.06%	0.007%
11	5.080	1237	1241	1244	rBV	1032	1035	0.06%	0.007%
12	5.116	1248	1252	1257	rVV	1564	1454	0.08%	0.009%
13	5.141	1257	1260	1264	rVV2	838	749	0.04%	0.005%
14	5.337	1298	1321	1345	rBV2	547226	1616352	90.45%	10.527%
15	5.884	1478	1491	1525	rBV	556524	1123094	62.84%	7.315%
16	6.183	1570	1584	1615	rBV	913295	1787096	100.00%	11.639%
17	6.328	1616	1629	1662	rVB	362248	737965	41.29%	4.806%
18	6.572	1702	1705	1710	rVB	1537	1107	0.06%	0.007%
19	6.601	1710	1714	1719	rBV	1281	1261	0.07%	0.008%
20	6.726	1749	1753	1756	rVV2	872	808	0.05%	0.005%
21	6.749	1756	1760	1763	rVV	871	822	0.05%	0.005%
22	6.900	1803	1807	1811	rVV3	1092	997	0.06%	0.006%
23	6.923	1811	1814	1816	rVV	1061	814	0.05%	0.005%
24	6.987	1829	1834	1840	rVB	1554	1851	0.10%	0.012%
25	7.022	1840	1845	1848	rBV	1422	1472	0.08%	0.010%
26	7.061	1853	1857	1862	rVB2	1281	1320	0.07%	0.009%
27	7.099	1866	1869	1873	rVB2	973	771	0.04%	0.005%
28	7.122	1873	1876	1879	rBV	837	712	0.04%	0.005%
29	7.225	1897	1908	1930	rBV	194805	361385	20.22%	2.354%
30	7.389	1956	1959	1962	rBV2	993	908	0.05%	0.006%
31	7.444	1970	1976	1978	rBV2	1321	1451	0.08%	0.009%
32	7.482	1984	1988	1994	rVB2	1180	1428	0.08%	0.009%
33	7.562	1998	2013	2040	rBV	718502	1297889	72.63%	8.453%
34	7.717	2057	2061	2064	rBV4	1206	812	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030317.D
 Acq On : 22 Mar 2019 18:43
 Operator : JC/SP
 Sample : K2048-06 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.759	2071	2074	2078	rBV	1209	1056	0.06%	0.007%
36	7.797	2083	2086	2091	rVB	2051	1737	0.10%	0.011%
37	7.849	2091	2102	2129	rBV	136043	250108	14.00%	1.629%
38	8.019	2153	2155	2157	rBV2	1271	767	0.04%	0.005%
39	8.173	2199	2203	2205	rBV2	2005	1799	0.10%	0.012%
40	8.228	2212	2220	2230	rBV4	6192	9993	0.56%	0.065%
41	8.308	2232	2245	2273	rBV	543250	987014	55.23%	6.428%
42	8.562	2321	2324	2331	rVB2	1068	842	0.05%	0.005%
43	8.697	2364	2366	2371	rVB	1513	915	0.05%	0.006%
44	8.736	2375	2378	2383	rVV2	763	781	0.04%	0.005%
45	8.829	2402	2407	2411	rBV3	766	726	0.04%	0.005%
46	8.861	2411	2417	2426	rVB3	1137	1576	0.09%	0.010%
47	8.900	2426	2429	2434	rBV2	874	656	0.04%	0.004%
48	9.087	2473	2487	2512	rBV	819742	1405372	78.64%	9.153%
49	9.241	2533	2535	2543	rVB3	1375	1213	0.07%	0.008%
50	9.279	2543	2547	2553	rVB	1550	1639	0.09%	0.011%
51	9.312	2553	2557	2562	rBV	926	1177	0.07%	0.008%
52	9.344	2562	2567	2570	rVB2	1135	1192	0.07%	0.008%
53	9.395	2580	2583	2593	rBV	1182	1959	0.11%	0.013%
54	9.466	2598	2605	2609	rBV	1044	928	0.05%	0.006%
55	9.521	2618	2622	2625	rVB2	889	765	0.04%	0.005%
56	9.636	2652	2658	2660	rBV	1055	1062	0.06%	0.007%
57	9.681	2669	2672	2676	rBV2	1162	907	0.05%	0.006%
58	9.720	2680	2684	2688	rVB	1531	1306	0.07%	0.009%
59	9.832	2714	2719	2720	rBV	1002	766	0.04%	0.005%
60	9.974	2760	2763	2769	rVB	1495	1212	0.07%	0.008%
61	10.006	2769	2773	2776	rBV	1478	1183	0.07%	0.008%
62	10.080	2793	2796	2801	rVB	1326	1029	0.06%	0.007%
63	10.180	2821	2827	2832	rBV3	898	1314	0.07%	0.009%
64	10.254	2844	2850	2854	rBV3	1249	1339	0.07%	0.009%
65	10.308	2863	2867	2871	rVB2	1439	1077	0.06%	0.007%
66	10.379	2883	2889	2891	rBV3	825	1009	0.06%	0.007%
67	10.427	2892	2904	2925	rVB	581673	930730	52.08%	6.062%
68	10.607	2952	2960	2969	rVB5	3263	5537	0.31%	0.036%
69	10.730	2996	2998	3002	rVB	1147	687	0.04%	0.004%
70	10.752	3002	3005	3010	rBV2	1251	987	0.06%	0.006%
71	10.820	3023	3026	3031	rVB	1637	1517	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030317.D
 Acq On : 22 Mar 2019 18:43
 Operator : JC/SP
 Sample : K2048-06 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF198

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.858	3031	3038	3041	rBV2	1590	1917	0.11%	0.012%
73	10.958	3061	3069	3071	rBV2	2067	2226	0.12%	0.014%
74	11.086	3105	3109	3117	rVB2	1677	2034	0.11%	0.013%
75	11.128	3117	3122	3124	rBV2	1135	1101	0.06%	0.007%
76	11.340	3185	3188	3193	rVB	1391	989	0.06%	0.006%
77	11.379	3193	3200	3204	rBV3	1580	2336	0.13%	0.015%
78	11.482	3220	3232	3253	rBV	790742	1295011	72.46%	8.434%
79	11.807	3328	3333	3335	rBV3	1063	1165	0.07%	0.008%
80	11.858	3336	3349	3373	rVV	727475	1226444	68.63%	7.988%
81	12.299	3482	3486	3489	rBV2	1431	1099	0.06%	0.007%
82	12.366	3501	3507	3512	rVB	1716	2289	0.13%	0.015%
83	12.398	3512	3517	3520	rBV3	961	1073	0.06%	0.007%
84	12.443	3528	3531	3537	rBV3	1086	1322	0.07%	0.009%
85	12.524	3552	3556	3558	rBV	1627	1132	0.06%	0.007%
86	12.617	3579	3585	3589	rBV	1429	1664	0.09%	0.011%
87	12.710	3612	3614	3617	rVB	1349	711	0.04%	0.005%
88	12.823	3646	3649	3655	rVV2	1425	1383	0.08%	0.009%
89	12.881	3664	3667	3671	rBV	1197	932	0.05%	0.006%
90	13.012	3705	3708	3709	rBV	994	634	0.04%	0.004%
91	13.247	3775	3781	3786	rBV2	1357	1856	0.10%	0.012%
92	13.318	3799	3803	3807	rVB	1701	1502	0.08%	0.010%
93	13.344	3807	3811	3813	rBV2	1442	1211	0.07%	0.008%
94	13.430	3835	3838	3841	rBV	1235	1030	0.06%	0.007%
95	13.588	3882	3887	3890	rBV2	1579	1587	0.09%	0.010%
96	13.662	3907	3910	3913	rBV2	948	743	0.04%	0.005%
97	13.816	3955	3958	3962	rBV	1662	1496	0.08%	0.010%
98	14.016	4017	4020	4023	rVV	1509	890	0.05%	0.006%
99	14.038	4024	4027	4030	rVB2	1358	900	0.05%	0.006%
100	14.514	4169	4175	4178	rBV2	1537	1813	0.10%	0.012%


Sum of corrected areas: 15354303

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030317.D
Acq On : 22 Mar 2019 18:43
Operator : JC/SP
Sample : K2048-06 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

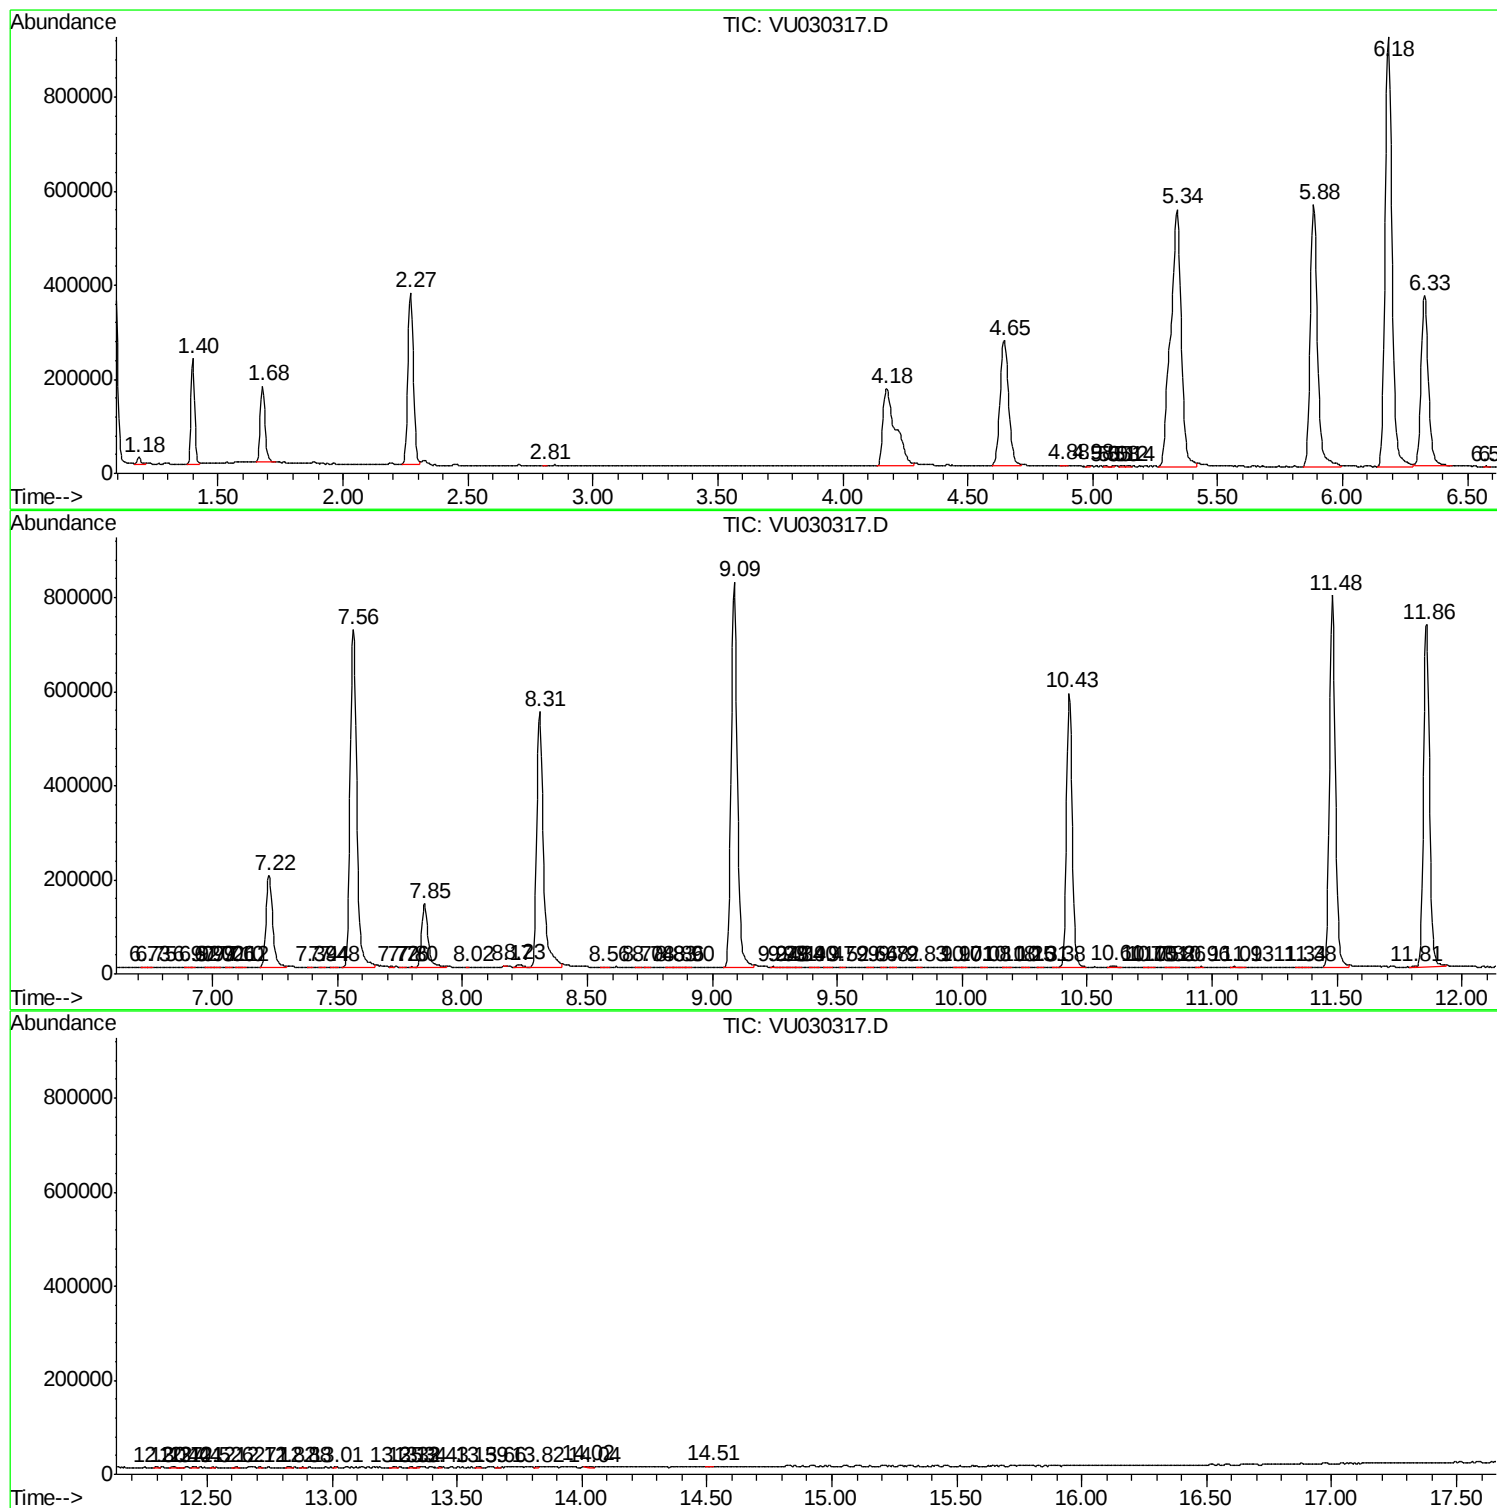

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030317.D
Acq On : 22 Mar 2019 18:43
Operator : JC/SP
Sample : K2048-06 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030317.D
Acq On : 22 Mar 2019 18:43
Operator : JC/SP
Sample : K2048-06 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF198

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc