

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030323.D
 Acq On : 22 Mar 2019 21:00
 Operator : JC/SP
 Sample : K2048-08 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rVB3	12949	12121	0.41%	0.074%
2	1.399	89	96	106	rBV	212211	216548	7.38%	1.323%
3	1.678	176	183	197	rVB	166229	209435	7.14%	1.279%
4	2.270	357	367	379	rBV	355520	537166	18.31%	3.281%
5	2.547	446	453	455	rBV	942	1083	0.04%	0.007%
6	2.659	484	488	495	rBV	949	1233	0.04%	0.008%
7	2.704	495	502	503	rBV5	2294	2425	0.08%	0.015%
8	2.759	516	519	523	rVB	1270	1077	0.04%	0.007%
9	2.923	567	570	573	rBV2	1062	975	0.03%	0.006%
10	2.981	582	588	594	rBV	2089	2019	0.07%	0.012%
11	3.016	594	599	605	rBV2	1085	1573	0.05%	0.010%
12	3.048	605	609	612	rVB2	950	905	0.03%	0.006%
13	3.148	637	640	648	rVB	1268	1260	0.04%	0.008%
14	3.389	713	715	724	rVB	1451	1547	0.05%	0.009%
15	3.431	724	728	732	rBV	2085	1856	0.06%	0.011%
16	3.460	733	737	741	rVB	1397	1063	0.04%	0.006%
17	3.508	747	752	756	rBV	1317	1203	0.04%	0.007%
18	3.772	827	834	838	rVB	2314	2914	0.10%	0.018%
19	3.797	838	842	848	rBV2	1289	1041	0.04%	0.006%
20	4.006	901	907	910	rBV2	1490	1672	0.06%	0.010%
21	4.048	917	920	923	rBV	1067	980	0.03%	0.006%
22	4.109	935	939	942	rBV	1191	1120	0.04%	0.007%
23	4.177	948	960	993	rBV	155250	500616	17.07%	3.058%
24	4.415	1031	1034	1038	rBV	1424	1078	0.04%	0.007%
25	4.440	1039	1042	1045	rVV	1859	1282	0.04%	0.008%
26	4.460	1045	1048	1052	rVB	1182	888	0.03%	0.005%
27	4.646	1090	1106	1129	rBV	266118	638435	21.76%	3.900%
28	4.846	1164	1168	1175	rVB	1467	2029	0.07%	0.012%
29	4.891	1175	1182	1185	rBV2	1884	2317	0.08%	0.014%
30	5.215	1277	1283	1287	rBV3	1058	1102	0.04%	0.007%
31	5.337	1297	1321	1360	rBV2	543413	1612828	54.98%	9.852%
32	5.675	1422	1426	1431	rBV3	975	1082	0.04%	0.007%
33	5.884	1474	1491	1518	rBV	561585	1143423	38.98%	6.985%
34	6.183	1569	1584	1614	rBV	1501922	2933581	100.00%	17.920%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030323.D
 Acq On : 22 Mar 2019 21:00
 Operator : JC/SP
 Sample : K2048-08 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.328	1617	1629	1654	rVB	355629	727707	24.81%	4.445%
36	6.733	1751	1755	1758	rBV	1643	1423	0.05%	0.009%
37	7.038	1846	1850	1856	rVB	1738	1497	0.05%	0.009%
38	7.080	1856	1863	1866	rBV2	1649	2101	0.07%	0.013%
39	7.144	1879	1883	1890	rBV3	864	971	0.03%	0.006%
40	7.225	1897	1908	1929	rBV	190586	351584	11.98%	2.148%
41	7.402	1956	1963	1968	rVB	960	1141	0.04%	0.007%
42	7.431	1968	1972	1975	rVB	1389	1093	0.04%	0.007%
43	7.476	1981	1986	1994	rVB	2077	2947	0.10%	0.018%
44	7.517	1994	1999	2000	rBV2	1802	1395	0.05%	0.009%
45	7.562	2000	2013	2052	rBV	703981	1282458	43.72%	7.834%
46	7.697	2052	2055	2060	rVV2	1643	1242	0.04%	0.008%
47	7.849	2091	2102	2123	rBV	129451	236489	8.06%	1.445%
48	8.132	2186	2190	2193	rBV	1595	1099	0.04%	0.007%
49	8.173	2195	2203	2211	rVV3	6478	10548	0.36%	0.064%
50	8.228	2211	2220	2234	rVB2	16569	28521	0.97%	0.174%
51	8.308	2234	2245	2284	rBV	516249	970177	33.07%	5.926%
52	8.537	2311	2316	2321	rBV2	1980	2513	0.09%	0.015%
53	8.768	2386	2388	2396	rVV2	1348	1577	0.05%	0.010%
54	8.881	2419	2423	2428	rBV2	1462	1556	0.05%	0.010%
55	9.086	2475	2487	2514	rBV	828726	1411220	48.11%	8.620%
56	9.279	2539	2547	2549	rBV	902	1124	0.04%	0.007%
57	9.321	2556	2560	2563	rBV	1440	1121	0.04%	0.007%
58	9.379	2575	2578	2581	rBV2	1359	1202	0.04%	0.007%
59	9.447	2596	2599	2602	rBV	1145	930	0.03%	0.006%
60	9.466	2602	2605	2607	rVV	1544	1034	0.04%	0.006%
61	9.781	2700	2703	2709	rVB	1274	1212	0.04%	0.007%
62	9.868	2725	2730	2736	rBV	1333	1716	0.06%	0.010%
63	9.935	2747	2751	2753	rBV	1136	937	0.03%	0.006%
64	10.131	2807	2812	2816	rBV2	1610	1850	0.06%	0.011%
65	10.286	2856	2860	2868	rVB	1469	2053	0.07%	0.013%
66	10.427	2889	2904	2923	rBV	569506	926406	31.58%	5.659%
67	10.604	2949	2959	2966	rBV2	5504	8359	0.28%	0.051%
68	10.742	2999	3002	3005	rBV	1187	970	0.03%	0.006%
69	10.813	3021	3024	3026	rBV	1386	914	0.03%	0.006%
70	10.836	3029	3031	3035	rVB	2221	1539	0.05%	0.009%
71	10.861	3035	3039	3046	rBV	1681	2436	0.08%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030323.D
 Acq On : 22 Mar 2019 21:00
 Operator : JC/SP
 Sample : K2048-08 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.932	3058	3061	3064	rVB	2420	1485	0.05%	0.009%
73	10.958	3064	3069	3072	rBV	1912	1578	0.05%	0.010%
74	11.318	3178	3181	3184	rBV	1253	1199	0.04%	0.007%
75	11.482	3219	3232	3259	rBV	777951	1307204	44.56%	7.985%
76	11.726	3305	3308	3316	rVB2	1551	2183	0.07%	0.013%
77	11.858	3335	3349	3369	rBV	716751	1195493	40.75%	7.303%
78	12.086	3417	3420	3424	rBV2	1320	1349	0.05%	0.008%
79	12.337	3494	3498	3502	rVV2	1646	1608	0.05%	0.010%
80	12.469	3536	3539	3542	rBV2	1458	1186	0.04%	0.007%
81	12.614	3580	3584	3586	rBV	1312	908	0.03%	0.006%
82	12.688	3602	3607	3610	rBV	1010	1172	0.04%	0.007%
83	12.720	3614	3617	3624	rVB2	945	964	0.03%	0.006%
84	12.842	3651	3655	3662	rBV	1920	2340	0.08%	0.014%
85	12.890	3666	3670	3673	rBV2	1211	1123	0.04%	0.007%
86	12.935	3680	3684	3688	rVB	1696	1233	0.04%	0.008%
87	13.115	3735	3740	3743	rBV	1681	1342	0.05%	0.008%
88	13.138	3743	3747	3753	rVV	968	996	0.03%	0.006%
89	13.167	3753	3756	3760	rBV	1334	964	0.03%	0.006%
90	13.450	3837	3844	3846	rBV2	1487	1814	0.06%	0.011%
91	13.601	3888	3891	3894	rBV	1345	1109	0.04%	0.007%
92	13.668	3907	3912	3915	rBV	1234	1137	0.04%	0.007%
93	13.710	3922	3925	3929	rBV	1391	1174	0.04%	0.007%
94	14.057	4030	4033	4036	rVB	1516	983	0.03%	0.006%
95	14.360	4123	4127	4130	rBV	1217	936	0.03%	0.006%
96	14.424	4142	4147	4151	rBV2	1754	1483	0.05%	0.009%
97	14.565	4188	4191	4194	rBV	1789	1262	0.04%	0.008%
98	14.688	4226	4229	4233	rVB2	1588	1483	0.05%	0.009%
99	14.755	4247	4250	4254	rVB2	1276	1041	0.04%	0.006%
100	14.784	4255	4259	4260	rBV	1322	899	0.03%	0.005%


Sum of corrected areas: 16370587

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030323.D
Acq On : 22 Mar 2019 21:00
Operator : JC/SP
Sample : K2048-08 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

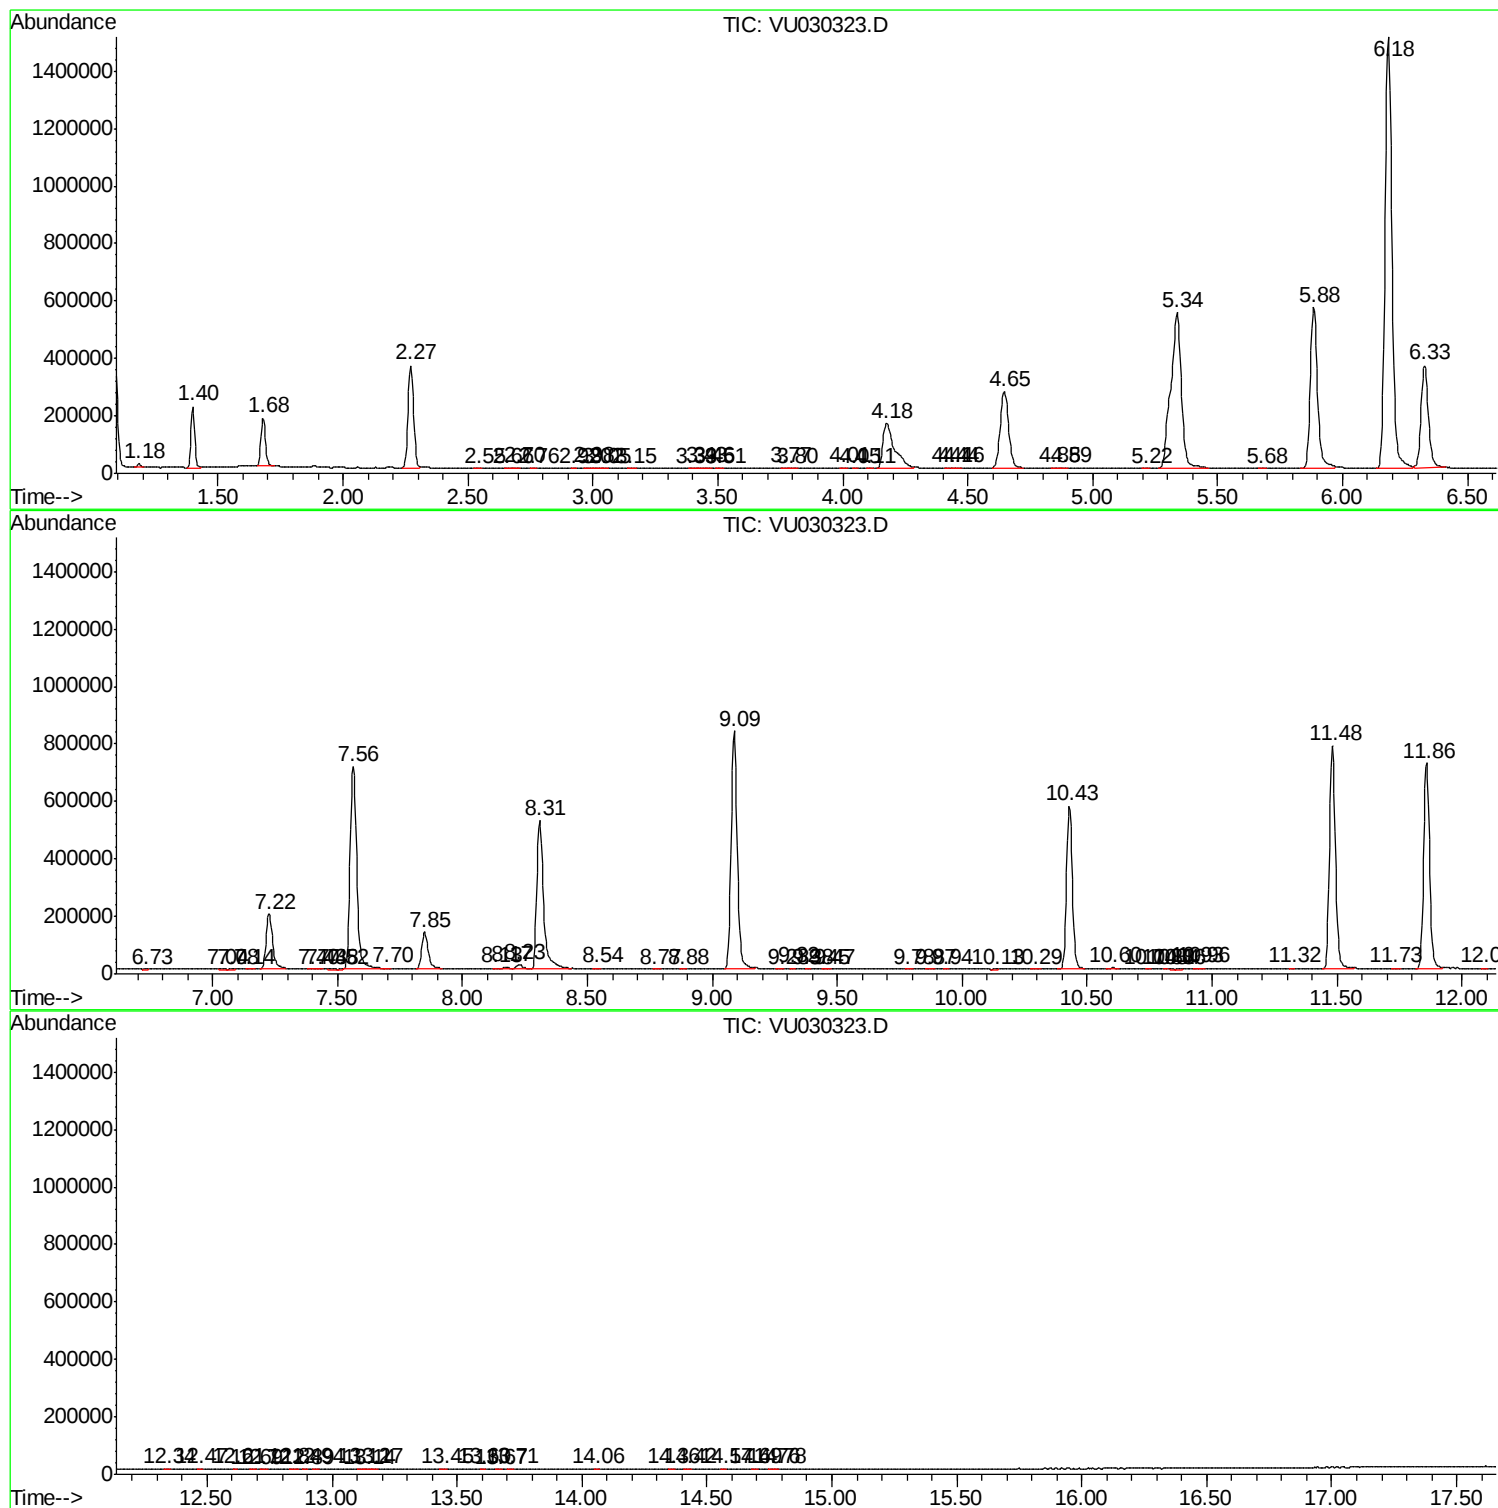

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030323.D
Acq On : 22 Mar 2019 21:00
Operator : JC/SP
Sample : K2048-08 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030323.D
Acq On : 22 Mar 2019 21:00
Operator : JC/SP
Sample : K2048-08 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc