

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030325.D
 Acq On : 22 Mar 2019 21:46
 Operator : JC/SP
 Sample : K2062-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	13129	12364	0.78%	0.093%
2	1.399	89	96	105	rBV	206037	203327	12.86%	1.532%
3	1.682	176	184	200	rVB	161836	208577	13.19%	1.572%
4	2.270	357	367	381	rBV	341237	515246	32.59%	3.883%
5	2.582	458	464	469	rVB	2038	2079	0.13%	0.016%
6	2.694	495	499	500	rBV	1676	1140	0.07%	0.009%
7	2.749	511	516	518	rBV	1050	974	0.06%	0.007%
8	2.765	518	521	525	rVB2	1307	1164	0.07%	0.009%
9	2.820	532	538	544	rBV2	2121	3281	0.21%	0.025%
10	2.874	551	555	557	rBV2	1331	1011	0.06%	0.008%
11	3.071	611	616	620	rBV2	1958	1835	0.12%	0.014%
12	3.177	643	649	654	rBV	1308	1606	0.10%	0.012%
13	3.215	658	661	663	rBV	1238	942	0.06%	0.007%
14	3.386	710	714	716	rBV	1112	1012	0.06%	0.008%
15	3.656	792	798	801	rBV	1545	1881	0.12%	0.014%
16	3.701	808	812	814	rBV	1325	952	0.06%	0.007%
17	3.932	879	884	887	rBV	1309	1216	0.08%	0.009%
18	3.977	893	898	900	rBV	1053	906	0.06%	0.007%
19	4.026	908	913	919	rVB2	1228	1361	0.09%	0.010%
20	4.071	919	927	929	rBV2	850	1032	0.07%	0.008%
21	4.177	947	960	993	rBV	165283	442423	27.98%	3.334%
22	4.527	1064	1069	1073	rBV	1048	1264	0.08%	0.010%
23	4.646	1090	1106	1128	rVV	264144	625615	39.57%	4.715%
24	4.865	1169	1174	1177	rBV4	1130	1026	0.06%	0.008%
25	4.887	1178	1181	1184	rVV2	1218	860	0.05%	0.006%
26	5.067	1233	1237	1240	rBV2	1114	1080	0.07%	0.008%
27	5.193	1272	1276	1279	rVB	1355	921	0.06%	0.007%
28	5.212	1279	1282	1289	rVB	1770	2043	0.13%	0.015%
29	5.337	1298	1321	1358	rBV2	531930	1581198	100.00%	11.916%
30	5.620	1404	1409	1414	rBV5	853	1155	0.07%	0.009%
31	5.884	1478	1491	1520	rBV	540063	1092034	69.06%	8.230%
32	6.186	1572	1585	1602	rBV	104498	207910	13.15%	1.567%
33	6.328	1615	1629	1662	rVB	347903	706217	44.66%	5.322%
34	6.749	1756	1760	1762	rBV	1165	964	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030325.D
 Acq On : 22 Mar 2019 21:46
 Operator : JC/SP
 Sample : K2062-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	6.865	1790	1796	1802	rBV	1043	1211	0.08%	0.009%
36	6.900	1802	1807	1812	rBV4	1393	1770	0.11%	0.013%
37	6.929	1813	1816	1824	rVB	1587	1749	0.11%	0.013%
38	6.968	1824	1828	1832	rBV	2004	2393	0.15%	0.018%
39	7.067	1856	1859	1863	rVV	1416	952	0.06%	0.007%
40	7.173	1887	1892	1896	rBV2	1024	1132	0.07%	0.009%
41	7.225	1896	1908	1935	rVV	183631	345000	21.82%	2.600%
42	7.437	1971	1974	1978	rBV2	1164	932	0.06%	0.007%
43	7.562	1996	2013	2047	rBV	681455	1244516	78.71%	9.379%
44	7.765	2073	2076	2080	rVB	1719	1190	0.08%	0.009%
45	7.784	2080	2082	2087	rVB	1738	1320	0.08%	0.010%
46	7.848	2087	2102	2125	rBV	129150	236307	14.94%	1.781%
47	8.109	2179	2183	2187	rBV	1146	1331	0.08%	0.010%
48	8.183	2197	2206	2210	rBV4	1918	3132	0.20%	0.024%
49	8.228	2213	2220	2226	rVV6	2468	3529	0.22%	0.027%
50	8.308	2234	2245	2283	rBV	537727	996401	63.02%	7.509%
51	8.594	2330	2334	2336	rBV	1102	779	0.05%	0.006%
52	8.633	2341	2346	2348	rBV2	1668	1786	0.11%	0.013%
53	8.983	2448	2455	2461	rBV	1657	2225	0.14%	0.017%
54	9.086	2475	2487	2516	rBV	810910	1375529	86.99%	10.366%
55	9.328	2554	2562	2565	rVB	1888	2433	0.15%	0.018%
56	9.437	2594	2596	2603	rVB2	2074	2184	0.14%	0.016%
57	9.472	2603	2607	2612	rBV	1020	1253	0.08%	0.009%
58	9.504	2612	2617	2619	rBV	1239	962	0.06%	0.007%
59	9.610	2647	2650	2654	rVB	1210	769	0.05%	0.006%
60	9.643	2654	2660	2661	rBV	1524	1306	0.08%	0.010%
61	9.906	2738	2742	2749	rVB2	977	1081	0.07%	0.008%
62	9.942	2749	2753	2763	rBV2	1454	2059	0.13%	0.016%
63	9.996	2764	2770	2774	rBV2	1178	1243	0.08%	0.009%
64	10.051	2785	2787	2793	rVB3	1238	1092	0.07%	0.008%
65	10.093	2797	2800	2805	rVB	1342	927	0.06%	0.007%
66	10.118	2805	2808	2812	rVB	1697	1175	0.07%	0.009%
67	10.147	2812	2817	2819	rBV2	942	1024	0.06%	0.008%
68	10.260	2845	2852	2854	rBV	846	976	0.06%	0.007%
69	10.302	2860	2865	2869	rBV	1628	1499	0.09%	0.011%
70	10.427	2888	2904	2930	rVV	566884	930267	58.83%	7.011%
71	10.520	2930	2933	2937	rVB	1769	1129	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030325.D
 Acq On : 22 Mar 2019 21:46
 Operator : JC/SP
 Sample : K2062-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	10.601	2954	2958	2960	rBV	1089	958	0.06%	0.007%
73	10.922	3053	3058	3061	rBV	1170	931	0.06%	0.007%
74	11.173	3132	3136	3138	rBV	1505	1113	0.07%	0.008%
75	11.241	3155	3157	3164	rVB	1246	1284	0.08%	0.010%
76	11.340	3185	3188	3201	rVB2	1145	2056	0.13%	0.015%
77	11.482	3220	3232	3256	rVV	765072	1253928	79.30%	9.450%
78	11.614	3271	3273	3277	rVB	2006	1315	0.08%	0.010%
79	11.720	3302	3306	3310	rBV2	1327	1416	0.09%	0.011%
80	11.803	3321	3332	3335	rBV	1497	2175	0.14%	0.016%
81	11.858	3335	3349	3366	rBV	711537	1175180	74.32%	8.856%
82	12.302	3482	3487	3490	rBV	934	952	0.06%	0.007%
83	12.321	3490	3493	3496	rVV	1674	1529	0.10%	0.012%
84	12.395	3511	3516	3519	rBV	984	1181	0.07%	0.009%
85	12.437	3525	3529	3533	rBV2	1357	1341	0.08%	0.010%
86	12.475	3537	3541	3547	rVB3	2187	2519	0.16%	0.019%
87	12.507	3547	3551	3553	rBV	1417	983	0.06%	0.007%
88	12.678	3599	3604	3609	rVB2	1168	1312	0.08%	0.010%
89	12.710	3609	3614	3616	rBV	880	861	0.05%	0.006%
90	12.832	3646	3652	3655	rBV2	1777	2036	0.13%	0.015%
91	12.861	3658	3661	3666	rVB2	1527	1369	0.09%	0.010%
92	12.970	3691	3695	3704	rBV2	1414	2251	0.14%	0.017%
93	13.028	3710	3713	3717	rBV2	1717	1693	0.11%	0.013%
94	13.141	3745	3748	3751	rBV2	1301	860	0.05%	0.006%
95	13.270	3785	3788	3794	rBV	1261	1360	0.09%	0.010%
96	13.501	3857	3860	3866	rVB	1280	1453	0.09%	0.011%
97	13.758	3937	3940	3945	rBV	879	890	0.06%	0.007%
98	14.196	4073	4076	4081	rBV	1205	1007	0.06%	0.008%
99	14.498	4164	4170	4173	rBV2	1485	1804	0.11%	0.014%
100	14.755	4247	4250	4256	rBV	2228	2399	0.15%	0.018%


Sum of corrected areas: 13269335

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030325.D
Acq On : 22 Mar 2019 21:46
Operator : JC/SP
Sample : K2062-07 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

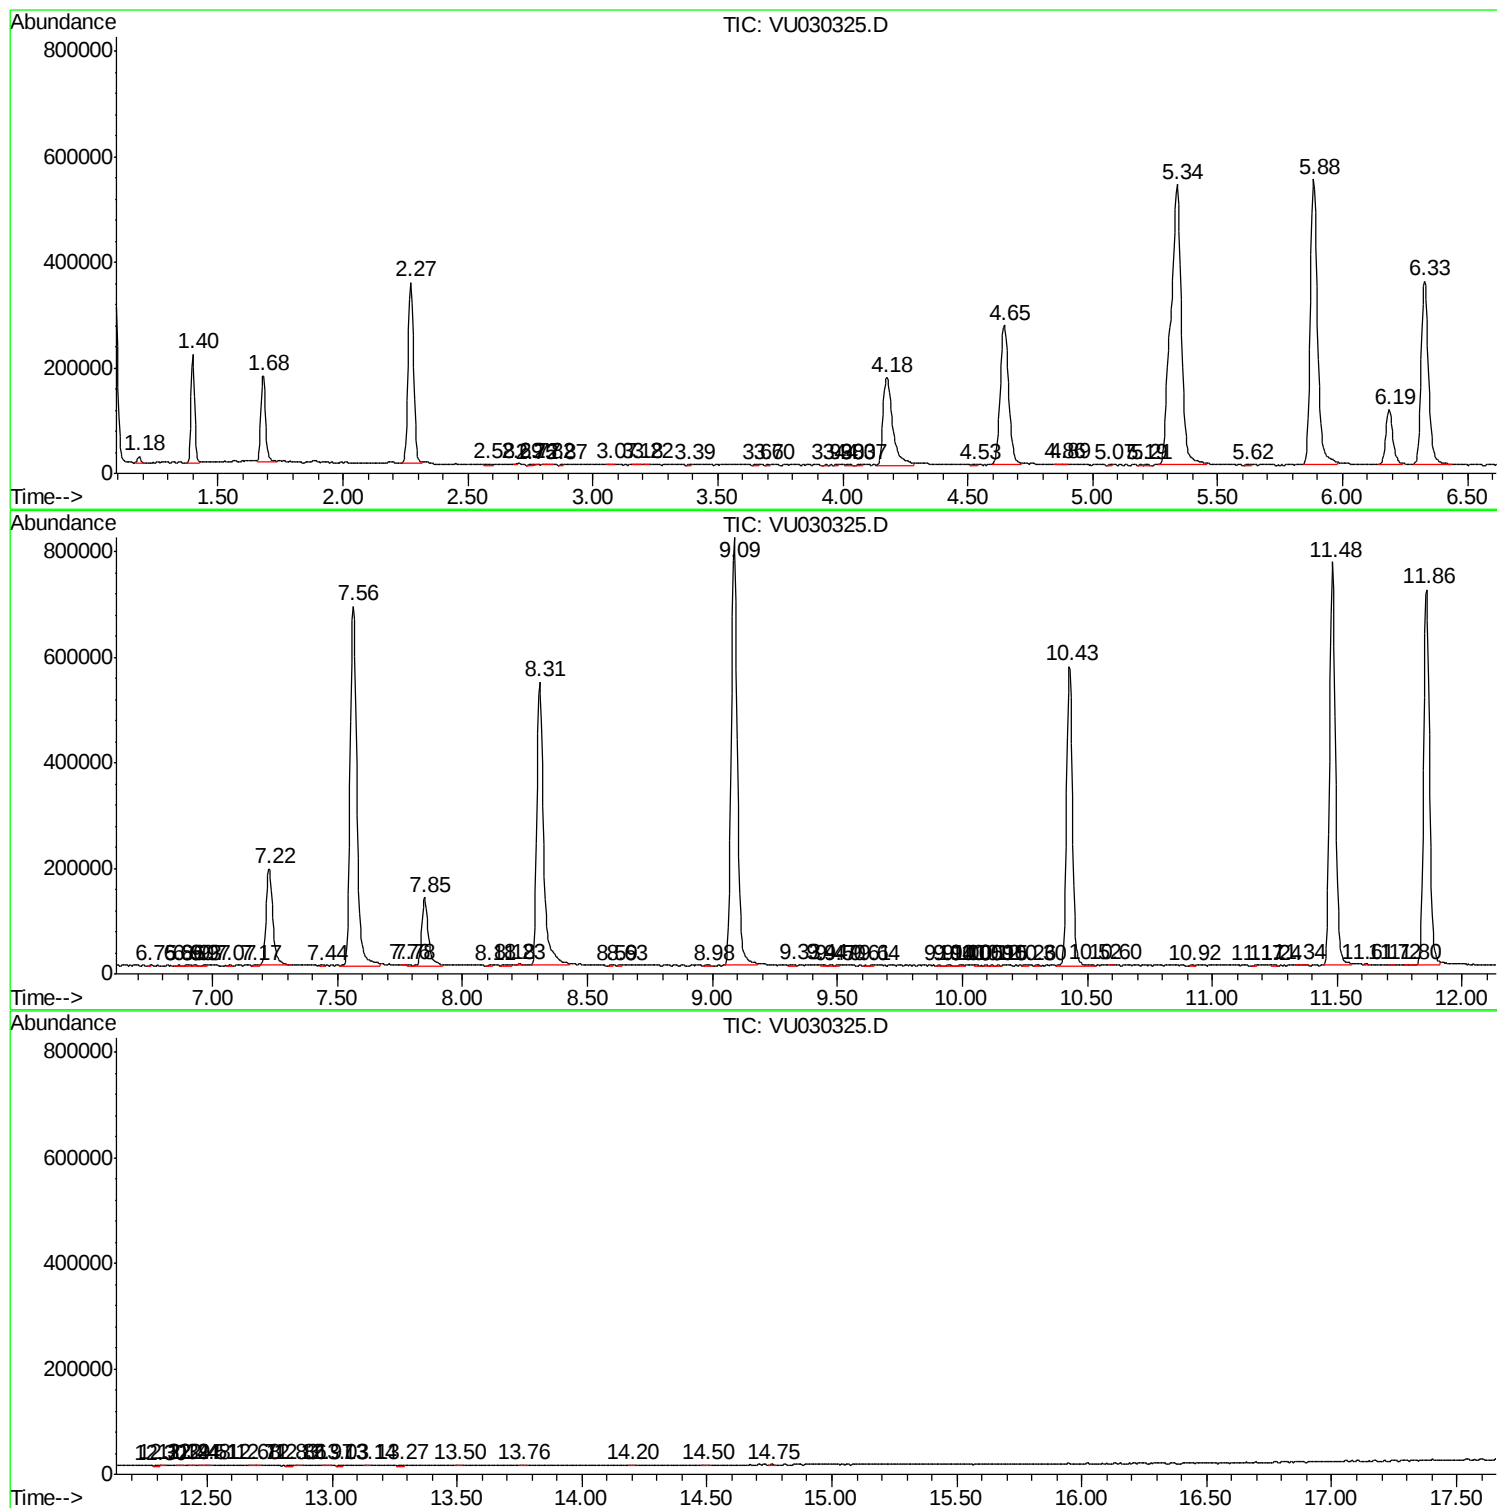

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030325.D
Acq On : 22 Mar 2019 21:46
Operator : JC/SP
Sample : K2062-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030325.D
Acq On : 22 Mar 2019 21:46
Operator : JC/SP
Sample : K2062-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc