

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030326.D
 Acq On : 22 Mar 2019 22:09
 Operator : JC/SP
 Sample : K2062-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB2	12050	11674	0.77%	0.091%
2	1.399	89	96	107	rBV	202574	198622	13.05%	1.547%
3	1.679	176	183	196	rVB	154911	193834	12.73%	1.510%
4	2.270	357	367	382	rBV	329050	495319	32.54%	3.859%
5	2.399	404	407	412	rVB	1681	1395	0.09%	0.011%
6	2.527	444	447	452	rVB	1103	1007	0.07%	0.008%
7	2.637	477	481	484	rVB	1353	1049	0.07%	0.008%
8	2.701	491	501	510	rBV4	3203	6588	0.43%	0.051%
9	2.826	536	540	541	rBV	1456	1023	0.07%	0.008%
10	2.981	585	588	591	rBV	1262	828	0.05%	0.006%
11	3.055	608	611	615	rVB	1193	862	0.06%	0.007%
12	3.148	637	640	648	rVB	1516	1675	0.11%	0.013%
13	3.187	648	652	655	rVB	1501	1006	0.07%	0.008%
14	3.370	706	709	711	rBV	1058	797	0.05%	0.006%
15	3.469	736	740	741	rBV	1819	1092	0.07%	0.009%
16	3.537	757	761	764	rBV2	1321	1120	0.07%	0.009%
17	3.598	774	780	784	rBV	1533	2077	0.14%	0.016%
18	3.817	845	848	853	rVB	940	832	0.05%	0.006%
19	4.125	937	944	948	rBV	1465	2087	0.14%	0.016%
20	4.177	948	960	986	rBV	159950	411508	27.03%	3.206%
21	4.646	1090	1106	1126	rBV	253255	606352	39.84%	4.723%
22	4.875	1173	1177	1180	rBV	1922	1545	0.10%	0.012%
23	5.010	1216	1219	1224	rBV3	1261	1254	0.08%	0.010%
24	5.190	1272	1275	1279	rBV	1301	1027	0.07%	0.008%
25	5.338	1298	1321	1347	rBV3	512092	1522131	100.00%	11.857%
26	5.707	1433	1436	1440	rBV	1471	1189	0.08%	0.009%
27	5.749	1444	1449	1452	rBV2	1339	1435	0.09%	0.011%
28	5.884	1477	1491	1530	rBV	536079	1111409	73.02%	8.658%
29	6.135	1566	1569	1572	rBV	1179	801	0.05%	0.006%
30	6.174	1577	1581	1582	rBV2	1612	1190	0.08%	0.009%
31	6.328	1615	1629	1654	rBV	340126	698580	45.89%	5.442%
32	6.752	1757	1761	1764	rVB	1299	945	0.06%	0.007%
33	6.804	1774	1777	1780	rVB	1828	1234	0.08%	0.010%
34	6.826	1780	1784	1786	rBV	1089	805	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030326.D
 Acq On : 22 Mar 2019 22:09
 Operator : JC/SP
 Sample : K2062-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

35	7.116	1869	1874	1879	rVB	1498	1687	0.11%	0.013%
36	7.157	1885	1887	1891	rVB	1568	926	0.06%	0.007%
37	7.225	1895	1908	1935	rBV	178304	338084	22.21%	2.634%
38	7.563	1999	2013	2048	rBV	667883	1213132	79.70%	9.450%
39	7.736	2064	2067	2075	rVB3	1943	2056	0.14%	0.016%
40	7.849	2092	2102	2127	rBV	122772	223399	14.68%	1.740%
41	8.035	2153	2160	2163	rBV2	1452	1875	0.12%	0.015%
42	8.055	2163	2166	2170	rVB	1545	1247	0.08%	0.010%
43	8.164	2195	2200	2203	rBV2	1721	1979	0.13%	0.015%
44	8.225	2209	2219	2233	rBV3	46362	80095	5.26%	0.624%
45	8.309	2234	2245	2277	rBV	523170	956663	62.85%	7.452%
46	8.614	2335	2340	2344	rVB	1462	1741	0.11%	0.014%
47	8.678	2357	2360	2365	rVB3	843	931	0.06%	0.007%
48	8.733	2374	2377	2386	rVB3	830	1057	0.07%	0.008%
49	8.788	2389	2394	2395	rBV	1131	828	0.05%	0.006%
50	8.971	2448	2451	2455	rVB	1512	1041	0.07%	0.008%
51	9.087	2470	2487	2513	rBV	795607	1370304	90.03%	10.675%
52	9.334	2558	2564	2567	rBV	2090	1818	0.12%	0.014%
53	9.472	2603	2607	2610	rBV	1217	1014	0.07%	0.008%
54	9.524	2619	2623	2626	rBV	1102	1160	0.08%	0.009%
55	9.575	2635	2639	2642	rBV3	1409	1296	0.09%	0.010%
56	9.595	2642	2645	2650	rVB2	1078	1059	0.07%	0.008%
57	9.633	2654	2657	2659	rBV	1173	801	0.05%	0.006%
58	9.688	2668	2674	2676	rBV	1676	1410	0.09%	0.011%
59	9.791	2698	2706	2708	rBV2	825	924	0.06%	0.007%
60	9.968	2756	2761	2764	rVB	954	867	0.06%	0.007%
61	10.006	2769	2773	2778	rVB	1275	1306	0.09%	0.010%
62	10.141	2811	2815	2821	rBV3	987	1182	0.08%	0.009%
63	10.170	2821	2824	2827	rVB2	1415	948	0.06%	0.007%
64	10.289	2853	2861	2864	rBV2	1630	1657	0.11%	0.013%
65	10.427	2892	2904	2928	rBV	549759	899208	59.08%	7.005%
66	10.598	2950	2957	2961	rBV3	1886	2479	0.16%	0.019%
67	10.630	2964	2967	2974	rVV	2169	1945	0.13%	0.015%
68	10.672	2978	2980	2986	rVB	1145	1021	0.07%	0.008%
69	10.919	3052	3057	3059	rBV	1423	1355	0.09%	0.011%
70	11.006	3080	3084	3090	rBV2	1064	1044	0.07%	0.008%
71	11.103	3110	3114	3117	rBV	1684	1443	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032219\
 Data File : VU030326.D
 Acq On : 22 Mar 2019 22:09
 Operator : JC/SP
 Sample : K2062-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
 Title : VOC Analysis

72	11.167	3129	3134	3136	rVV2	1105	1209	0.08%	0.009%
73	11.276	3164	3168	3173	rVB3	1002	934	0.06%	0.007%
74	11.308	3175	3178	3186	rVB2	1332	1628	0.11%	0.013%
75	11.360	3186	3194	3200	rBV2	1621	2450	0.16%	0.019%
76	11.389	3200	3203	3207	rBV	1479	1363	0.09%	0.011%
77	11.482	3219	3232	3259	rBV	762894	1252618	82.29%	9.758%
78	11.672	3288	3291	3295	rBV	1865	1427	0.09%	0.011%
79	11.762	3316	3319	3324	rVB	1376	1289	0.08%	0.010%
80	11.858	3336	3349	3373	rVV	669060	1143616	75.13%	8.909%
81	12.308	3483	3489	3492	rBV2	1631	1619	0.11%	0.013%
82	12.350	3498	3502	3506	rBV	1676	1479	0.10%	0.012%
83	12.376	3506	3510	3512	rBV2	1157	956	0.06%	0.007%
84	12.450	3530	3533	3536	rBV2	1210	935	0.06%	0.007%
85	12.646	3591	3594	3599	rVB	1447	1367	0.09%	0.011%
86	12.688	3604	3607	3612	rBV	1189	978	0.06%	0.008%
87	13.064	3721	3724	3730	rBV	914	1041	0.07%	0.008%
88	13.186	3759	3762	3771	rBV	1575	2402	0.16%	0.019%
89	13.279	3788	3791	3794	rBV2	955	878	0.06%	0.007%
90	13.318	3800	3803	3806	rBV2	1069	825	0.05%	0.006%
91	13.575	3880	3883	3885	rBV	1172	801	0.05%	0.006%
92	13.836	3961	3964	3967	rBV	1284	830	0.05%	0.006%
93	13.890	3976	3981	3988	rBV2	1678	1747	0.11%	0.014%
94	13.926	3988	3992	3995	rBV2	1783	1413	0.09%	0.011%
95	14.054	4028	4032	4034	rBV	1314	1135	0.07%	0.009%
96	14.308	4109	4111	4116	rVB	1365	946	0.06%	0.007%
97	14.623	4206	4209	4211	rBV	1473	1033	0.07%	0.008%
98	14.922	4299	4302	4307	rBV2	2206	2134	0.14%	0.017%
99	15.106	4356	4359	4364	rBV3	1615	1339	0.09%	0.010%
100	15.469	4469	4472	4474	rBV2	1743	1300	0.09%	0.010%


Sum of corrected areas: 12836966

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032219\
Data File : VU030326.D
Acq On : 22 Mar 2019 22:09
Operator : JC/SP
Sample : K2062-08 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BF1D7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

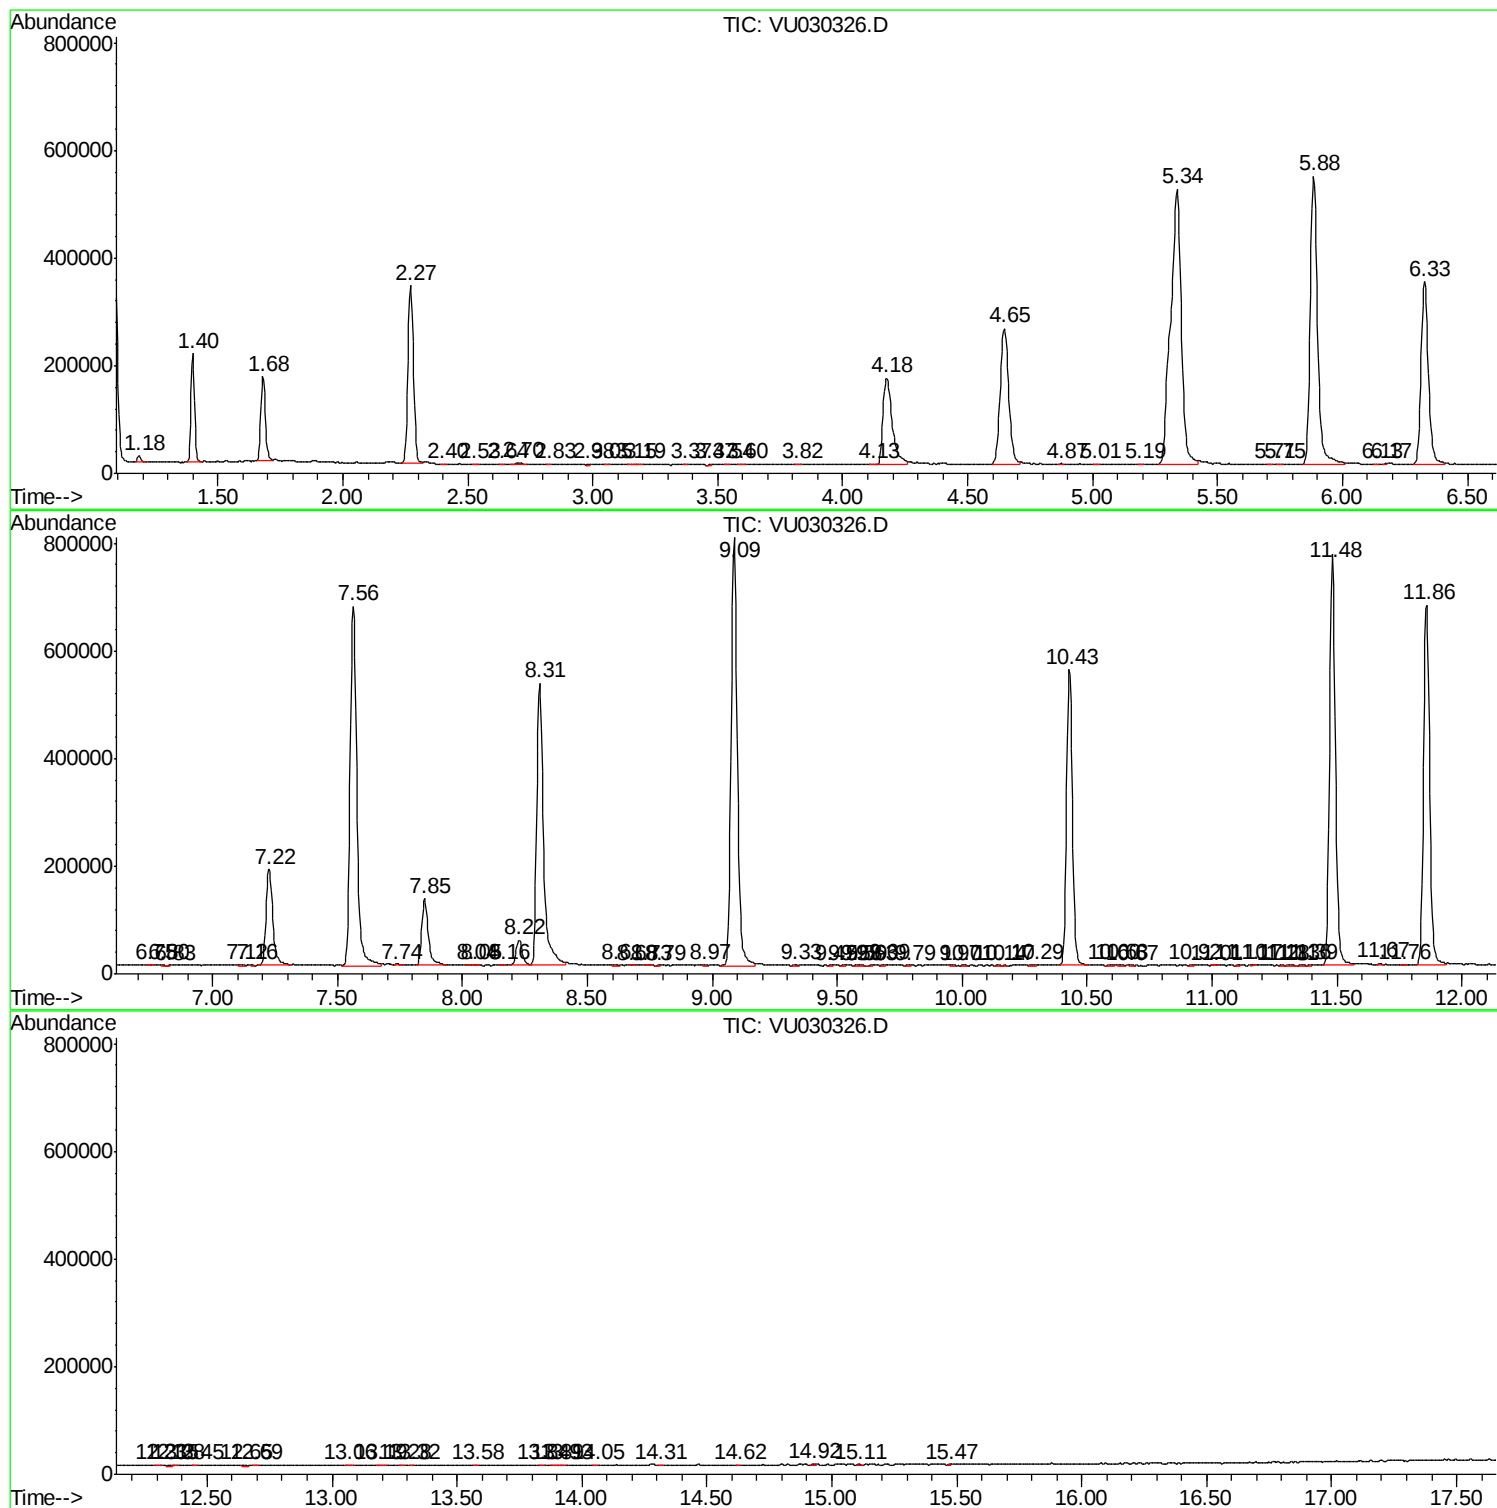

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030326.D
Acq On : 22 Mar 2019 22:09
Operator : JC/SP
Sample : K2062-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032219\
Data File : VU030326.D
Acq On : 22 Mar 2019 22:09
Operator : JC/SP
Sample : K2062-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc