


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032219\
Data File : VU030294.D
Acq On : 22 Mar 2019 09:38
Operator : JC/SP
Sample : BFB40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031919WMA.M
Title : VOC Analysis
Last Update : Mon Mar 25 12:01:39 2019

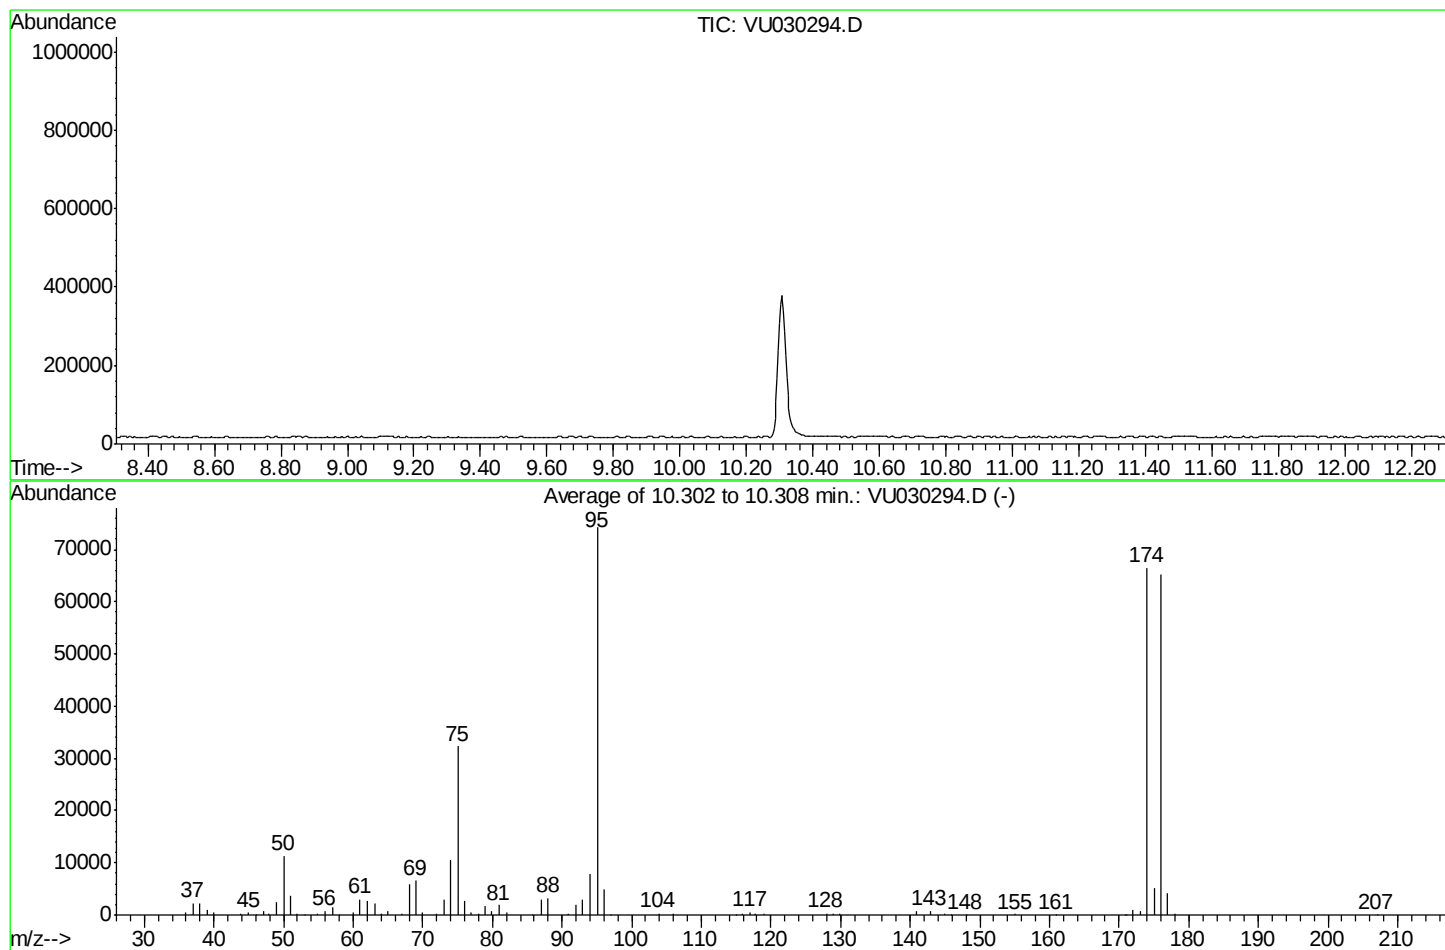

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	11323	PASS
75	95	30	80	43.5	32322	PASS
95	95	100	100	100.0	74253	PASS
96	95	5	9	6.7	4958	PASS
173	174	0.00	2	0.9	632	PASS
174	95	50	120	89.6	66562	PASS
175	174	5	9	7.8	5183	PASS
176	174	95	101	98.1	65328	PASS
177	176	5	9	6.4	4163	PASS

Scan 2854 (10.267 min): VU030294.D
BFB40

m/z	Abundance
40.00	16992.0
43.90	427.0
207.10	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	529.0
37.00	2199.0
38.00	2229.0
39.00	958.0
40.00	17360.0
43.90	648.0
44.90	501.0
46.00	112.0
47.00	804.0
47.90	303.0
49.00	2364.0
50.00	11302.0
51.00	3539.0
52.00	157.0
53.00	106.0
54.80	188.0
56.00	773.0
57.00	1429.0
59.90	548.0
61.00	2873.0
62.00	2769.0
63.10	2129.0
64.10	317.0
65.00	624.0
67.00	284.0
68.00	5822.0
69.00	6194.0
70.00	377.0
72.00	329.0
73.00	2872.0
74.00	10366.0
75.00	31440.0
76.10	2628.0
77.00	334.0
77.90	289.0
78.90	1592.0
79.90	655.0
80.90	1921.0
82.00	400.0
85.90	105.0
87.00	2960.0
88.00	3159.0
90.90	194.0
92.00	1967.0
93.00	2740.0
94.00	7902.0
95.10	72088.0
96.00	4899.0
103.90	216.0
105.90	229.0
115.00	101.0
115.90	243.0
117.00	464.0
117.80	168.0
119.00	340.0
127.90	346.0
129.00	143.0
129.90	302.0
140.90	701.0
142.90	865.0
144.90	195.0
145.80	224.0
148.00	123.0
155.10	199.0
161.00	112.0
170.80	117.0
172.00	859.0
173.10	503.0
174.00	63296.0
175.00	5168.0
176.00	60792.0
177.00	3897.0
177.90	160.0
207.00	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	495.0
37.00	2363.0
38.00	2329.0
39.00	994.0
40.00	17440.0
43.90	776.0
45.00	453.0
47.10	869.0
47.90	324.0
49.00	2418.0
50.00	11638.0
51.00	3746.0
51.90	145.0
54.80	212.0
55.90	824.0
57.00	1399.0
58.00	104.0
60.00	617.0
61.00	3089.0
62.00	2835.0
63.10	2287.0
64.00	371.0
65.00	720.0
67.00	317.0
68.00	6127.0
69.00	6604.0
70.00	403.0
72.00	350.0
73.00	3003.0
74.00	10859.0
75.00	33152.0
76.00	2768.0
77.00	458.0
78.00	356.0
78.90	1756.0
79.90	708.0
80.90	1922.0
82.00	465.0
85.80	102.0
87.00	3005.0
88.00	3282.0
91.00	200.0
92.00	2095.0
93.00	2909.0
94.00	8119.0
95.10	76672.0
96.00	5022.0
96.90	109.0
103.90	273.0
105.90	200.0
115.90	265.0
117.00	520.0
117.80	248.0
119.00	305.0
128.00	358.0
129.00	148.0
129.90	283.0
140.90	828.0
142.90	876.0
144.90	204.0
145.80	141.0
148.10	127.0
155.00	172.0
171.00	124.0
171.90	959.0
173.10	633.0
174.00	68552.0
175.00	5357.0
176.00	67464.0
177.00	4298.0
177.90	153.0
207.00	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	421.0
37.00	2428.0
38.00	2248.0
39.00	962.0
40.00	17424.0
43.90	832.0
45.00	437.0
47.10	859.0
48.00	293.0
49.00	2422.0
50.00	11030.0
51.00	3609.0
52.00	155.0
54.90	176.0
55.90	849.0
57.00	1334.0
58.00	125.0
60.00	590.0
61.00	2980.0
62.00	2788.0
63.10	2158.0
64.00	344.0
65.00	754.0
67.00	261.0
68.00	5999.0
69.00	6789.0
69.90	393.0
72.00	338.0
73.00	2961.0
74.00	10457.0
75.10	32376.0
76.00	2694.0
77.00	529.0
78.00	407.0
78.90	1816.0
79.90	686.0
80.90	1765.0
82.00	453.0
85.70	113.0
87.00	2787.0
88.00	3172.0
91.00	214.0
91.90	1933.0
93.00	2937.0
94.00	7493.0
95.10	74000.0
96.00	4954.0
103.90	316.0
105.90	179.0
115.90	273.0
117.00	542.0
117.80	335.0
119.00	279.0
128.00	335.0
129.00	139.0
129.90	262.0
140.90	775.0
142.90	802.0
144.90	191.0
148.00	143.0
155.00	179.0
171.00	105.0
171.90	1065.0
173.10	760.0
174.00	67840.0
175.00	5025.0
176.00	67728.0
177.00	4296.0
178.00	112.0
207.00	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40