

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053346.D
 Acq On : 22 Mar 2023 12:50
 Operator : JC/MD
 Sample : 01979-16ME
 Misc : 6.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYGC7ME

Quant Time: Mar 23 02:43:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 23 02:41:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	124749	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	118664	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	53937	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	38794	33.708	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.420%		
7) Chloroethane-d5	1.909	69	50883	54.659	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	109.320%		
11) 1,1-Dichloroethene-d2	2.552	63	58946	29.566	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	59.140%#		
21) 2-Butanone-d5	4.633	46	42034	78.747	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	78.750%		
24) Chloroform-d	5.057	84	61391	32.387	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	64.780%#		
26) 1,2-Dichloroethane-d4	5.697	65	50857	43.201	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.400%		
32) Benzene-d6	5.719	84	157008	40.793	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.580%		
36) 1,2-Dichloropropane-d6	6.684	67	50653	40.776	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	81.560%		
41) Toluene-d8	7.893	98	141100	39.375	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.760%#		
43) trans-1,3-Dichloroprop...	8.179	79	23931	39.046	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.100%		
47) 2-Hexanone-d5	8.649	63	33914	87.326	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.330%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	66468	41.305	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.620%		
66) 1,2-Dichlorobenzene-d4	12.192	152	45955	44.003	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.000%		
Target Compounds					Qvalue	
25) Chloroform	5.080	83	11595	6.107	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053346.D
Acq On : 22 Mar 2023 12:50
Operator : JC/MD
Sample : 01979-16ME
Misc : 6.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYGC7ME

Quant Time: Mar 23 02:43:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 23 02:41:20 2023
Response via : Initial Calibration

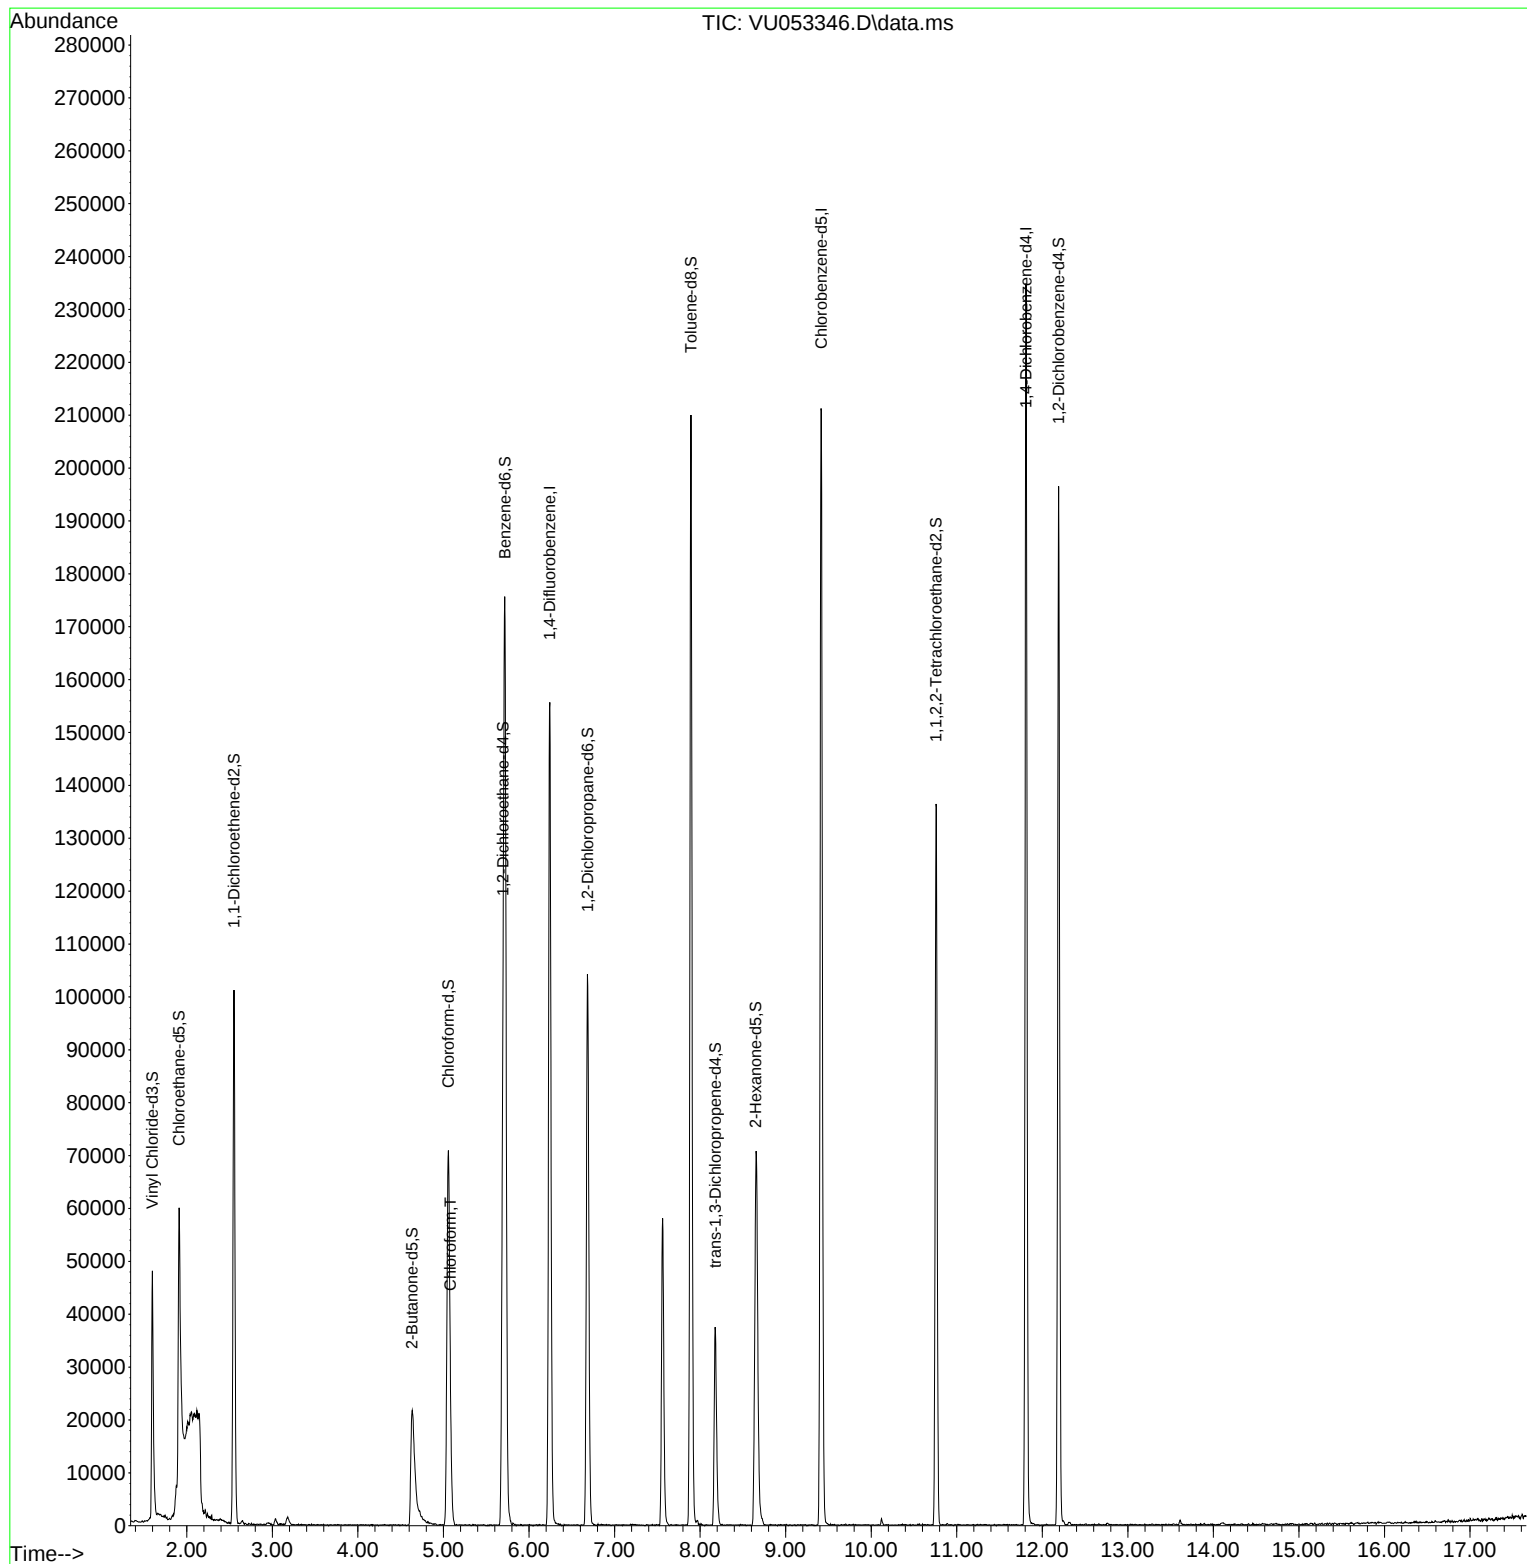

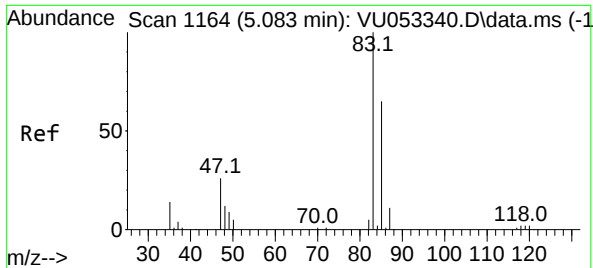

#25
 Chloroform
 Concen: 6.107 ug/L
 RT: 5.080 min Scan# 11
 Delta R.T. -0.003 min
 Lab File: VU053346.D
 Acq: 22 Mar 2023 12:50

Instrument :
 MSVOA_U
 ClientSampleId :
 EYGC7ME

Tgt Ion: 83 Resp: 11595
 Ion Ratio Lower Upper
 83 100
 85 67.5 44.9 83.3

