

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053341.D
 Acq On : 22 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0322MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK056

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	93	rVB	59686	68857	15.44%	2.046%
2	1.912	170	178	195	rVB	59054	80464	18.04%	2.391%
3	2.565	370	381	395	rVB	91165	150628	33.77%	4.476%
4	3.179	565	572	577	rBV3	496	851	0.19%	0.025%
5	3.343	619	623	626	rBV	265	295	0.07%	0.009%
6	3.388	634	637	639	rBV	182	110	0.02%	0.003%
7	3.645	713	717	720	rBV	263	273	0.06%	0.008%
8	3.793	759	763	767	rBV	226	262	0.06%	0.008%
9	3.896	792	795	799	rBB	163	151	0.03%	0.004%
10	3.967	814	817	819	rBV	139	122	0.03%	0.004%
11	4.163	874	878	879	rBV	178	148	0.03%	0.004%
12	4.269	909	911	915	rBB	141	120	0.03%	0.004%
13	4.301	916	921	923	rBV	218	188	0.04%	0.006%
14	4.343	931	934	940	rBB	159	199	0.04%	0.006%
15	4.385	944	947	949	rBV	148	122	0.03%	0.004%
16	4.459	967	970	973	rBV	258	235	0.05%	0.007%
17	4.620	1009	1020	1049	rBV	33268	86408	19.37%	2.568%
18	4.915	1107	1112	1116	rBV	209	290	0.07%	0.009%
19	5.057	1141	1156	1181	rBV	81544	180134	40.39%	5.353%
20	5.160	1183	1188	1190	rBB2	264	204	0.05%	0.006%
21	5.208	1200	1203	1205	rBB	171	108	0.02%	0.003%
22	5.224	1205	1208	1212	rBB	195	179	0.04%	0.005%
23	5.247	1212	1215	1217	rBV	182	142	0.03%	0.004%
24	5.369	1247	1253	1255	rBV	201	260	0.06%	0.008%
25	5.507	1293	1296	1298	rBV	138	121	0.03%	0.004%
26	5.555	1308	1311	1313	rBB	168	108	0.02%	0.003%
27	5.568	1313	1315	1317	rBV	147	105	0.02%	0.003%
28	5.636	1333	1336	1339	rBV	188	182	0.04%	0.005%
29	5.723	1342	1363	1388	rVV2	163421	446032	100.00%	13.254%
30	5.854	1400	1404	1409	rVB2	210	168	0.04%	0.005%
31	5.880	1409	1412	1414	rBV	171	109	0.02%	0.003%
32	5.932	1426	1428	1430	rBV	165	109	0.02%	0.003%
33	5.977	1440	1442	1444	rBV	151	107	0.02%	0.003%
34	6.022	1453	1456	1458	rBB	201	127	0.03%	0.004%
35	6.108	1478	1483	1485	rBV	202	220	0.05%	0.007%
36	6.243	1513	1525	1549	rVB	143573	266901	59.84%	7.931%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053341.D
 Acq On : 22 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0322MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK056

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.395	1570	1572	1574	rBB	265	139	0.03%	0.004%
38	6.417	1575	1579	1581	rBB	194	148	0.03%	0.004%
39	6.446	1585	1588	1592	rBV	194	195	0.04%	0.006%
40	6.491	1600	1602	1605	rBV	143	119	0.03%	0.004%
41	6.552	1619	1621	1626	rVB	259	202	0.05%	0.006%
42	6.578	1626	1629	1634	rBV	153	200	0.04%	0.006%
43	6.626	1639	1644	1647	rBV	187	214	0.05%	0.006%
44	6.684	1649	1662	1682	rVV	104548	202353	45.37%	6.013%
45	6.870	1717	1720	1722	rBV	158	139	0.03%	0.004%
46	6.973	1749	1752	1753	rBV	153	108	0.02%	0.003%
47	7.022	1764	1767	1769	rBV	176	149	0.03%	0.004%
48	7.150	1804	1807	1811	rBV	170	192	0.04%	0.006%
49	7.179	1813	1816	1819	rBB2	318	215	0.05%	0.006%
50	7.195	1819	1821	1824	rBV	218	140	0.03%	0.004%
51	7.243	1832	1836	1838	rBV	211	153	0.03%	0.005%
52	7.321	1857	1860	1863	rBV	174	173	0.04%	0.005%
53	7.430	1889	1894	1899	rBV	255	340	0.08%	0.010%
54	7.488	1905	1912	1915	rBV	246	307	0.07%	0.009%
55	7.562	1923	1935	1956	rBV	59434	104301	23.38%	3.099%
56	7.758	1994	1996	2000	rBB	178	112	0.03%	0.003%
57	7.790	2001	2006	2009	rBV2	313	359	0.08%	0.011%
58	7.893	2025	2038	2058	rBV	208299	352437	79.02%	10.473%
59	8.047	2082	2086	2088	rBB	158	129	0.03%	0.004%
60	8.063	2088	2091	2098	rBV	302	379	0.08%	0.011%
61	8.173	2115	2125	2143	rBV2	39962	67597	15.16%	2.009%
62	8.269	2152	2155	2158	rBV	173	168	0.04%	0.005%
63	8.542	2237	2240	2244	rBV	246	264	0.06%	0.008%
64	8.629	2256	2267	2297	rBV3	94630	183060	41.04%	5.440%
65	8.960	2367	2370	2373	rBV	180	168	0.04%	0.005%
66	9.073	2402	2405	2408	rBB	228	158	0.04%	0.005%
67	9.102	2409	2414	2416	rBV	176	167	0.04%	0.005%
68	9.211	2445	2448	2451	rBV	277	238	0.05%	0.007%
69	9.308	2474	2478	2482	rBB	201	203	0.05%	0.006%
70	9.333	2483	2486	2488	rBV	187	157	0.04%	0.005%
71	9.414	2498	2511	2531	rBV	198951	333598	74.79%	9.913%
72	9.652	2581	2585	2587	rBV	145	149	0.03%	0.004%
73	9.693	2593	2598	2601	rBV2	541	593	0.13%	0.018%
74	9.751	2614	2616	2619	rBV	121	107	0.02%	0.003%
75	10.041	2703	2706	2711	rBV	176	212	0.05%	0.006%
76	10.111	2722	2728	2729	rBV4	1294	1173	0.26%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053341.D
 Acq On : 22 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0322MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK056

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.211	2755	2759	2760	rBV	155	129	0.03%	0.004%
78	10.388	2809	2814	2820	rBV	191	294	0.07%	0.009%
79	10.468	2836	2839	2840	rBV	243	103	0.02%	0.003%
80	10.587	2873	2876	2877	rBV	191	128	0.03%	0.004%
81	10.629	2884	2889	2898	rBV2	1480	2249	0.50%	0.067%
82	10.751	2915	2927	2941	rBV2	134831	218725	49.04%	6.499%
83	10.928	2977	2982	2984	rBV	218	240	0.05%	0.007%
84	11.082	3027	3030	3033	rBV	241	235	0.05%	0.007%
85	11.407	3127	3131	3135	rBV	226	292	0.07%	0.009%
86	11.459	3143	3147	3148	rBV	208	147	0.03%	0.004%
87	11.497	3157	3159	3164	rBB	141	120	0.03%	0.004%
88	11.523	3165	3167	3168	rBV	200	107	0.02%	0.003%
89	11.751	3230	3238	3241	rBV2	542	602	0.13%	0.018%
90	11.806	3243	3255	3273	rBV	194550	310375	69.59%	9.223%
91	12.189	3360	3374	3394	rBV	175989	289471	64.90%	8.602%
92	12.317	3407	3414	3419	rVB3	648	873	0.20%	0.026%
93	12.500	3466	3471	3473	rBV	206	228	0.05%	0.007%
94	13.211	3689	3692	3693	rBV	418	200	0.04%	0.006%
95	13.841	3883	3888	3896	rBV3	1282	1515	0.34%	0.045%
96	14.327	4032	4039	4048	rVB3	1552	2114	0.47%	0.063%
97	14.963	4234	4237	4241	rBV	225	232	0.05%	0.007%
98	15.397	4368	4372	4376	rBV2	298	263	0.06%	0.008%
99	15.455	4387	4390	4392	rBV	265	169	0.04%	0.005%
100	15.507	4403	4406	4408	rBV	270	198	0.04%	0.006%


Sum of corrected areas: 3365263

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053341.D
Acq On : 22 Mar 2023 10:53
Operator : JC/MD
Sample : VU0322MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

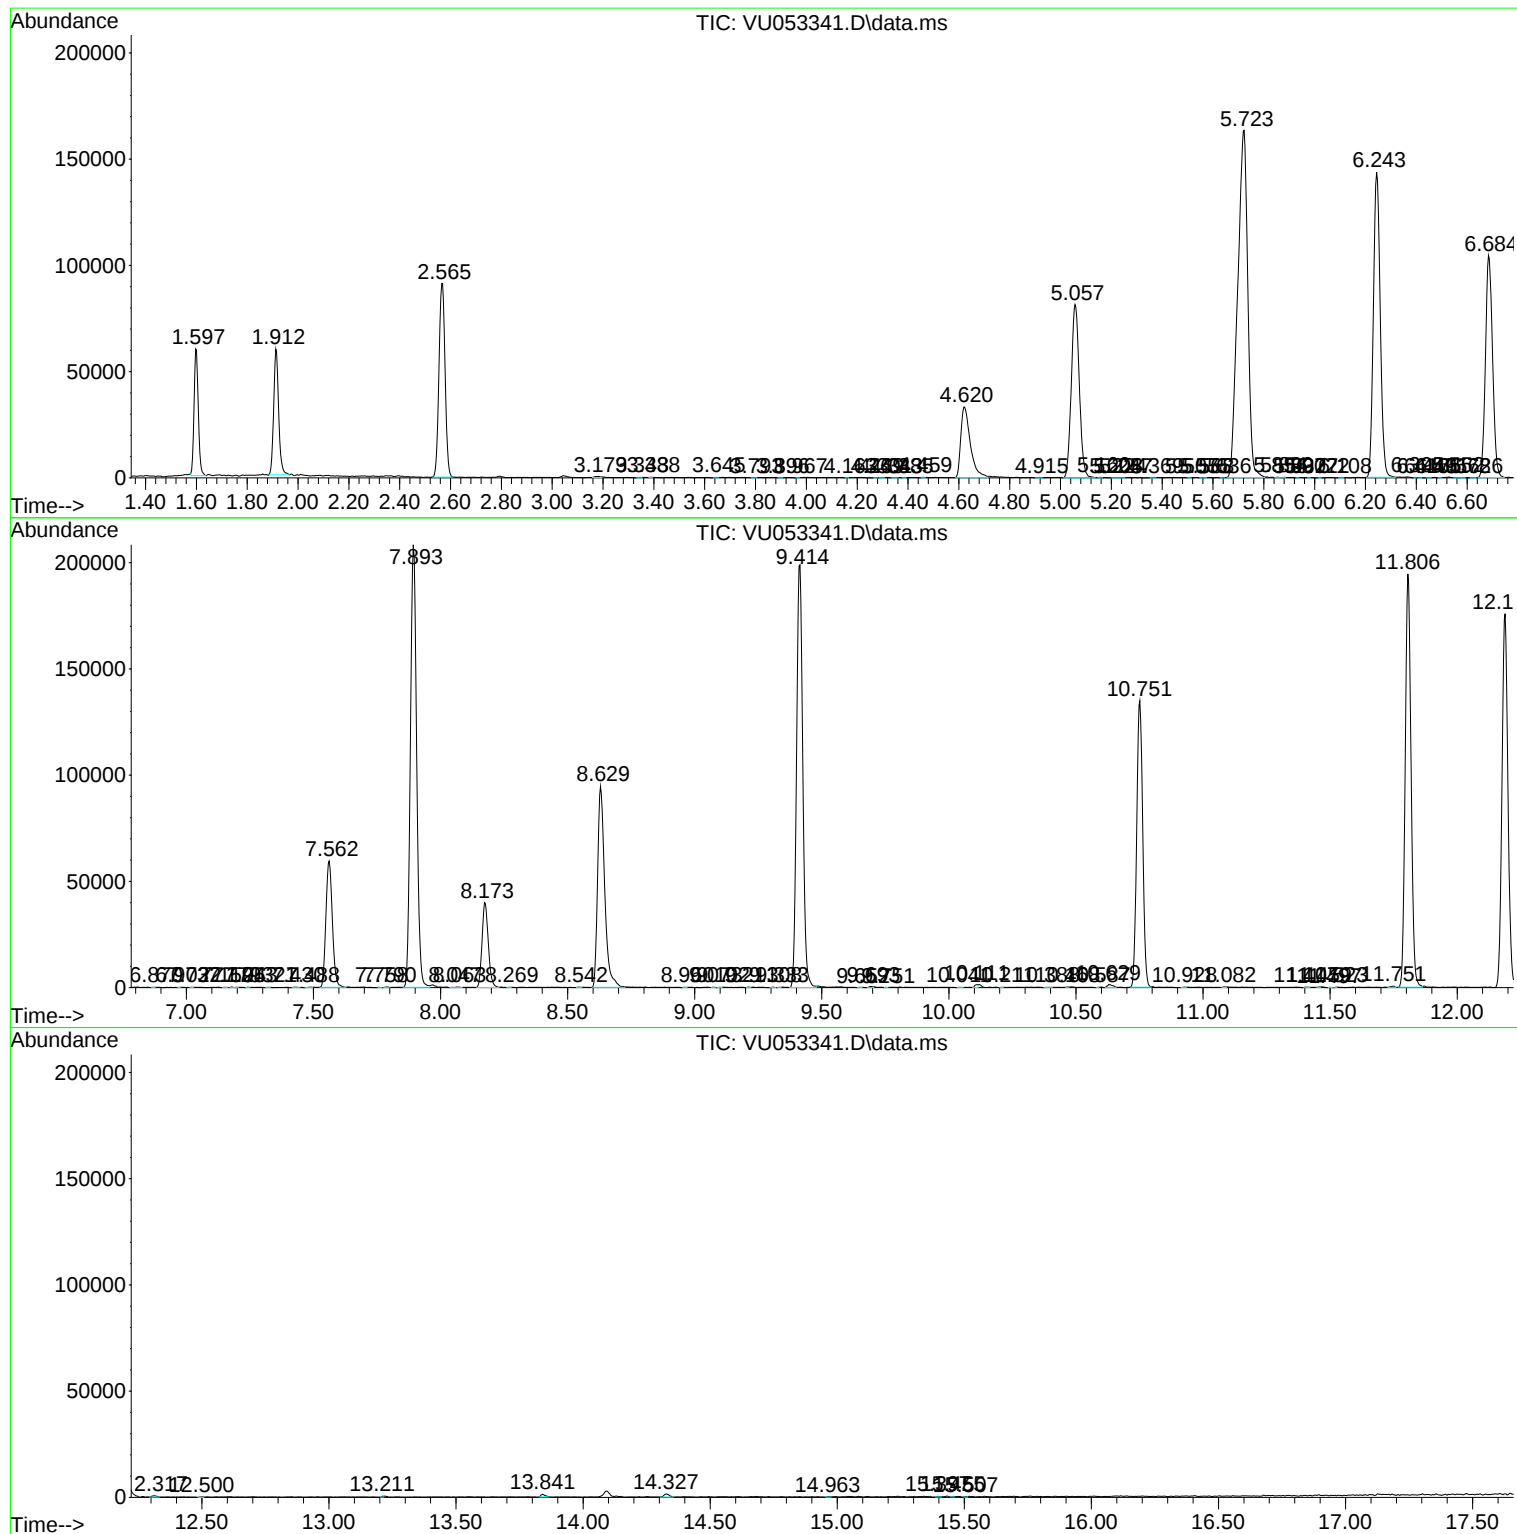

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053341.D
Acq On : 22 Mar 2023 10:53
Operator : JC/MD
Sample : VU0322MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053341.D
Acq On : 22 Mar 2023 10:53
Operator : JC/MD
Sample : VU0322MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc