

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053344.D
 Acq On : 22 Mar 2023 12:04
 Operator : JC/MD
 Sample : 01961-03DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	59708	68813	15.51%	1.874%
2	1.912	170	178	198	rVB	57544	77813	17.54%	2.119%
3	2.565	370	381	394	rBV	92928	148538	33.49%	4.046%
4	3.041	521	529	540	rVB4	1042	1748	0.39%	0.048%
5	3.266	596	599	602	rBV	161	166	0.04%	0.005%
6	3.356	618	627	638	rBV4	1893	3028	0.68%	0.082%
7	3.449	652	656	660	rBV	247	312	0.07%	0.008%
8	3.539	681	684	691	rVB	227	137	0.03%	0.004%
9	3.652	714	719	725	rBV	251	353	0.08%	0.010%
10	4.015	830	832	833	rBV	207	82	0.02%	0.002%
11	4.176	876	882	886	rBV	160	263	0.06%	0.007%
12	4.250	901	905	909	rBV	188	217	0.05%	0.006%
13	4.388	944	948	951	rBV	188	201	0.05%	0.005%
14	4.404	951	953	955	rVV	240	116	0.03%	0.003%
15	4.433	959	962	965	rBB	167	134	0.03%	0.004%
16	4.462	968	971	976	rBB	171	200	0.05%	0.005%
17	4.491	977	980	984	rBV	174	194	0.04%	0.005%
18	4.552	993	999	1002	rBV2	301	329	0.07%	0.009%
19	4.661	1010	1033	1059	rBV3	127055	360437	81.26%	9.817%
20	4.967	1126	1128	1130	rBV	122	85	0.02%	0.002%
21	5.009	1138	1141	1142	rBV	152	103	0.02%	0.003%
22	5.057	1142	1156	1174	rVV	82841	177250	39.96%	4.828%
23	5.163	1186	1189	1195	rVB	212	131	0.03%	0.004%
24	5.350	1244	1247	1249	rBV	197	156	0.04%	0.004%
25	5.440	1273	1275	1277	rBV	146	99	0.02%	0.003%
26	5.536	1302	1305	1310	rBV	167	209	0.05%	0.006%
27	5.719	1342	1362	1387	rBV2	160421	443547	100.00%	12.081%
28	5.835	1395	1398	1401	rBV2	169	139	0.03%	0.004%
29	5.886	1411	1414	1416	rBV	142	126	0.03%	0.003%
30	5.964	1436	1438	1442	rBB	231	140	0.03%	0.004%
31	5.993	1443	1447	1449	rBV	167	135	0.03%	0.004%
32	6.031	1457	1459	1461	rBV	192	81	0.02%	0.002%
33	6.070	1469	1471	1472	rBV	212	88	0.02%	0.002%
34	6.112	1481	1484	1489	rBB	170	192	0.04%	0.005%
35	6.137	1490	1492	1495	rBB	168	115	0.03%	0.003%
36	6.166	1499	1501	1503	rBV	142	98	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053344.D
 Acq On : 22 Mar 2023 12:04
 Operator : JC/MD
 Sample : 01961-03DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.243	1512	1525	1543	rBV	148914	278356	62.76%	7.581%
38	6.369	1561	1564	1566	rVB	302	207	0.05%	0.006%
39	6.382	1566	1568	1571	rBV	183	146	0.03%	0.004%
40	6.430	1575	1583	1589	rBB	214	387	0.09%	0.011%
41	6.459	1590	1592	1595	rBV	168	126	0.03%	0.003%
42	6.565	1622	1625	1628	rBV	170	181	0.04%	0.005%
43	6.629	1643	1645	1647	rBV	182	120	0.03%	0.003%
44	6.684	1649	1662	1681	rVV2	104138	202092	45.56%	5.504%
45	6.793	1694	1696	1699	rBV	160	131	0.03%	0.004%
46	6.813	1699	1702	1703	rVV	155	98	0.02%	0.003%
47	6.861	1713	1717	1722	rBB	216	247	0.06%	0.007%
48	6.886	1722	1725	1727	rBB	171	114	0.03%	0.003%
49	6.919	1730	1735	1738	rBV	145	197	0.04%	0.005%
50	6.999	1758	1760	1763	rBV	160	130	0.03%	0.004%
51	7.025	1766	1768	1770	rBV	146	97	0.02%	0.003%
52	7.105	1790	1793	1795	rBB	130	88	0.02%	0.002%
53	7.128	1795	1800	1804	rBB	203	240	0.05%	0.007%
54	7.150	1804	1807	1809	rBB	148	101	0.02%	0.003%
55	7.179	1810	1816	1821	rBV2	292	402	0.09%	0.011%
56	7.353	1867	1870	1873	rBV	131	139	0.03%	0.004%
57	7.462	1901	1904	1907	rBB	157	126	0.03%	0.003%
58	7.485	1907	1911	1916	rBB	192	223	0.05%	0.006%
59	7.562	1923	1935	1955	rBV	59059	103838	23.41%	2.828%
60	7.829	2016	2018	2020	rBV	111	83	0.02%	0.002%
61	7.893	2026	2038	2059	rBV	203449	353622	79.73%	9.631%
62	8.176	2114	2126	2142	rBV	40947	68291	15.40%	1.860%
63	8.308	2163	2167	2171	rBV	213	244	0.06%	0.007%
64	8.417	2198	2201	2205	rBV	207	211	0.05%	0.006%
65	8.465	2213	2216	2218	rBV	180	146	0.03%	0.004%
66	8.629	2254	2267	2293	rBV2	92165	180502	40.70%	4.916%
67	8.809	2318	2323	2327	rBB	299	304	0.07%	0.008%
68	8.841	2328	2333	2336	rBV	213	254	0.06%	0.007%
69	8.909	2351	2354	2359	rBV	149	212	0.05%	0.006%
70	9.082	2405	2408	2414	rBV	200	267	0.06%	0.007%
71	9.230	2449	2454	2456	rBV2	310	292	0.07%	0.008%
72	9.282	2467	2470	2471	rBV	167	112	0.03%	0.003%
73	9.288	2471	2472	2476	rVB	175	83	0.02%	0.002%
74	9.414	2498	2511	2537	rBV	207237	347878	78.43%	9.475%
75	9.536	2545	2549	2554	rBV	207	288	0.06%	0.008%
76	9.571	2557	2560	2561	rBV	170	112	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053344.D
 Acq On : 22 Mar 2023 12:04
 Operator : JC/MD
 Sample : 01961-03DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.703	2598	2601	2603	rBB	138	95	0.02%	0.003%
78	9.722	2604	2607	2611	rBV	191	206	0.05%	0.006%
79	9.951	2676	2678	2680	rBV	153	108	0.02%	0.003%
80	10.047	2705	2708	2714	rBV	198	267	0.06%	0.007%
81	10.118	2726	2730	2734	rVB3	956	912	0.21%	0.025%
82	10.137	2734	2736	2740	rVB2	286	178	0.04%	0.005%
83	10.201	2751	2756	2759	rBV	155	206	0.05%	0.006%
84	10.311	2788	2790	2791	rBV	153	86	0.02%	0.002%
85	10.562	2862	2868	2872	rBV	185	297	0.07%	0.008%
86	10.751	2914	2927	2940	rBV	138748	221397	49.92%	6.030%
87	10.870	2959	2964	2966	rBV	203	207	0.05%	0.006%
88	11.208	3061	3069	3075	rBV	259	451	0.10%	0.012%
89	11.806	3244	3255	3271	rBV	202245	324995	73.27%	8.852%
90	11.925	3289	3292	3297	rVB	222	143	0.03%	0.004%
91	12.188	3362	3374	3393	rBV	182592	293903	66.26%	8.005%
92	12.288	3403	3405	3407	rBV	238	108	0.02%	0.003%
93	12.311	3407	3412	3416	rBV3	477	582	0.13%	0.016%
94	13.266	3706	3709	3712	rBV	182	128	0.03%	0.003%
95	13.854	3889	3892	3897	rVB	248	185	0.04%	0.005%
96	15.092	4274	4277	4279	rBV	215	122	0.03%	0.003%
97	15.140	4290	4292	4297	rBB	224	87	0.02%	0.002%
98	15.240	4321	4323	4324	rBV2	178	95	0.02%	0.003%
99	15.439	4382	4385	4386	rBV	206	107	0.02%	0.003%
100	15.783	4490	4492	4496	rBV	284	193	0.04%	0.005%


Sum of corrected areas: 3671520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053344.D
Acq On : 22 Mar 2023 12:04
Operator : JC/MD
Sample : 01961-03DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

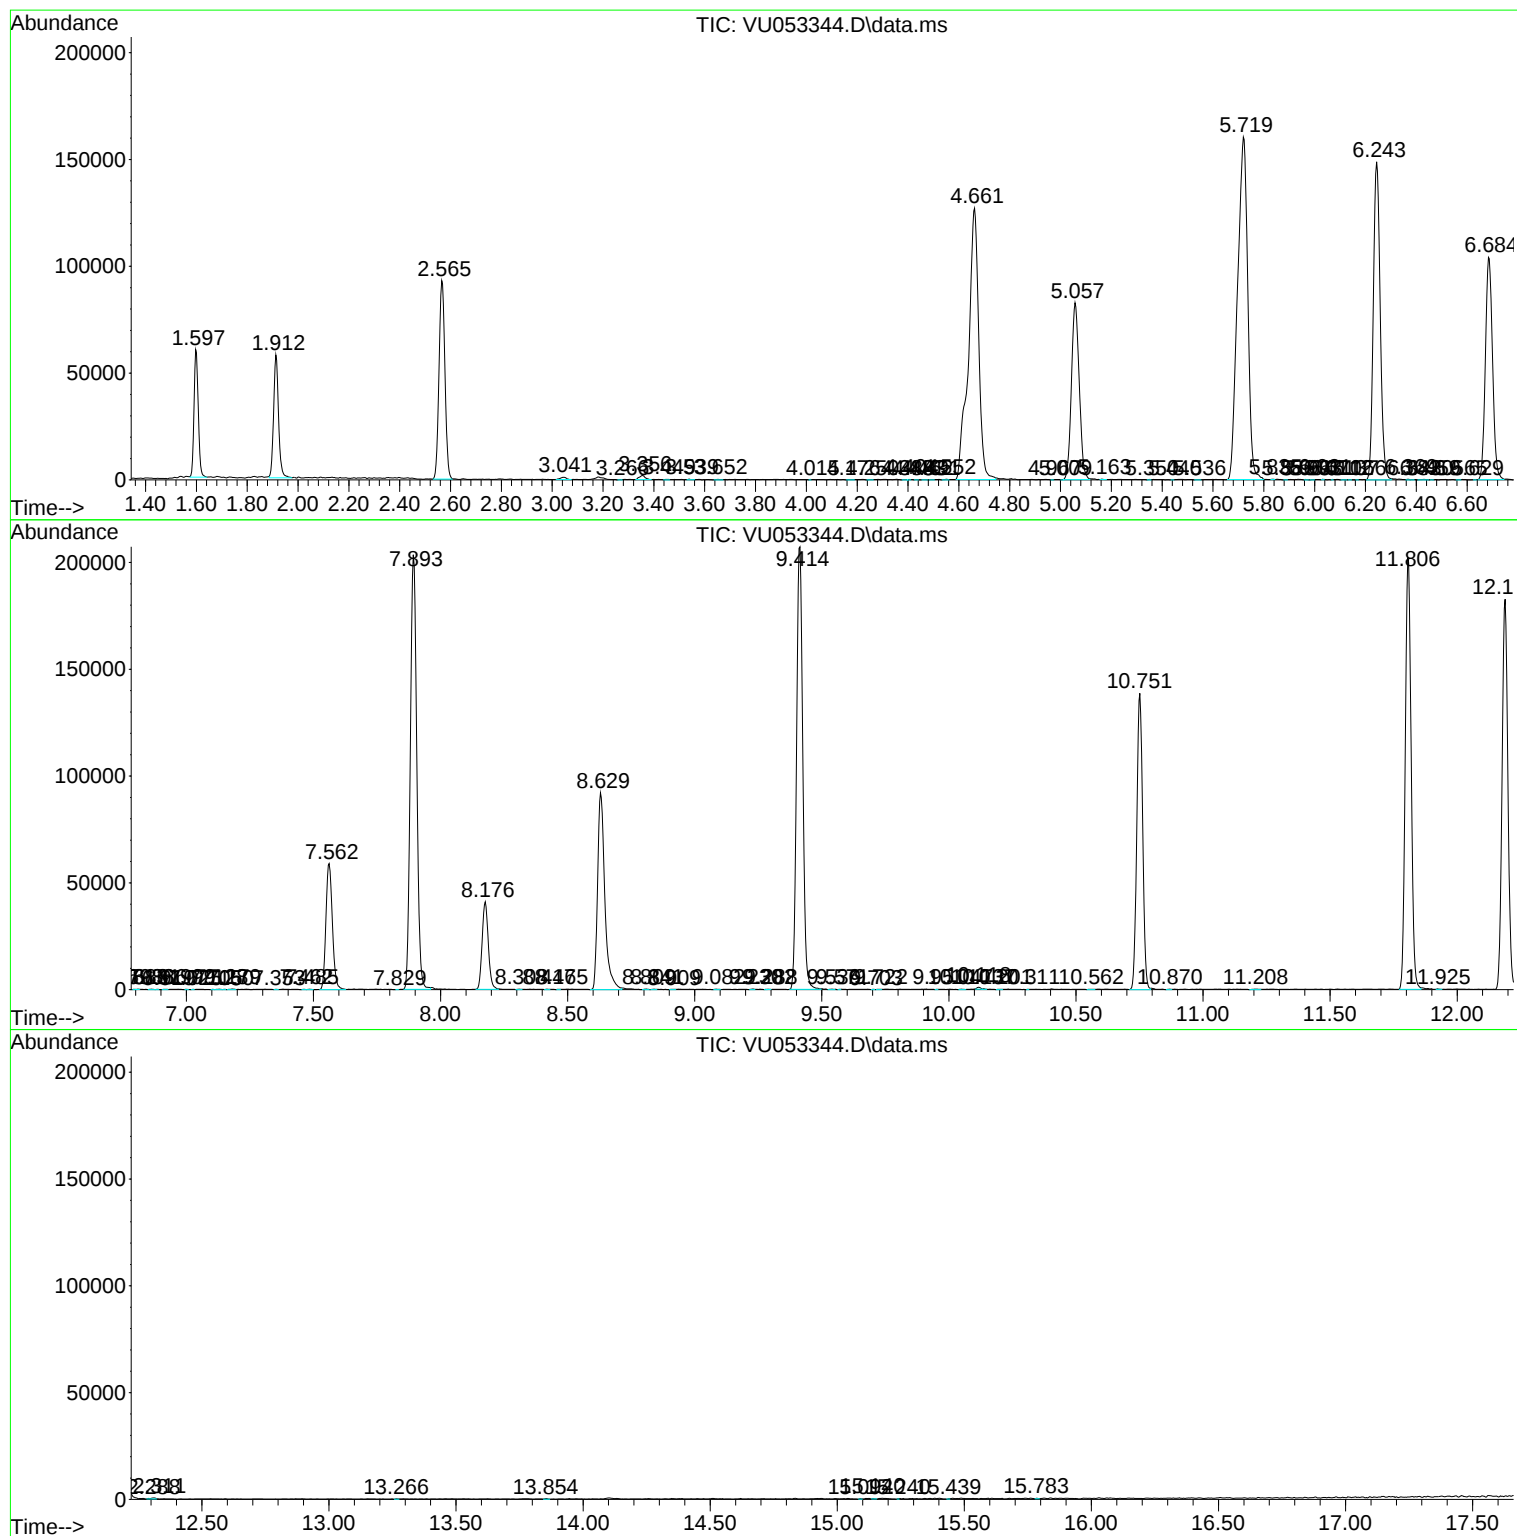

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053344.D
Acq On : 22 Mar 2023 12:04
Operator : JC/MD
Sample : 01961-03DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053344.D
Acq On : 22 Mar 2023 12:04
Operator : JC/MD
Sample : 01961-03DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------