

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053348.D
 Acq On : 22 Mar 2023 13:37
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rVB2	82637	99627	22.90%	2.964%
2	1.913	171	178	191	rVB	53541	70914	16.30%	2.110%
3	2.565	370	381	397	rVB	91647	147340	33.87%	4.384%
4	2.684	416	418	425	rVB	270	141	0.03%	0.004%
5	3.041	526	529	530	rBV	418	267	0.06%	0.008%
6	3.356	618	627	635	rVB2	1123	1915	0.44%	0.057%
7	3.916	797	801	804	rBB	173	137	0.03%	0.004%
8	3.941	804	809	811	rBV	205	219	0.05%	0.007%
9	4.028	832	836	839	rBB	194	146	0.03%	0.004%
10	4.054	839	844	846	rBV	281	273	0.06%	0.008%
11	4.183	880	884	889	rBB	220	249	0.06%	0.007%
12	4.221	890	896	900	rBB	224	290	0.07%	0.009%
13	4.244	900	903	905	rBV	159	137	0.03%	0.004%
14	4.398	948	951	953	rBV	140	124	0.03%	0.004%
15	4.620	1009	1020	1025	rBV	31468	60443	13.90%	1.798%
16	4.864	1092	1096	1098	rBV	190	169	0.04%	0.005%
17	4.957	1123	1125	1127	rBV	132	91	0.02%	0.003%
18	5.057	1140	1156	1176	rVV	82336	176793	40.64%	5.260%
19	5.253	1214	1217	1221	rBV	209	214	0.05%	0.006%
20	5.305	1231	1233	1236	rBB	156	105	0.02%	0.003%
21	5.321	1236	1238	1240	rBV	148	106	0.02%	0.003%
22	5.401	1259	1263	1265	rBB	321	188	0.04%	0.006%
23	5.433	1270	1273	1275	rBV	153	124	0.03%	0.004%
24	5.517	1296	1299	1301	rBV	187	148	0.03%	0.004%
25	5.588	1318	1321	1325	rBB	190	174	0.04%	0.005%
26	5.723	1341	1363	1385	rBV2	158055	434989	100.00%	12.943%
27	5.999	1445	1449	1452	rBV	202	217	0.05%	0.006%
28	6.070	1468	1471	1474	rBV	184	175	0.04%	0.005%
29	6.160	1495	1499	1503	rBB	185	194	0.04%	0.006%
30	6.244	1512	1525	1544	rBV	144781	271704	62.46%	8.085%
31	6.456	1584	1591	1594	rBV	265	241	0.06%	0.007%
32	6.510	1604	1608	1611	rBV	229	152	0.03%	0.005%
33	6.543	1611	1618	1624	rBV4	1434	2045	0.47%	0.061%
34	6.610	1636	1639	1645	rBV	258	292	0.07%	0.009%
35	6.684	1649	1662	1686	rVB2	103428	201353	46.29%	5.991%
36	6.787	1687	1694	1698	rBV	334	406	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053348.D
 Acq On : 22 Mar 2023 13:37
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.825	1703	1706	1708	rBV	144	124	0.03%	0.004%
38	6.838	1708	1710	1712	rVB2	265	142	0.03%	0.004%
39	6.854	1712	1715	1717	rBV	164	132	0.03%	0.004%
40	6.890	1723	1726	1728	rBB	159	112	0.03%	0.003%
41	6.912	1729	1733	1734	rBV	151	108	0.02%	0.003%
42	6.951	1738	1745	1747	rBV	229	281	0.06%	0.008%
43	7.025	1765	1768	1774	rBB	208	247	0.06%	0.007%
44	7.083	1783	1786	1788	rBV	156	128	0.03%	0.004%
45	7.141	1801	1804	1807	rBB	204	159	0.04%	0.005%
46	7.179	1813	1816	1818	rBV	311	226	0.05%	0.007%
47	7.234	1831	1833	1835	rBV	142	100	0.02%	0.003%
48	7.276	1841	1846	1849	rBB	154	178	0.04%	0.005%
49	7.308	1853	1856	1858	rBB	152	103	0.02%	0.003%
50	7.359	1868	1872	1874	rBV	137	146	0.03%	0.004%
51	7.414	1886	1889	1891	rBB	173	118	0.03%	0.004%
52	7.436	1892	1896	1898	rBB	148	99	0.02%	0.003%
53	7.465	1899	1905	1906	rBV	174	202	0.05%	0.006%
54	7.562	1923	1935	1956	rVB2	59257	102394	23.54%	3.047%
55	7.716	1978	1983	1986	rBV	144	205	0.05%	0.006%
56	7.774	1997	2001	2003	rBV	172	169	0.04%	0.005%
57	7.893	2025	2038	2062	rBV	208796	352554	81.05%	10.490%
58	8.041	2081	2084	2086	rBV	200	141	0.03%	0.004%
59	8.128	2109	2111	2115	rVV	302	218	0.05%	0.006%
60	8.176	2115	2126	2146	rVV2	39608	67556	15.53%	2.010%
61	8.256	2148	2151	2162	rVB2	286	330	0.08%	0.010%
62	8.379	2183	2189	2193	rBV	148	258	0.06%	0.008%
63	8.430	2202	2205	2210	rBV	176	226	0.05%	0.007%
64	8.530	2233	2236	2238	rBV	238	163	0.04%	0.005%
65	8.629	2256	2267	2293	rBV2	90085	170807	39.27%	5.082%
66	8.919	2355	2357	2360	rBV	173	143	0.03%	0.004%
67	9.182	2437	2439	2443	rVB	286	188	0.04%	0.006%
68	9.333	2483	2486	2488	rBV	164	133	0.03%	0.004%
69	9.414	2498	2511	2531	rBV	205382	340377	78.25%	10.128%
70	9.542	2549	2551	2554	rVV2	259	166	0.04%	0.005%
71	9.562	2554	2557	2563	rVV2	319	234	0.05%	0.007%
72	9.677	2589	2593	2596	rBV	170	168	0.04%	0.005%
73	9.745	2609	2614	2616	rBV	194	208	0.05%	0.006%
74	9.867	2650	2652	2655	rBV	137	114	0.03%	0.003%
75	10.015	2693	2698	2702	rBV	232	282	0.06%	0.008%
76	10.070	2713	2715	2718	rBB	155	104	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053348.D
 Acq On : 22 Mar 2023 13:37
 Operator : JC/MD
 Sample : 01961-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.095	2718	2723	2725	rBV	316	274	0.06%	0.008%
78	10.112	2725	2728	2730	rBV2	578	401	0.09%	0.012%
79	10.192	2748	2753	2757	rBB	210	238	0.05%	0.007%
80	10.218	2758	2761	2763	rBV	168	133	0.03%	0.004%
81	10.308	2785	2789	2791	rBV	199	186	0.04%	0.006%
82	10.478	2837	2842	2847	rBV	221	328	0.08%	0.010%
83	10.751	2915	2927	2941	rBV	136127	216050	49.67%	6.429%
84	11.642	3201	3204	3207	rBV	200	191	0.04%	0.006%
85	11.806	3244	3255	3271	rBV	205437	325552	74.84%	9.687%
86	12.095	3343	3345	3350	rBV	264	197	0.05%	0.006%
87	12.189	3361	3374	3391	rBV	188970	302366	69.51%	8.997%
88	12.288	3403	3405	3407	rBV	160	81	0.02%	0.002%
89	12.311	3407	3412	3417	rVV2	506	533	0.12%	0.016%
90	12.439	3449	3452	3456	rBV	222	239	0.05%	0.007%
91	12.767	3548	3554	3559	rBV2	398	488	0.11%	0.015%
92	13.697	3840	3843	3846	rBV	143	119	0.03%	0.004%
93	13.738	3853	3856	3862	rBV	225	188	0.04%	0.006%
94	14.092	3964	3966	3969	rBV2	179	125	0.03%	0.004%
95	14.423	4066	4069	4073	rBV	190	170	0.04%	0.005%
96	14.918	4221	4223	4225	rBV	199	114	0.03%	0.003%
97	15.066	4266	4269	4276	rBV	345	337	0.08%	0.010%
98	15.497	4399	4403	4409	rVB2	292	300	0.07%	0.009%
99	15.526	4409	4412	4414	rBV	222	129	0.03%	0.004%
100	15.767	4484	4487	4489	rBV2	292	209	0.05%	0.006%


Sum of corrected areas: 3360793

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053348.D
Acq On : 22 Mar 2023 13:37
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

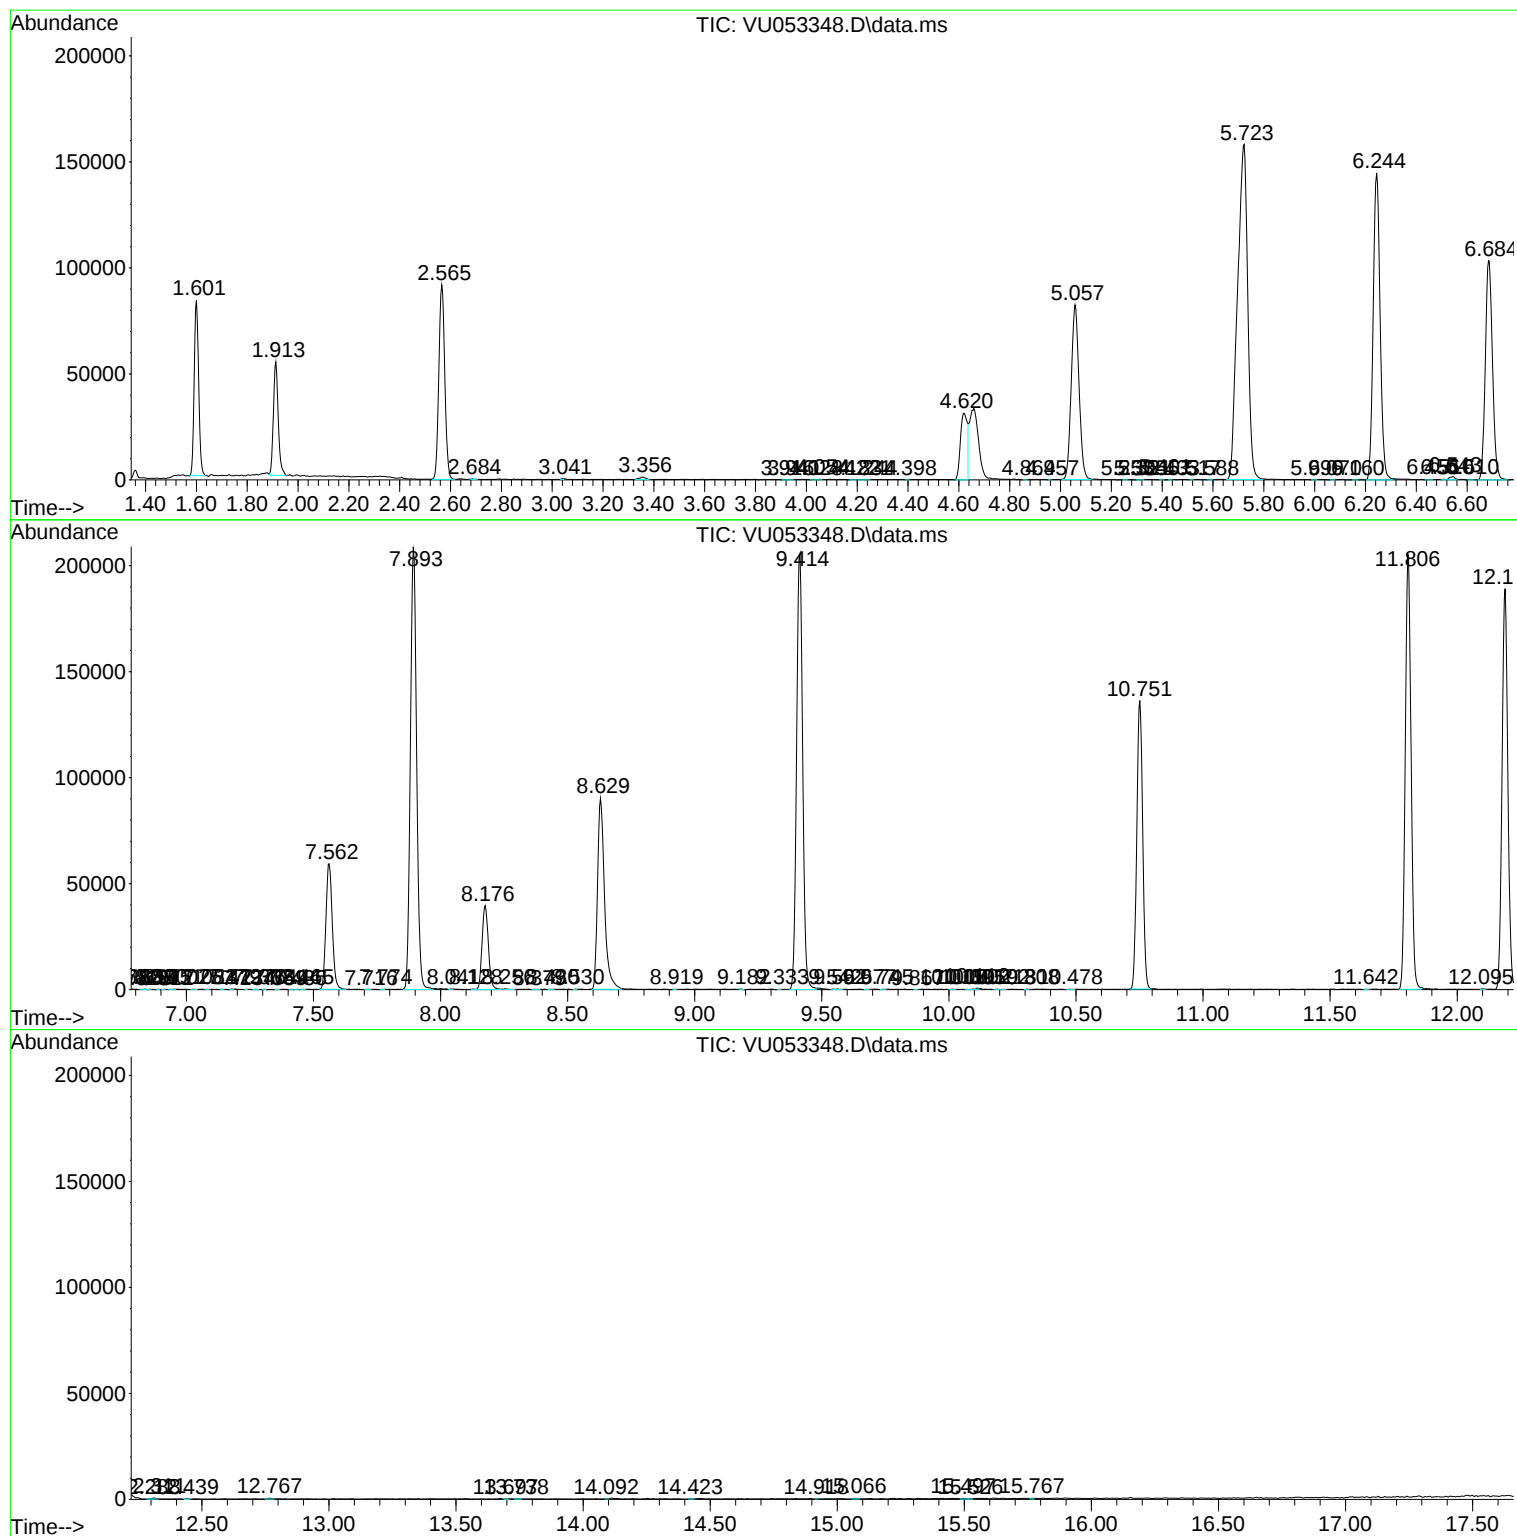

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053348.D
Acq On : 22 Mar 2023 13:37
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053348.D
Acq On : 22 Mar 2023 13:37
Operator : JC/MD
Sample : 01961-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------