

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053349.D
 Acq On : 22 Mar 2023 14:01
 Operator : JC/MD
 Sample : 01961-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	42	55	62	rBV3	4059	11044	2.51%	0.328%
2	1.601	73	81	95	rVB2	86691	105971	24.07%	3.150%
3	1.912	171	178	194	rVB	52695	71360	16.21%	2.121%
4	2.565	370	381	397	rVB	91031	146701	33.32%	4.361%
5	2.633	397	402	404	rBV2	309	328	0.07%	0.010%
6	3.038	525	528	529	rBV	306	187	0.04%	0.006%
7	3.353	618	626	632	rBV4	934	1481	0.34%	0.044%
8	3.398	638	640	642	rBV	152	108	0.02%	0.003%
9	3.465	658	661	663	rBV	203	155	0.04%	0.005%
10	3.861	777	784	787	rBV	270	411	0.09%	0.012%
11	3.932	804	806	808	rBV	111	56	0.01%	0.002%
12	4.150	869	874	876	rBV	200	221	0.05%	0.007%
13	4.256	903	907	918	rBV	303	549	0.12%	0.016%
14	4.398	946	951	953	rBV	159	185	0.04%	0.005%
15	4.501	979	983	985	rBV	165	167	0.04%	0.005%
16	4.623	1008	1021	1026	rBV	30386	63984	14.53%	1.902%
17	4.986	1130	1134	1138	rBV	161	217	0.05%	0.006%
18	5.002	1138	1139	1141	rVV	165	52	0.01%	0.002%
19	5.057	1141	1156	1178	rVV	82096	177256	40.25%	5.269%
20	5.224	1205	1208	1210	rBV	174	139	0.03%	0.004%
21	5.234	1210	1211	1215	rVB	174	86	0.02%	0.003%
22	5.356	1246	1249	1251	rBV	239	176	0.04%	0.005%
23	5.411	1264	1266	1267	rBV	143	77	0.02%	0.002%
24	5.453	1276	1279	1280	rBV	142	100	0.02%	0.003%
25	5.520	1298	1300	1302	rVB	142	73	0.02%	0.002%
26	5.565	1312	1314	1315	rBV	120	66	0.01%	0.002%
27	5.719	1341	1362	1387	rBV2	161888	440341	100.00%	13.091%
28	5.919	1422	1424	1426	rBV	151	108	0.02%	0.003%
29	5.961	1435	1437	1440	rBV	119	67	0.02%	0.002%
30	6.012	1448	1453	1458	rBV	175	290	0.07%	0.009%
31	6.108	1481	1483	1488	rVB	260	186	0.04%	0.006%
32	6.137	1489	1492	1494	rBV	121	85	0.02%	0.003%
33	6.244	1511	1525	1541	rBV	141008	264917	60.16%	7.875%
34	6.395	1569	1572	1575	rBV	209	99	0.02%	0.003%
35	6.433	1582	1584	1586	rBB	135	71	0.02%	0.002%
36	6.465	1592	1594	1597	rBB	147	101	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053349.D
 Acq On : 22 Mar 2023 14:01
 Operator : JC/MD
 Sample : 01961-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.491	1598	1602	1605	rBV	209	212	0.05%	0.006%
38	6.536	1609	1616	1618	rBV3	1180	1256	0.29%	0.037%
39	6.684	1649	1662	1680	rBV	103666	200416	45.51%	5.958%
40	6.800	1693	1698	1701	rBB	156	173	0.04%	0.005%
41	6.825	1704	1706	1708	rBB	146	77	0.02%	0.002%
42	6.845	1709	1712	1713	rBV	116	65	0.01%	0.002%
43	6.899	1724	1729	1732	rBV	154	189	0.04%	0.006%
44	6.951	1742	1745	1747	rBV	185	154	0.03%	0.005%
45	7.086	1783	1787	1789	rBV	188	183	0.04%	0.005%
46	7.134	1798	1802	1806	rBV	192	259	0.06%	0.008%
47	7.173	1812	1814	1815	rBV	164	43	0.01%	0.001%
48	7.237	1831	1834	1836	rBV	161	126	0.03%	0.004%
49	7.372	1875	1876	1878	rBB	111	42	0.01%	0.001%
50	7.388	1878	1881	1884	rBB	189	152	0.03%	0.005%
51	7.411	1885	1888	1892	rBB	190	192	0.04%	0.006%
52	7.443	1895	1898	1903	rBV	225	247	0.06%	0.007%
53	7.488	1909	1912	1914	rBB	144	95	0.02%	0.003%
54	7.504	1914	1917	1918	rBV	129	93	0.02%	0.003%
55	7.562	1923	1935	1952	rBV	58812	102666	23.32%	3.052%
56	7.623	1952	1954	1959	rVB2	370	328	0.07%	0.010%
57	7.649	1959	1962	1964	rBV	237	199	0.05%	0.006%
58	7.893	2024	2038	2056	rBV	204012	349601	79.39%	10.393%
59	8.034	2080	2082	2088	rVB	255	220	0.05%	0.007%
60	8.073	2091	2094	2095	rBV	223	115	0.03%	0.003%
61	8.115	2104	2107	2112	rBV	253	256	0.06%	0.008%
62	8.176	2115	2126	2143	rVV	39709	66141	15.02%	1.966%
63	8.311	2165	2168	2170	rBV	142	123	0.03%	0.004%
64	8.420	2199	2202	2205	rBV	149	153	0.03%	0.005%
65	8.462	2211	2215	2217	rBB	149	102	0.02%	0.003%
66	8.478	2218	2220	2222	rBV	170	109	0.02%	0.003%
67	8.629	2256	2267	2295	rBV2	90774	173621	39.43%	5.161%
68	8.890	2346	2348	2350	rBB	123	65	0.01%	0.002%
69	8.906	2350	2353	2356	rBB	182	142	0.03%	0.004%
70	8.919	2356	2357	2360	rBB	109	41	0.01%	0.001%
71	8.941	2361	2364	2366	rBV	199	169	0.04%	0.005%
72	9.314	2475	2480	2482	rBB	157	153	0.03%	0.005%
73	9.330	2482	2485	2488	rBV	157	148	0.03%	0.004%
74	9.411	2499	2510	2531	rBV	200989	332737	75.56%	9.892%
75	9.507	2538	2540	2543	rBV2	240	140	0.03%	0.004%
76	9.568	2556	2559	2561	rBV	249	142	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053349.D
 Acq On : 22 Mar 2023 14:01
 Operator : JC/MD
 Sample : 01961-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.626	2575	2577	2578	rBV	117	66	0.01%	0.002%
78	9.694	2596	2598	2599	rBV	103	59	0.01%	0.002%
79	9.880	2654	2656	2657	rBB	56	43	0.01%	0.001%
80	9.931	2668	2672	2677	rBV	228	290	0.07%	0.009%
81	10.118	2722	2730	2736	rBV2	671	844	0.19%	0.025%
82	10.221	2758	2762	2768	rBB	258	300	0.07%	0.009%
83	10.253	2769	2772	2777	rBV	179	226	0.05%	0.007%
84	10.623	2884	2887	2889	rBV	163	138	0.03%	0.004%
85	10.751	2915	2927	2944	rBV	136555	216734	49.22%	6.443%
86	10.861	2959	2961	2964	rBV	258	162	0.04%	0.005%
87	10.899	2971	2973	2975	rBV	202	139	0.03%	0.004%
88	11.610	3191	3194	3199	rVB	190	142	0.03%	0.004%
89	11.665	3207	3211	3214	rBV	234	258	0.06%	0.008%
90	11.806	3244	3255	3273	rBV	204558	321995	73.12%	9.572%
91	11.902	3284	3285	3288	rVB	144	55	0.01%	0.002%
92	11.938	3292	3296	3300	rVB	269	178	0.04%	0.005%
93	12.047	3327	3330	3335	rBV	167	109	0.02%	0.003%
94	12.189	3362	3374	3393	rBV	183289	302008	68.59%	8.978%
95	12.308	3408	3411	3413	rBV2	363	281	0.06%	0.008%
96	12.417	3443	3445	3448	rVB	180	58	0.01%	0.002%
97	12.681	3519	3527	3531	rBV	285	466	0.11%	0.014%
98	12.787	3557	3560	3562	rBV	121	81	0.02%	0.002%
99	13.047	3634	3641	3644	rBV	249	372	0.08%	0.011%
100	14.539	4103	4105	4106	rBV	162	55	0.01%	0.002%




Sum of corrected areas: 3363819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053349.D
Acq On : 22 Mar 2023 14:01
Operator : JC/MD
Sample : 01961-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

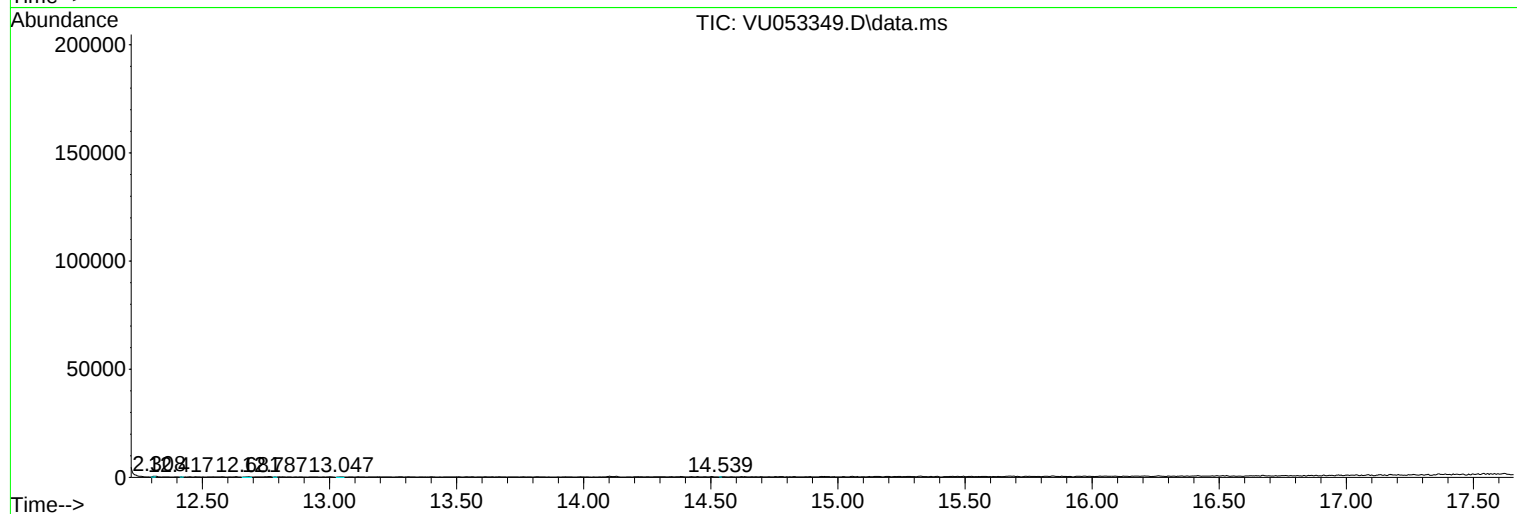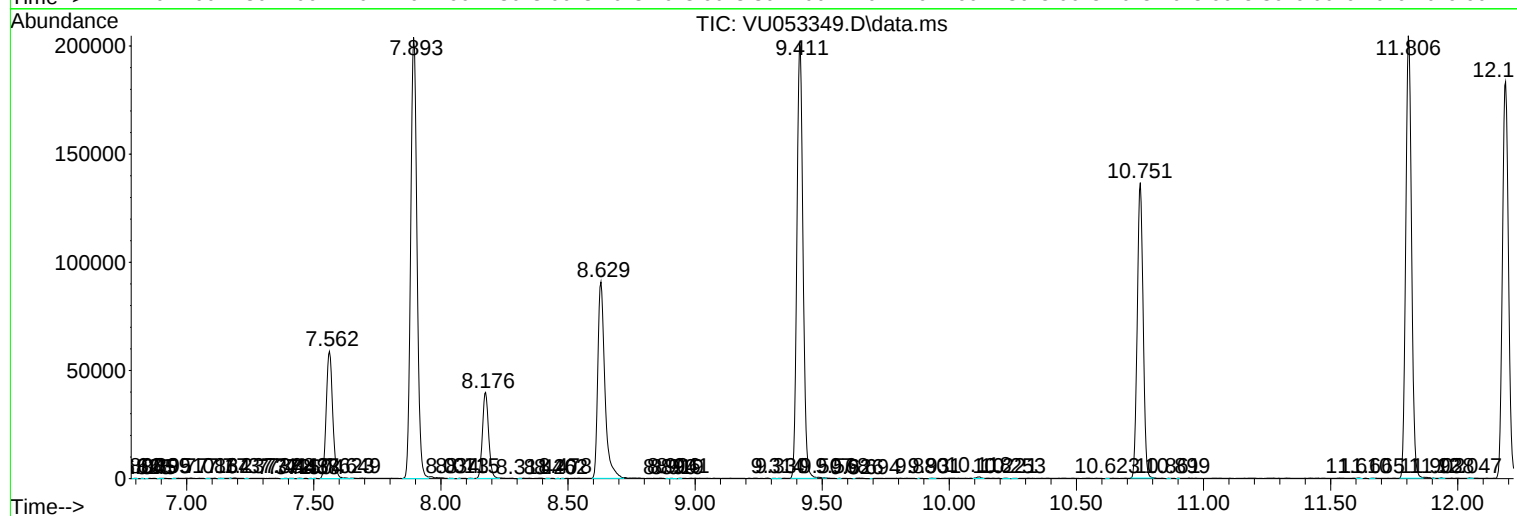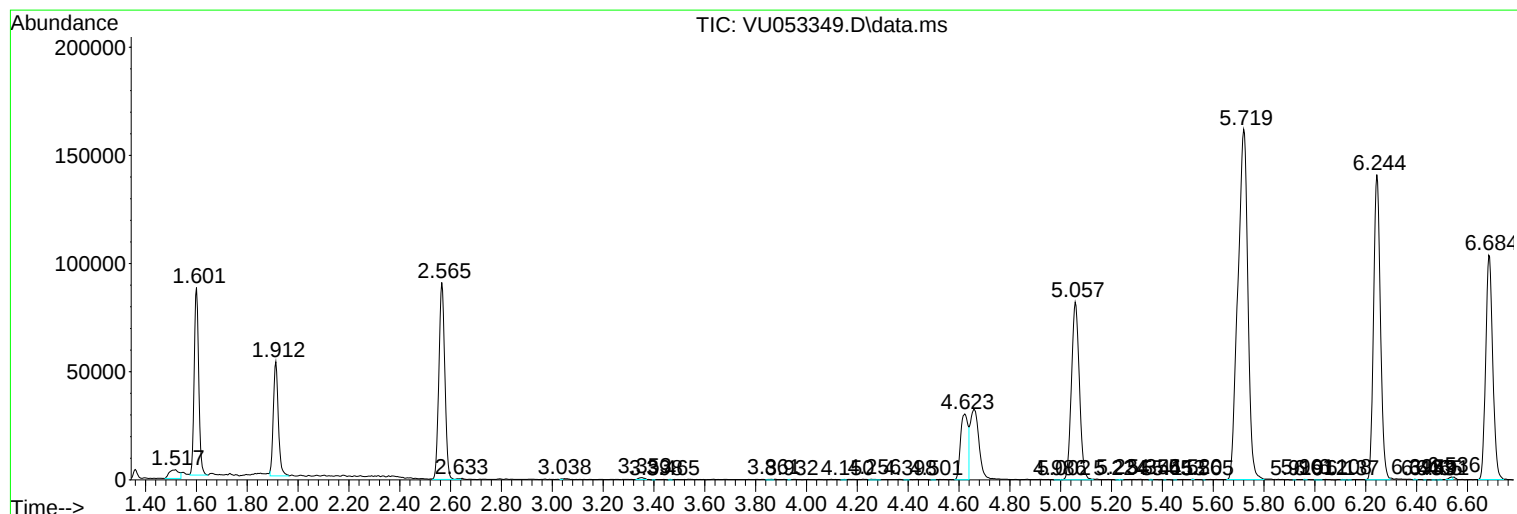

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053349.D
Acq On : 22 Mar 2023 14:01
Operator : JC/MD
Sample : 01961-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053349.D
Acq On : 22 Mar 2023 14:01
Operator : JC/MD
Sample : 01961-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------