

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053352.D
 Acq On : 22 Mar 2023 15:10
 Operator : JC/MD
 Sample : 01961-18DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rVB2	87360	105342	22.98%	2.799%
2	1.913	170	178	193	rVB	51426	70407	15.36%	1.871%
3	2.565	370	381	399	rVB	91384	150699	32.87%	4.005%
4	3.044	522	530	543	rVB3	1170	2244	0.49%	0.060%
5	3.179	564	572	586	rVB2	970	2163	0.47%	0.057%
6	3.337	618	621	622	rBV	161	77	0.02%	0.002%
7	3.350	622	625	634	rVB4	562	532	0.12%	0.014%
8	3.848	775	780	784	rBV	213	302	0.07%	0.008%
9	3.912	794	800	803	rBV	272	342	0.07%	0.009%
10	4.022	830	834	838	rBV	181	220	0.05%	0.006%
11	4.144	869	872	874	rBV	195	160	0.03%	0.004%
12	4.343	932	934	936	rBV	167	112	0.02%	0.003%
13	4.395	945	950	952	rBV	179	207	0.05%	0.006%
14	4.527	987	991	994	rBV	154	197	0.04%	0.005%
15	4.662	1009	1033	1055	rBV2	170360	458409	100.00%	12.182%
16	5.057	1141	1156	1176	rBV2	79016	173383	37.82%	4.607%
17	5.195	1195	1199	1200	rBV	192	150	0.03%	0.004%
18	5.269	1220	1222	1225	rBB	155	105	0.02%	0.003%
19	5.292	1226	1229	1230	rBV	114	65	0.01%	0.002%
20	5.324	1236	1239	1241	rBV	155	133	0.03%	0.004%
21	5.472	1278	1285	1290	rBB	210	349	0.08%	0.009%
22	5.510	1294	1297	1300	rBB	154	128	0.03%	0.003%
23	5.536	1301	1305	1309	rBV	269	318	0.07%	0.008%
24	5.578	1315	1318	1322	rBV	158	197	0.04%	0.005%
25	5.719	1341	1362	1393	rBV4	159810	432662	94.38%	11.498%
26	5.848	1399	1402	1405	rBB2	316	199	0.04%	0.005%
27	5.887	1408	1414	1417	rBV	245	299	0.07%	0.008%
28	6.002	1445	1450	1452	rBV	219	222	0.05%	0.006%
29	6.028	1455	1458	1460	rBV	186	158	0.03%	0.004%
30	6.179	1500	1505	1507	rBV	216	219	0.05%	0.006%
31	6.244	1512	1525	1547	rBV	141356	264283	57.65%	7.023%
32	6.362	1559	1562	1565	rVB2	178	100	0.02%	0.003%
33	6.382	1565	1568	1572	rVB	250	219	0.05%	0.006%
34	6.414	1575	1578	1580	rBV	291	168	0.04%	0.004%
35	6.443	1584	1587	1590	rVB	359	162	0.04%	0.004%
36	6.491	1600	1602	1604	rBB	127	66	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053352.D
 Acq On : 22 Mar 2023 15:10
 Operator : JC/MD
 Sample : 01961-18DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.539	1604	1617	1633	rBB3	22811	41797	9.12%	1.111%
38	6.604	1634	1637	1642	rBV	312	304	0.07%	0.008%
39	6.684	1649	1662	1679	rBV	102729	196040	42.77%	5.210%
40	6.797	1694	1697	1700	rBV	197	181	0.04%	0.005%
41	7.031	1766	1770	1773	rBB	207	181	0.04%	0.005%
42	7.051	1774	1776	1778	rBV	134	94	0.02%	0.002%
43	7.096	1784	1790	1792	rBB	182	174	0.04%	0.005%
44	7.115	1793	1796	1798	rBV	178	143	0.03%	0.004%
45	7.144	1803	1805	1810	rBB	167	160	0.03%	0.004%
46	7.163	1810	1811	1813	rBV	211	86	0.02%	0.002%
47	7.179	1813	1816	1818	rBV	210	159	0.03%	0.004%
48	7.272	1842	1845	1851	rBV	189	265	0.06%	0.007%
49	7.366	1872	1874	1878	rBV	128	136	0.03%	0.004%
50	7.427	1887	1893	1896	rBB	208	220	0.05%	0.006%
51	7.446	1897	1899	1902	rBV	181	142	0.03%	0.004%
52	7.481	1907	1910	1914	rBV	189	223	0.05%	0.006%
53	7.562	1923	1935	1950	rBV2	55837	97587	21.29%	2.593%
54	7.642	1958	1960	1962	rVB2	192	79	0.02%	0.002%
55	7.697	1974	1977	1981	rVB	377	280	0.06%	0.007%
56	7.819	2010	2015	2021	rBB	165	276	0.06%	0.007%
57	7.851	2021	2025	2026	rBV	188	156	0.03%	0.004%
58	7.893	2026	2038	2057	rBV	201115	342855	74.79%	9.111%
59	8.022	2075	2078	2080	rBV	268	213	0.05%	0.006%
60	8.057	2088	2089	2093	rVB	227	129	0.03%	0.003%
61	8.076	2093	2095	2097	rBB	137	74	0.02%	0.002%
62	8.102	2097	2103	2107	rBV	237	312	0.07%	0.008%
63	8.176	2115	2126	2142	rBV2	38938	66162	14.43%	1.758%
64	8.301	2161	2165	2167	rBB	160	129	0.03%	0.003%
65	8.317	2167	2170	2173	rBV	198	188	0.04%	0.005%
66	8.369	2183	2186	2189	rBV	144	141	0.03%	0.004%
67	8.475	2215	2219	2223	rBB	151	173	0.04%	0.005%
68	8.584	2250	2253	2256	rBV	148	145	0.03%	0.004%
69	8.629	2256	2267	2293	rVV2	94465	179687	39.20%	4.775%
70	8.932	2359	2361	2364	rBV	178	143	0.03%	0.004%
71	9.025	2387	2390	2393	rBV	205	214	0.05%	0.006%
72	9.076	2403	2406	2408	rBV	167	135	0.03%	0.004%
73	9.411	2498	2510	2530	rBV	199378	332422	72.52%	8.834%
74	9.562	2555	2557	2558	rBV	144	77	0.02%	0.002%
75	9.645	2580	2583	2586	rBV	270	227	0.05%	0.006%
76	9.713	2600	2604	2610	rBV	335	393	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053352.D
 Acq On : 22 Mar 2023 15:10
 Operator : JC/MD
 Sample : 01961-18DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.964	2676	2682	2684	rBV	163	198	0.04%	0.005%
78	10.047	2704	2708	2713	rBB	253	299	0.07%	0.008%
79	10.073	2714	2716	2717	rBV	171	92	0.02%	0.002%
80	10.108	2725	2727	2728	rBV	405	153	0.03%	0.004%
81	10.179	2742	2749	2752	rBV	307	344	0.08%	0.009%
82	10.195	2752	2754	2757	rVB	122	80	0.02%	0.002%
83	10.327	2792	2795	2797	rBV	148	86	0.02%	0.002%
84	10.632	2887	2890	2892	rBB	145	100	0.02%	0.003%
85	10.658	2893	2898	2902	rBV	347	356	0.08%	0.009%
86	10.700	2909	2911	2912	rBV	149	81	0.02%	0.002%
87	10.751	2915	2927	2943	rVV	136932	214438	46.78%	5.698%
88	11.070	3024	3026	3027	rBV	248	97	0.02%	0.003%
89	11.108	3034	3038	3040	rBV	248	256	0.06%	0.007%
90	11.182	3059	3061	3063	rBV	136	98	0.02%	0.003%
91	11.806	3244	3255	3275	rBV	202810	320478	69.91%	8.516%
92	11.935	3289	3295	3298	rBV	298	350	0.08%	0.009%
93	12.189	3362	3374	3391	rBV	184531	297086	64.81%	7.895%
94	12.308	3409	3411	3413	rBV	250	163	0.04%	0.004%
95	13.365	3738	3740	3744	rBV	210	108	0.02%	0.003%
96	13.857	3890	3893	3895	rBV	227	133	0.03%	0.004%
97	14.099	3966	3968	3970	rBV	201	124	0.03%	0.003%
98	14.713	4157	4159	4163	rBV	177	94	0.02%	0.002%
99	15.211	4311	4314	4317	rVB	291	184	0.04%	0.005%
100	15.401	4370	4373	4376	rBV2	303	181	0.04%	0.005%




Sum of corrected areas: 3763079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053352.D
Acq On : 22 Mar 2023 15:10
Operator : JC/MD
Sample : 01961-18DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

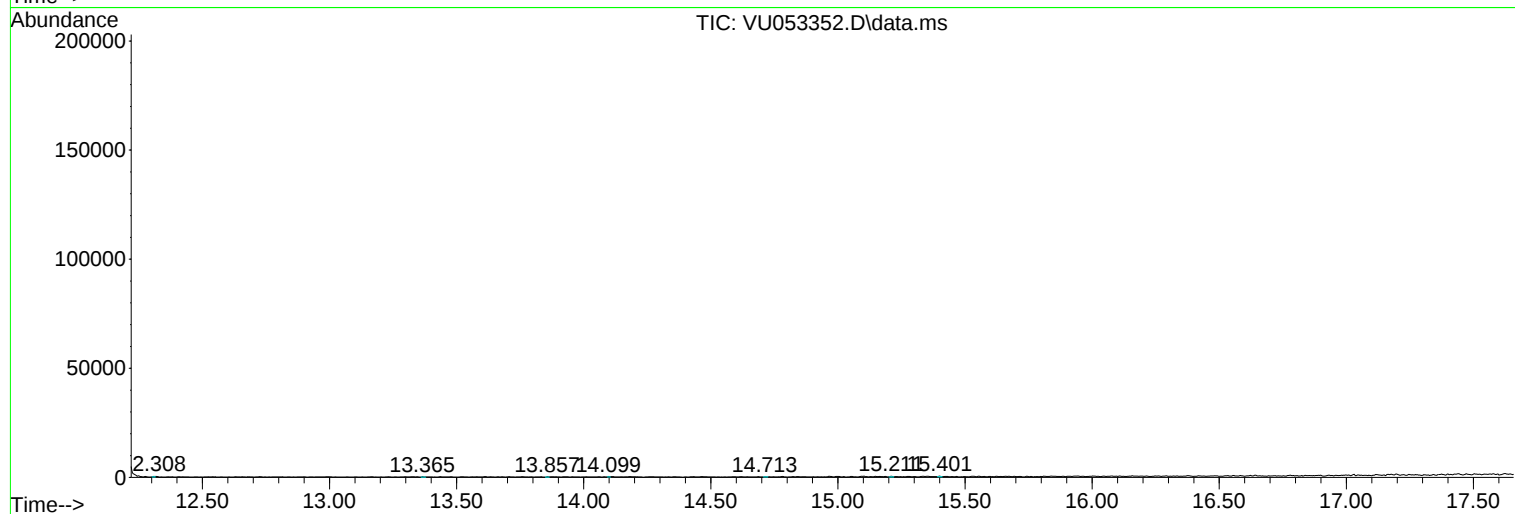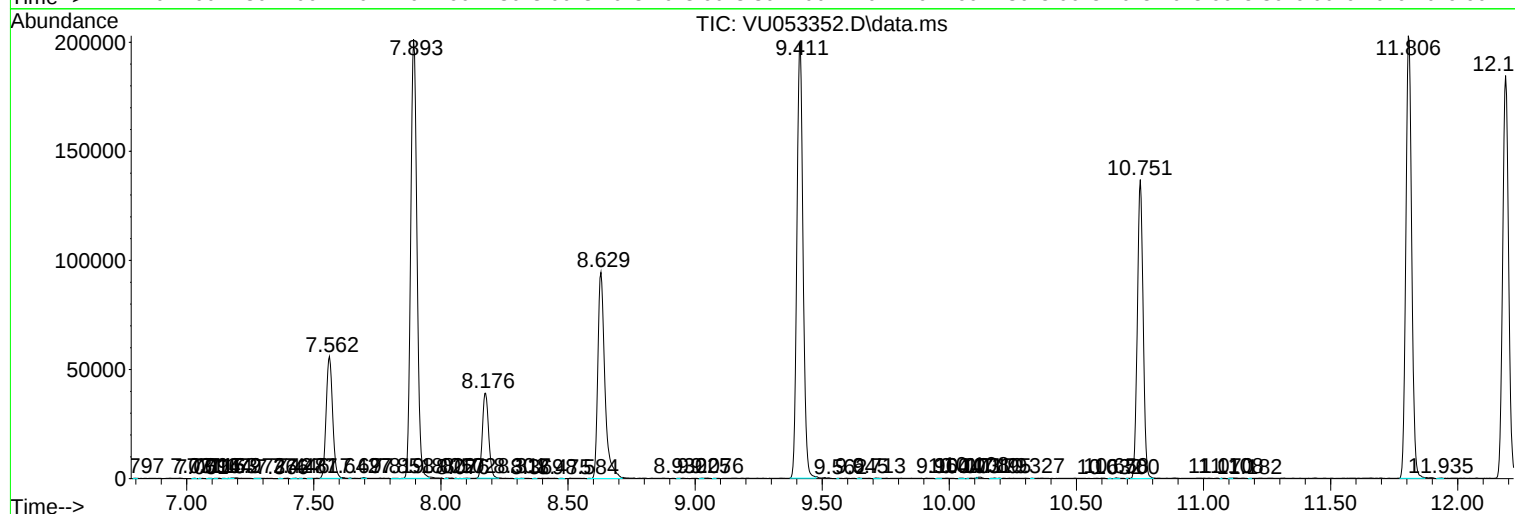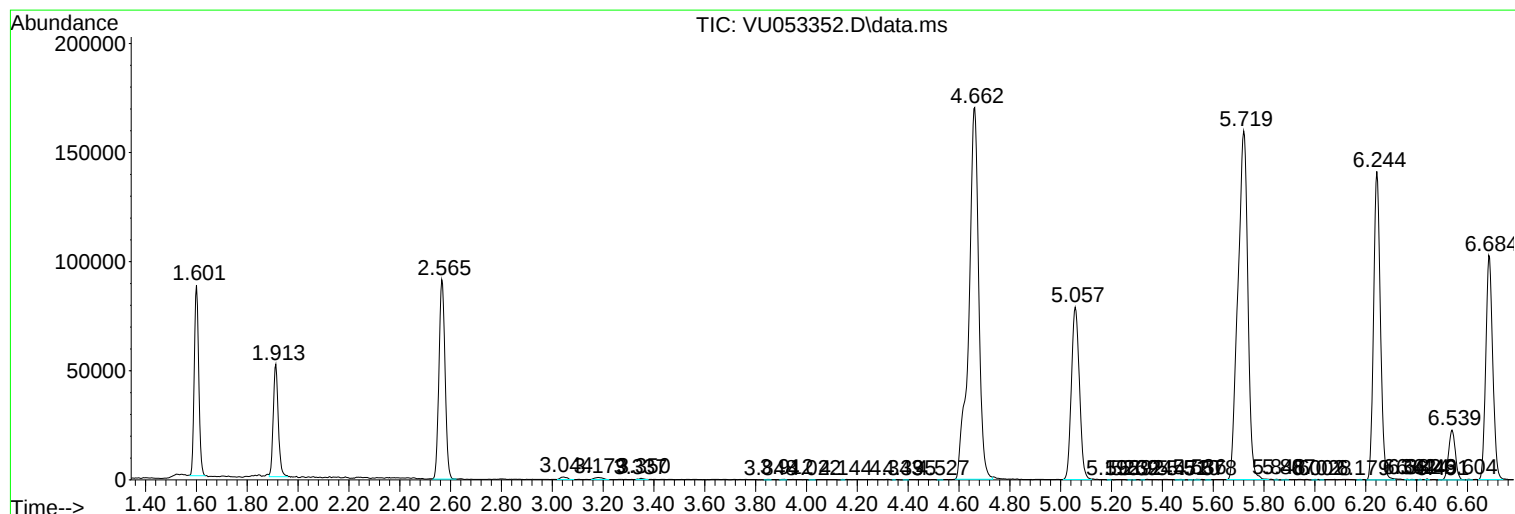

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053352.D
Acq On : 22 Mar 2023 15:10
Operator : JC/MD
Sample : 01961-18DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053352.D
Acq On : 22 Mar 2023 15:10
Operator : JC/MD
Sample : 01961-18DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------