

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053354.D
 Acq On : 22 Mar 2023 15:57
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB2	64773	78163	18.75%	2.442%
2	1.912	170	178	197	rVB	49072	66792	16.02%	2.086%
3	2.308	298	301	302	rBV	233	152	0.04%	0.005%
4	2.568	370	382	397	rVB	86548	139090	33.36%	4.345%
5	2.629	397	401	402	rBV	369	287	0.07%	0.009%
6	2.713	424	427	429	rBV	189	152	0.04%	0.005%
7	2.787	447	450	452	rBV2	312	192	0.05%	0.006%
8	2.948	496	500	502	rBV	220	197	0.05%	0.006%
9	3.044	527	530	535	rVB3	350	298	0.07%	0.009%
10	3.141	557	560	563	rBV	180	182	0.04%	0.006%
11	3.173	568	570	574	rVB2	173	141	0.03%	0.004%
12	3.459	657	659	661	rBV	219	112	0.03%	0.003%
13	3.639	713	715	717	rBV	148	109	0.03%	0.003%
14	3.732	741	744	746	rBV	140	119	0.03%	0.004%
15	3.861	781	784	787	rBB	169	134	0.03%	0.004%
16	3.896	792	795	800	rBB	240	226	0.05%	0.007%
17	3.931	801	806	809	rBV	249	298	0.07%	0.009%
18	3.970	815	818	823	rBV	235	245	0.06%	0.008%
19	4.047	838	842	846	rBB	181	208	0.05%	0.006%
20	4.070	846	849	852	rBV	163	162	0.04%	0.005%
21	4.414	954	956	959	rBV	187	135	0.03%	0.004%
22	4.552	996	999	1001	rBV	128	110	0.03%	0.003%
23	4.616	1007	1019	1049	rBV	31314	85679	20.55%	2.676%
24	4.922	1109	1114	1117	rBV	219	262	0.06%	0.008%
25	5.057	1141	1156	1178	rVV2	76719	169230	40.59%	5.286%
26	5.330	1238	1241	1244	rBV	173	181	0.04%	0.006%
27	5.369	1250	1253	1256	rBV	179	171	0.04%	0.005%
28	5.465	1278	1283	1286	rBB	162	177	0.04%	0.006%
29	5.484	1286	1289	1290	rBV	160	114	0.03%	0.004%
30	5.555	1308	1311	1313	rBV	157	137	0.03%	0.004%
31	5.623	1326	1332	1334	rBB	144	141	0.03%	0.004%
32	5.645	1335	1339	1341	rBV	143	147	0.04%	0.005%
33	5.719	1341	1362	1386	rBV2	154525	416904	100.00%	13.022%
34	5.947	1430	1433	1435	rBV	173	140	0.03%	0.004%
35	6.086	1473	1476	1479	rBB	190	141	0.03%	0.004%
36	6.134	1487	1491	1496	rBB	258	272	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053354.D
 Acq On : 22 Mar 2023 15:57
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.243	1510	1525	1544	rBV	136068	257303	61.72%	8.037%
38	6.333	1549	1553	1557	rBV2	275	260	0.06%	0.008%
39	6.369	1561	1564	1567	rBV2	165	165	0.04%	0.005%
40	6.423	1578	1581	1584	rBB	151	128	0.03%	0.004%
41	6.459	1588	1592	1594	rBV	140	146	0.04%	0.005%
42	6.513	1604	1609	1612	rBV	164	215	0.05%	0.007%
43	6.616	1638	1641	1645	rBV	254	229	0.05%	0.007%
44	6.687	1648	1663	1684	rVB2	97408	191607	45.96%	5.985%
45	6.835	1706	1709	1713	rBV2	278	261	0.06%	0.008%
46	6.941	1740	1742	1744	rBV	264	137	0.03%	0.004%
47	7.150	1802	1807	1811	rBB	172	188	0.05%	0.006%
48	7.173	1812	1814	1816	rBV	175	120	0.03%	0.004%
49	7.189	1816	1819	1821	rBV	344	214	0.05%	0.007%
50	7.295	1849	1852	1855	rBB	192	144	0.03%	0.004%
51	7.320	1856	1860	1867	rBB	172	264	0.06%	0.008%
52	7.356	1868	1871	1874	rBB	158	131	0.03%	0.004%
53	7.385	1875	1880	1882	rBB	128	111	0.03%	0.003%
54	7.449	1894	1900	1902	rBB	276	229	0.05%	0.007%
55	7.517	1919	1921	1923	rBV	166	114	0.03%	0.004%
56	7.562	1923	1935	1954	rVV	54953	95603	22.93%	2.986%
57	7.687	1971	1974	1975	rBV	163	114	0.03%	0.004%
58	7.809	2008	2012	2014	rBV	179	164	0.04%	0.005%
59	7.893	2025	2038	2057	rBV	195089	331626	79.54%	10.359%
60	8.025	2076	2079	2081	rBV	323	245	0.06%	0.008%
61	8.092	2097	2100	2105	rBV	167	235	0.06%	0.007%
62	8.176	2115	2126	2144	rBV	38527	63476	15.23%	1.983%
63	8.311	2164	2168	2176	rBV	200	339	0.08%	0.011%
64	8.629	2256	2267	2293	rBV4	87875	170008	40.78%	5.310%
65	8.764	2307	2309	2312	rVB	220	124	0.03%	0.004%
66	8.828	2322	2329	2330	rBV	156	177	0.04%	0.006%
67	8.877	2335	2344	2347	rBV	271	472	0.11%	0.015%
68	8.928	2357	2360	2363	rBV	151	158	0.04%	0.005%
69	8.954	2365	2368	2372	rBB	190	177	0.04%	0.006%
70	9.015	2384	2387	2391	rBV	241	251	0.06%	0.008%
71	9.092	2405	2411	2414	rBV	171	248	0.06%	0.008%
72	9.214	2446	2449	2450	rBV	160	112	0.03%	0.003%
73	9.301	2470	2476	2478	rBV	290	321	0.08%	0.010%
74	9.356	2490	2493	2495	rBV	183	158	0.04%	0.005%
75	9.414	2499	2511	2528	rVV	193257	319594	76.66%	9.983%
76	9.533	2545	2548	2552	rBV	198	218	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053354.D
 Acq On : 22 Mar 2023 15:57
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.578	2560	2562	2566	rVB	239	186	0.04%	0.006%
78	9.603	2566	2570	2573	rBV	173	198	0.05%	0.006%
79	9.661	2585	2588	2593	rBV	143	179	0.04%	0.006%
80	9.716	2602	2605	2607	rBV	150	125	0.03%	0.004%
81	9.803	2628	2632	2635	rBV	163	153	0.04%	0.005%
82	10.121	2726	2731	2732	rBV2	397	368	0.09%	0.011%
83	10.262	2771	2775	2779	rBV	301	352	0.08%	0.011%
84	10.314	2788	2791	2794	rVB	198	121	0.03%	0.004%
85	10.494	2843	2847	2849	rBV	144	123	0.03%	0.004%
86	10.751	2915	2927	2942	rBV	130710	207855	49.86%	6.493%
87	11.102	3031	3036	3038	rBV	294	248	0.06%	0.008%
88	11.767	3236	3243	3244	rBV2	410	428	0.10%	0.013%
89	11.806	3244	3255	3271	rVV	195769	310208	74.41%	9.690%
90	11.889	3279	3281	3283	rBV	230	124	0.03%	0.004%
91	12.018	3318	3321	3328	rBB	208	250	0.06%	0.008%
92	12.050	3328	3331	3333	rBV	171	139	0.03%	0.004%
93	12.134	3353	3357	3359	rBV2	220	184	0.04%	0.006%
94	12.188	3362	3374	3391	rVV	176672	281835	67.60%	8.803%
95	12.311	3409	3412	3417	rVB	521	466	0.11%	0.015%
96	12.397	3435	3439	3440	rBV	209	174	0.04%	0.005%
97	14.841	4196	4199	4202	rBV	180	148	0.04%	0.005%
98	15.011	4248	4252	4255	rBV	246	221	0.05%	0.007%
99	15.397	4369	4372	4374	rBV2	203	124	0.03%	0.004%
100	15.629	4441	4444	4449	rVB	262	238	0.06%	0.007%




Sum of corrected areas: 3201433

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053354.D
Acq On : 22 Mar 2023 15:57
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

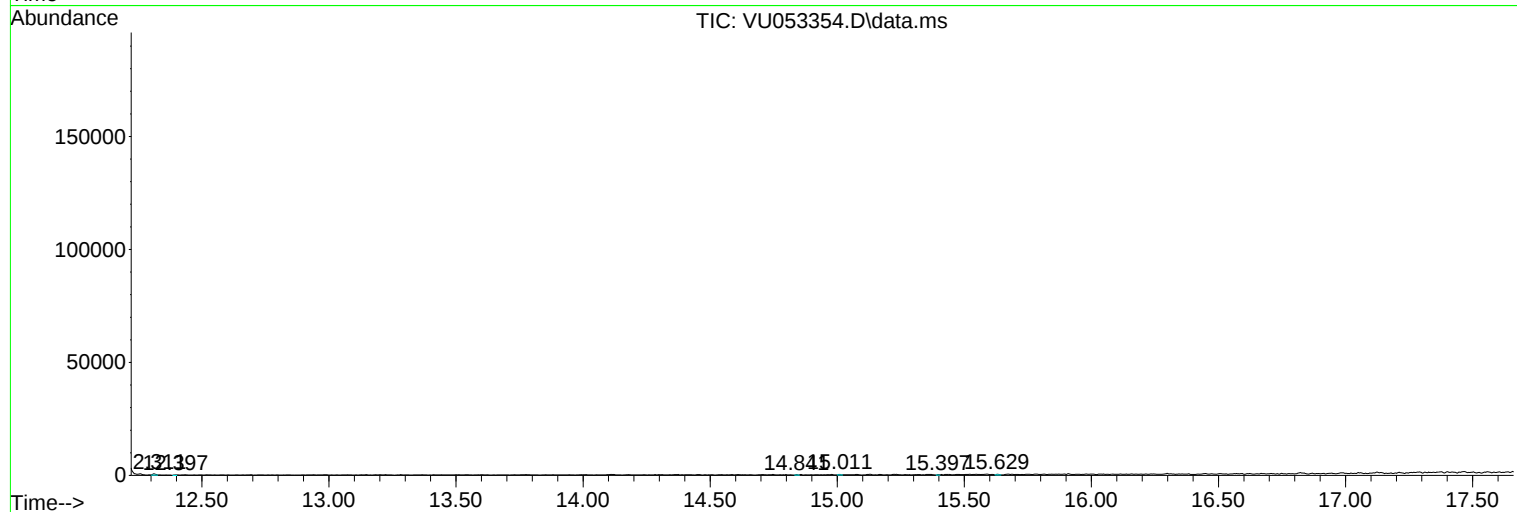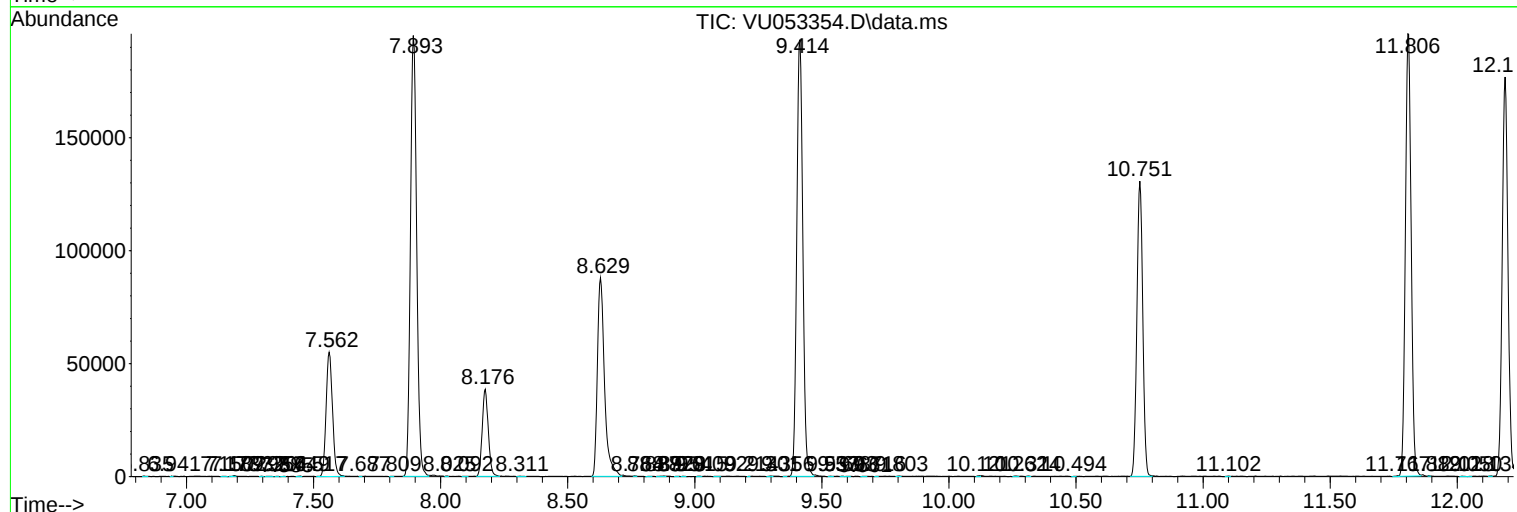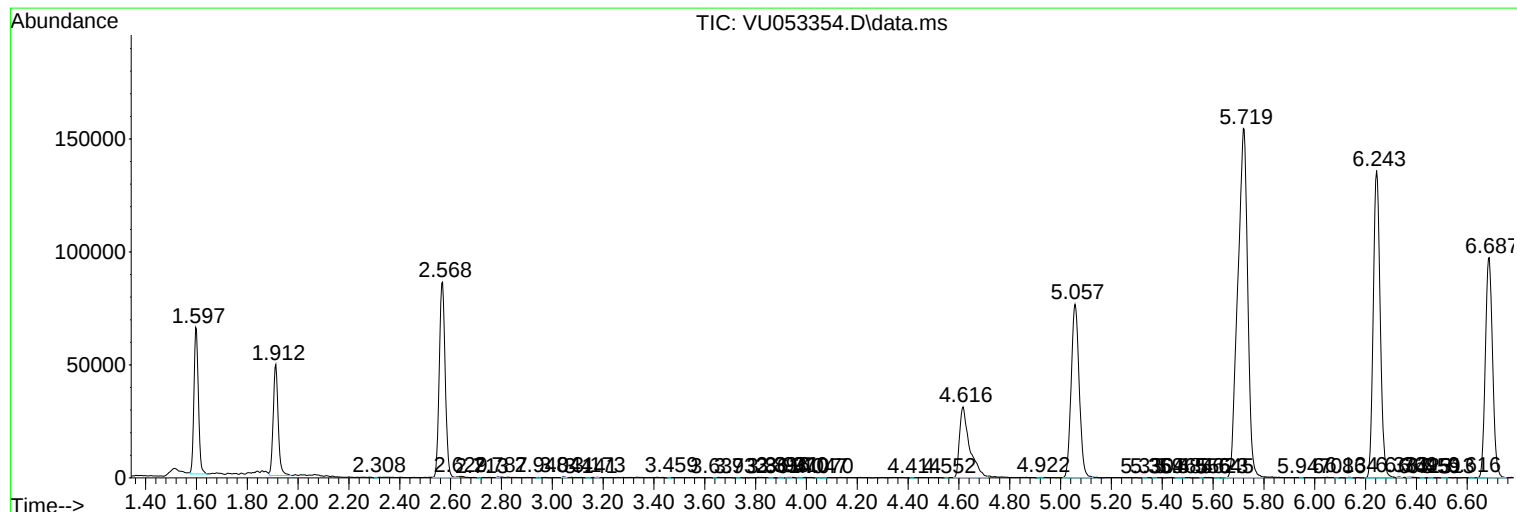

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053354.D
Acq On : 22 Mar 2023 15:57
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053354.D
Acq On : 22 Mar 2023 15:57
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------