

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053360.D
 Acq On : 22 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB2	53595	62591	16.01%	2.075%
2	1.912	171	178	192	rVB	45839	60410	15.46%	2.003%
3	2.565	370	381	393	rBV	74257	119073	30.47%	3.948%
4	3.202	575	579	584	rBV	130	166	0.04%	0.006%
5	3.353	621	626	634	rVB3	465	413	0.11%	0.014%
6	3.597	694	702	705	rBV	233	330	0.08%	0.011%
7	3.723	737	741	746	rBV	193	255	0.07%	0.008%
8	3.890	788	793	796	rBV	222	265	0.07%	0.009%
9	4.018	830	833	838	rBV	162	224	0.06%	0.007%
10	4.231	893	899	905	rBV	230	398	0.10%	0.013%
11	4.285	914	916	919	rBV	131	114	0.03%	0.004%
12	4.356	927	938	941	rBV	254	436	0.11%	0.014%
13	4.408	951	954	956	rBV	180	145	0.04%	0.005%
14	4.453	965	968	971	rBB	171	134	0.03%	0.004%
15	4.517	986	988	991	rBV	204	161	0.04%	0.005%
16	4.552	996	999	1001	rBV	184	150	0.04%	0.005%
17	4.620	1008	1020	1045	rBV2	30192	79408	20.32%	2.633%
18	4.819	1079	1082	1084	rBV2	144	125	0.03%	0.004%
19	4.912	1110	1111	1115	rVB	313	165	0.04%	0.005%
20	5.057	1141	1156	1185	rBB	73151	158668	40.60%	5.261%
21	5.202	1196	1201	1206	rBB	168	216	0.06%	0.007%
22	5.224	1206	1208	1212	rBV	126	129	0.03%	0.004%
23	5.414	1262	1267	1271	rBV	154	230	0.06%	0.008%
24	5.469	1281	1284	1286	rBB	162	109	0.03%	0.004%
25	5.485	1286	1289	1293	rBV	155	180	0.05%	0.006%
26	5.559	1309	1312	1314	rBV	181	147	0.04%	0.005%
27	5.719	1342	1362	1388	rBV3	143192	390831	100.00%	12.958%
28	5.858	1403	1405	1410	rBV	282	248	0.06%	0.008%
29	5.887	1410	1414	1416	rVV2	173	157	0.04%	0.005%
30	6.002	1441	1450	1454	rBV	154	305	0.08%	0.010%
31	6.102	1478	1481	1483	rBV	180	144	0.04%	0.005%
32	6.243	1512	1525	1541	rBV	125840	235623	60.29%	7.812%
33	6.366	1560	1563	1566	rBV	199	161	0.04%	0.005%
34	6.488	1597	1601	1604	rBB	143	145	0.04%	0.005%
35	6.510	1605	1608	1610	rBV	147	123	0.03%	0.004%
36	6.530	1610	1614	1617	rVV	296	289	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053360.D
 Acq On : 22 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.549	1617	1620	1624	rVB2	540	384	0.10%	0.013%
38	6.575	1625	1628	1632	rBV	149	182	0.05%	0.006%
39	6.684	1650	1662	1684	rVB	94178	181823	46.52%	6.028%
40	6.768	1684	1688	1691	rVB	517	374	0.10%	0.012%
41	6.790	1692	1695	1698	rBV	187	183	0.05%	0.006%
42	6.848	1710	1713	1715	rBV	144	124	0.03%	0.004%
43	6.941	1740	1742	1749	rBB	182	196	0.05%	0.006%
44	6.973	1750	1752	1755	rBV	198	148	0.04%	0.005%
45	7.070	1780	1782	1785	rBV	172	138	0.04%	0.005%
46	7.131	1798	1801	1804	rBV	150	155	0.04%	0.005%
47	7.189	1816	1819	1824	rVB	250	221	0.06%	0.007%
48	7.247	1834	1837	1840	rBB	201	147	0.04%	0.005%
49	7.276	1841	1846	1849	rBV	182	231	0.06%	0.008%
50	7.327	1859	1862	1865	rBV	199	175	0.04%	0.006%
51	7.356	1869	1871	1873	rBV	174	117	0.03%	0.004%
52	7.562	1923	1935	1956	rBV2	51858	90433	23.14%	2.998%
53	7.703	1977	1979	1983	rVB	278	188	0.05%	0.006%
54	7.848	2021	2024	2025	rBV	148	108	0.03%	0.004%
55	7.893	2025	2038	2056	rVV	178572	305042	78.05%	10.114%
56	8.038	2080	2083	2089	rVB	323	288	0.07%	0.010%
57	8.070	2090	2093	2098	rBV	184	240	0.06%	0.008%
58	8.176	2115	2126	2143	rBV2	36333	60319	15.43%	2.000%
59	8.295	2158	2163	2167	rBV	228	307	0.08%	0.010%
60	8.378	2187	2189	2191	rBV	168	108	0.03%	0.004%
61	8.391	2191	2193	2196	rVV	196	123	0.03%	0.004%
62	8.510	2224	2230	2232	rBV	174	226	0.06%	0.007%
63	8.546	2239	2241	2244	rBV	241	140	0.04%	0.005%
64	8.629	2256	2267	2295	rBV2	89298	171652	43.92%	5.691%
65	8.761	2304	2308	2311	rBV2	232	223	0.06%	0.007%
66	8.976	2369	2375	2380	rBV	272	330	0.08%	0.011%
67	9.259	2461	2463	2468	rBV	168	191	0.05%	0.006%
68	9.285	2468	2471	2475	rVB	289	233	0.06%	0.008%
69	9.308	2475	2478	2481	rBB	154	140	0.04%	0.005%
70	9.337	2482	2487	2491	rBV	217	305	0.08%	0.010%
71	9.411	2495	2510	2540	rBV	180918	304527	77.92%	10.097%
72	9.520	2542	2544	2553	rVV2	390	383	0.10%	0.013%
73	9.565	2553	2558	2564	rVV3	643	770	0.20%	0.026%
74	9.591	2564	2566	2569	rVV2	206	130	0.03%	0.004%
75	9.629	2573	2578	2580	rBV	183	198	0.05%	0.007%
76	9.693	2594	2598	2604	rVB3	507	601	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053360.D
 Acq On : 22 Mar 2023 18:20
 Operator : JC/MD
 Sample : 01961-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.758	2613	2618	2621	rBB	194	205	0.05%	0.007%
78	9.906	2660	2664	2666	rBV	205	195	0.05%	0.006%
79	10.034	2701	2704	2707	rBV	178	166	0.04%	0.006%
80	10.089	2718	2721	2723	rBV	204	153	0.04%	0.005%
81	10.118	2723	2730	2738	rVB4	1211	1702	0.44%	0.056%
82	10.337	2794	2798	2803	rVB2	231	185	0.05%	0.006%
83	10.411	2816	2821	2824	rBV	242	237	0.06%	0.008%
84	10.468	2835	2839	2840	rBV	337	232	0.06%	0.008%
85	10.751	2915	2927	2945	rVB	129869	206423	52.82%	6.844%
86	11.086	3026	3031	3039	rVB	359	452	0.12%	0.015%
87	11.468	3144	3150	3155	rBV	1089	1148	0.29%	0.038%
88	11.745	3231	3236	3241	rBV	1057	947	0.24%	0.031%
89	11.806	3244	3255	3275	rVV	180092	288506	73.82%	9.566%
90	12.189	3362	3374	3388	rBV2	167527	268207	68.62%	8.893%
91	12.308	3408	3411	3413	rBV2	231	165	0.04%	0.005%
92	12.369	3426	3430	3433	rBV	279	283	0.07%	0.009%
93	13.211	3688	3692	3694	rBV2	622	525	0.13%	0.017%
94	13.841	3881	3888	3896	rBV6	1800	2409	0.62%	0.080%
95	14.089	3956	3965	3979	rBV2	3618	5719	1.46%	0.190%
96	14.160	3985	3987	3990	rBV	156	111	0.03%	0.004%
97	14.285	4024	4026	4029	rBV	213	106	0.03%	0.004%
98	14.327	4033	4039	4047	rVB4	2332	3149	0.81%	0.104%
99	14.404	4061	4063	4071	rBV	230	234	0.06%	0.008%
100	14.899	4214	4217	4220	rBV	252	139	0.04%	0.005%




Sum of corrected areas: 3016069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053360.D
Acq On : 22 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

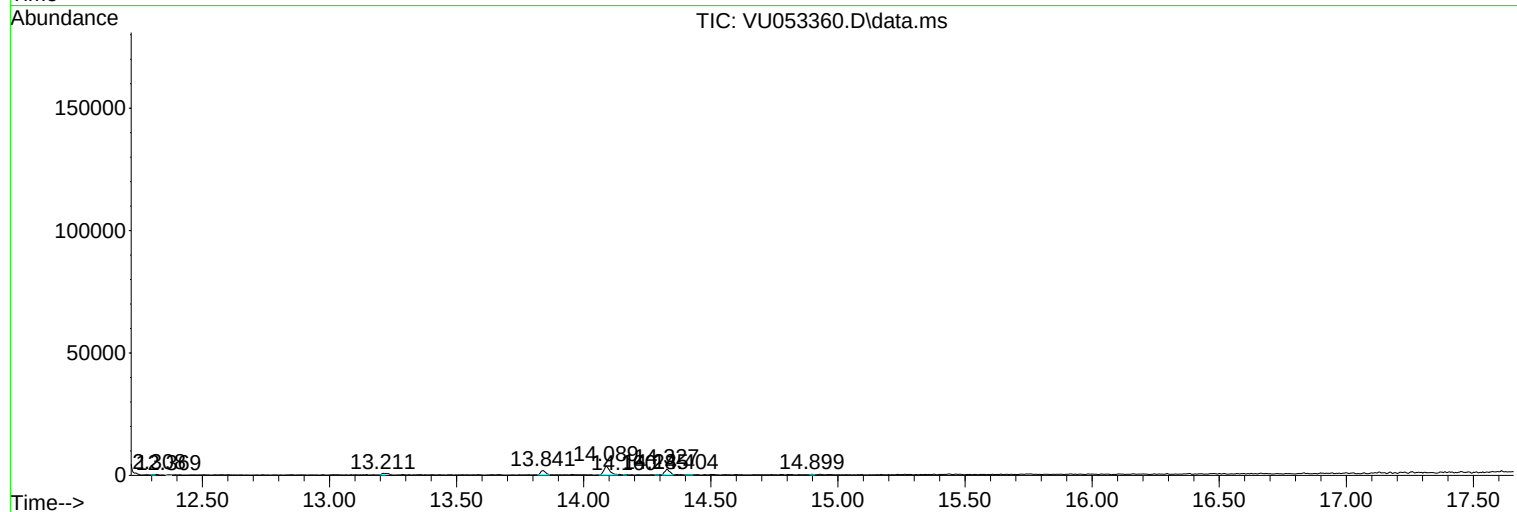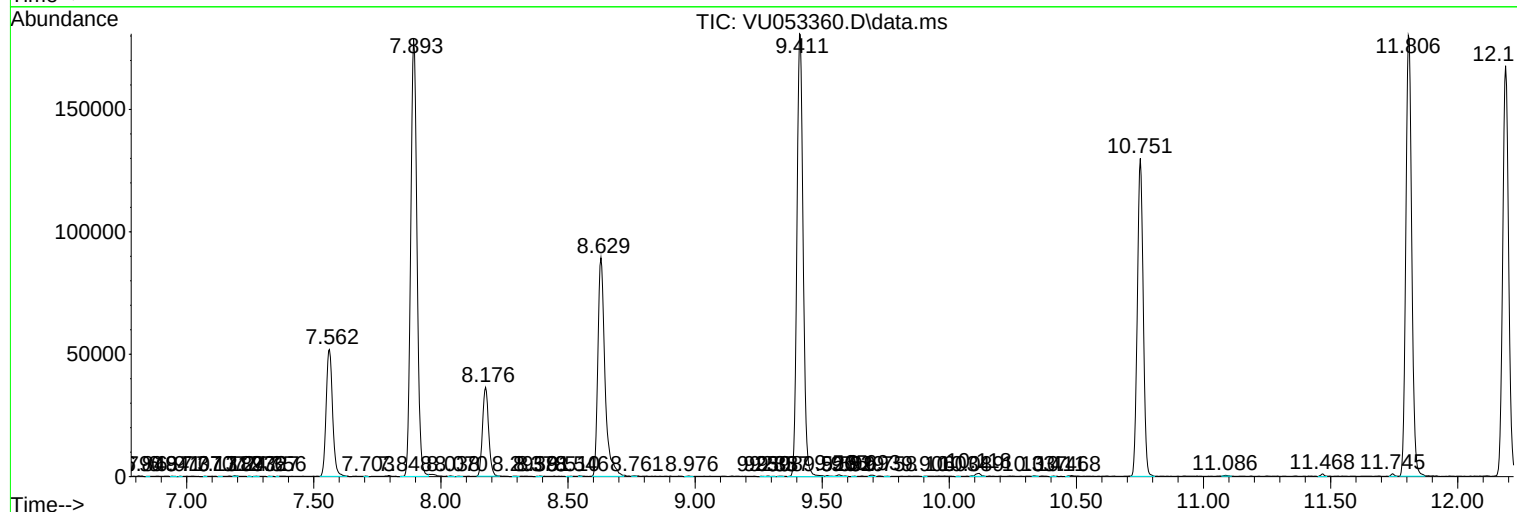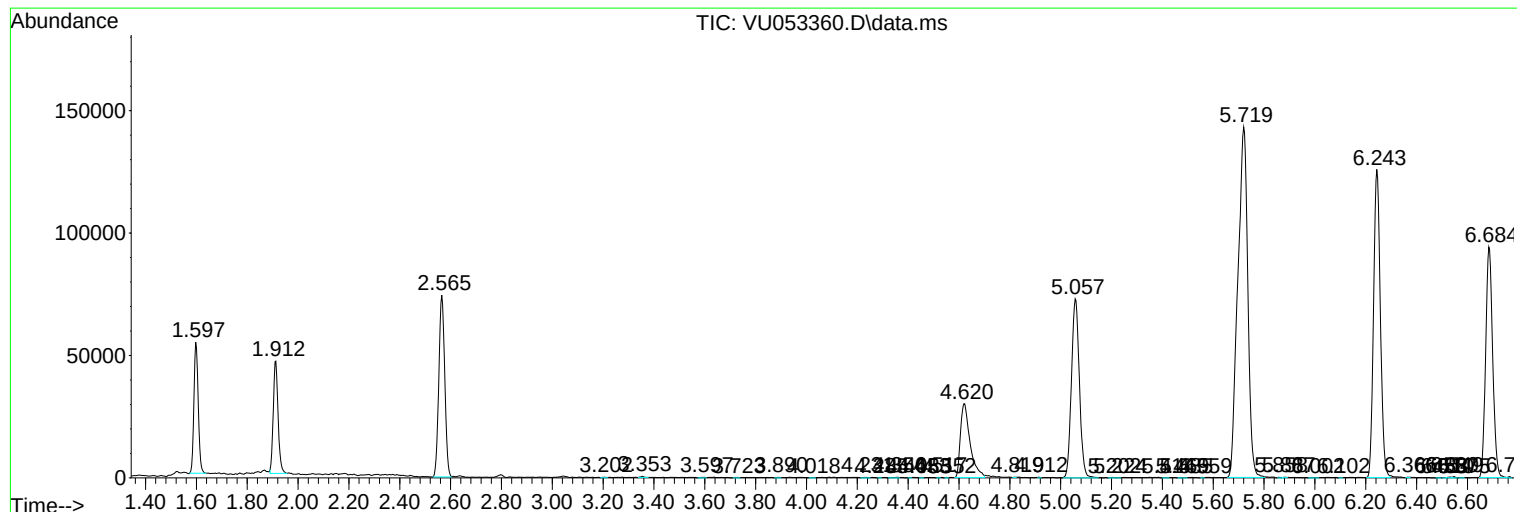

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053360.D
Acq On : 22 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053360.D
Acq On : 22 Mar 2023 18:20
Operator : JC/MD
Sample : 01961-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------