

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053361.D
 Acq On : 22 Mar 2023 18:44
 Operator : JC/MD
 Sample : 01995-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	95	rVB	58540	66640	15.22%	2.026%
2	1.912	170	178	194	rVB	54649	75348	17.21%	2.290%
3	2.565	370	381	397	rVB	87842	141557	32.33%	4.303%
4	3.038	524	528	536	rVB4	721	852	0.19%	0.026%
5	3.353	623	626	629	rBV	168	113	0.03%	0.003%
6	3.475	661	664	670	rVB	196	117	0.03%	0.004%
7	3.530	678	681	684	rBV	169	168	0.04%	0.005%
8	3.816	765	770	775	rBV	179	282	0.06%	0.009%
9	3.909	795	799	801	rBV	251	222	0.05%	0.007%
10	4.025	830	835	842	rBB	223	337	0.08%	0.010%
11	4.179	878	883	885	rBV	227	235	0.05%	0.007%
12	4.513	985	987	989	rBV	126	86	0.02%	0.003%
13	4.620	1009	1020	1045	rVV	34055	87665	20.02%	2.665%
14	4.870	1093	1098	1101	rVB2	282	273	0.06%	0.008%
15	4.893	1102	1105	1107	rBV	173	118	0.03%	0.004%
16	4.925	1113	1115	1117	rBV	147	97	0.02%	0.003%
17	5.057	1141	1156	1178	rBV	80228	175473	40.08%	5.333%
18	5.295	1226	1230	1236	rBV	223	356	0.08%	0.011%
19	5.369	1251	1253	1258	rVB	304	246	0.06%	0.007%
20	5.398	1259	1262	1264	rBV	158	129	0.03%	0.004%
21	5.446	1274	1277	1278	rBV	113	84	0.02%	0.003%
22	5.549	1306	1309	1312	rBV	189	176	0.04%	0.005%
23	5.607	1325	1327	1328	rBV	150	85	0.02%	0.003%
24	5.613	1328	1329	1332	rVV	177	82	0.02%	0.002%
25	5.719	1341	1362	1383	rBV2	158155	437810	100.00%	13.307%
26	5.845	1399	1401	1403	rBV	197	122	0.03%	0.004%
27	5.896	1412	1417	1421	rBV	270	347	0.08%	0.011%
28	5.954	1432	1435	1437	rBV	154	133	0.03%	0.004%
29	6.012	1450	1453	1456	rBB	169	144	0.03%	0.004%
30	6.054	1463	1466	1471	rVB2	184	133	0.03%	0.004%
31	6.124	1486	1488	1490	rBV	124	90	0.02%	0.003%
32	6.189	1505	1508	1511	rBB	187	146	0.03%	0.004%
33	6.243	1512	1525	1553	rVV	132253	248109	56.67%	7.541%
34	6.472	1593	1596	1600	rBB	180	180	0.04%	0.005%
35	6.501	1603	1605	1608	rBB	256	124	0.03%	0.004%
36	6.542	1615	1618	1620	rBV	259	184	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053361.D
 Acq On : 22 Mar 2023 18:44
 Operator : JC/MD
 Sample : 01995-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.684	1649	1662	1680	rBV2	103001	199665	45.61%	6.069%
38	6.758	1683	1685	1687	rVB	193	79	0.02%	0.002%
39	6.771	1687	1689	1691	rVB	279	126	0.03%	0.004%
40	6.787	1692	1694	1698	rBV	146	154	0.04%	0.005%
41	6.915	1731	1734	1739	rBV	165	203	0.05%	0.006%
42	6.944	1740	1743	1747	rVV	211	164	0.04%	0.005%
43	7.005	1755	1762	1767	rBB	246	320	0.07%	0.010%
44	7.037	1770	1772	1776	rBV	190	182	0.04%	0.006%
45	7.134	1796	1802	1807	rBV	167	257	0.06%	0.008%
46	7.308	1848	1856	1859	rBB	205	323	0.07%	0.010%
47	7.346	1866	1868	1870	rBV	150	102	0.02%	0.003%
48	7.391	1880	1882	1884	rBB	150	77	0.02%	0.002%
49	7.407	1884	1887	1889	rBV	132	111	0.03%	0.003%
50	7.475	1905	1908	1912	rBB	175	137	0.03%	0.004%
51	7.562	1923	1935	1952	rBV2	57599	100754	23.01%	3.062%
52	7.690	1970	1975	1976	rBV	276	197	0.04%	0.006%
53	7.735	1986	1989	1991	rVB	248	135	0.03%	0.004%
54	7.764	1992	1998	2001	rBV	274	333	0.08%	0.010%
55	7.893	2025	2038	2057	rBV	202996	344527	78.69%	10.472%
56	8.012	2071	2075	2081	rVB2	343	393	0.09%	0.012%
57	8.111	2103	2106	2107	rBV	171	119	0.03%	0.004%
58	8.176	2113	2126	2142	rBB2	40935	68487	15.64%	2.082%
59	8.250	2142	2149	2150	rBV	179	222	0.05%	0.007%
60	8.349	2178	2180	2182	rBV	133	97	0.02%	0.003%
61	8.439	2205	2208	2210	rBV	173	145	0.03%	0.004%
62	8.478	2216	2220	2226	rBV	183	279	0.06%	0.008%
63	8.545	2239	2241	2243	rBV	138	94	0.02%	0.003%
64	8.558	2243	2245	2253	rVB2	259	276	0.06%	0.008%
65	8.629	2256	2267	2296	rVV2	97822	186967	42.71%	5.683%
66	8.764	2305	2309	2312	rVB2	235	173	0.04%	0.005%
67	8.922	2356	2358	2360	rBV	170	121	0.03%	0.004%
68	8.986	2375	2378	2384	rBV	176	242	0.06%	0.007%
69	9.037	2391	2394	2397	rBV	201	113	0.03%	0.003%
70	9.266	2462	2465	2466	rBV	194	140	0.03%	0.004%
71	9.414	2499	2511	2529	rBV	189310	310781	70.99%	9.446%
72	9.526	2543	2546	2550	rBV2	191	207	0.05%	0.006%
73	9.658	2585	2587	2590	rBV	176	147	0.03%	0.004%
74	10.050	2706	2709	2712	rBB	220	159	0.04%	0.005%
75	10.073	2713	2716	2721	rBV	243	281	0.06%	0.009%
76	10.121	2725	2731	2739	rVV5	843	971	0.22%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053361.D
 Acq On : 22 Mar 2023 18:44
 Operator : JC/MD
 Sample : 01995-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.304	2784	2788	2791	rBV	188	204	0.05%	0.006%
78	10.488	2842	2845	2848	rVB2	200	140	0.03%	0.004%
79	10.597	2876	2879	2882	rBV	160	153	0.03%	0.005%
80	10.661	2897	2899	2901	rBV	144	103	0.02%	0.003%
81	10.751	2914	2927	2944	rBV	142060	223457	51.04%	6.792%
82	11.272	3086	3089	3096	rVB	284	378	0.09%	0.011%
83	11.307	3097	3100	3101	rBV	158	110	0.03%	0.003%
84	11.465	3147	3149	3150	rBV	450	208	0.05%	0.006%
85	11.674	3211	3214	3217	rVB	168	95	0.02%	0.003%
86	11.745	3231	3236	3242	rVB	480	544	0.12%	0.017%
87	11.806	3243	3255	3278	rBV	191190	305047	69.68%	9.272%
88	11.950	3298	3300	3306	rVB2	201	148	0.03%	0.004%
89	12.188	3362	3374	3390	rBV	186789	300028	68.53%	9.119%
90	12.561	3488	3490	3491	rBV	158	85	0.02%	0.003%
91	13.214	3690	3693	3700	rVB2	356	339	0.08%	0.010%
92	13.317	3723	3725	3727	rBV	157	104	0.02%	0.003%
93	13.478	3770	3775	3778	rBV	274	338	0.08%	0.010%
94	13.847	3883	3890	3897	rVB2	723	987	0.23%	0.030%
95	14.166	3986	3989	3993	rBV	301	178	0.04%	0.005%
96	14.925	4222	4225	4227	rBV	374	230	0.05%	0.007%
97	14.970	4237	4239	4242	rBV2	229	145	0.03%	0.004%
98	15.108	4279	4282	4285	rBV2	272	180	0.04%	0.005%
99	15.256	4326	4328	4332	rVB	286	176	0.04%	0.005%
100	15.278	4332	4335	4336	rBV	254	135	0.03%	0.004%




Sum of corrected areas: 3290035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053361.D
Acq On : 22 Mar 2023 18:44
Operator : JC/MD
Sample : 01995-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

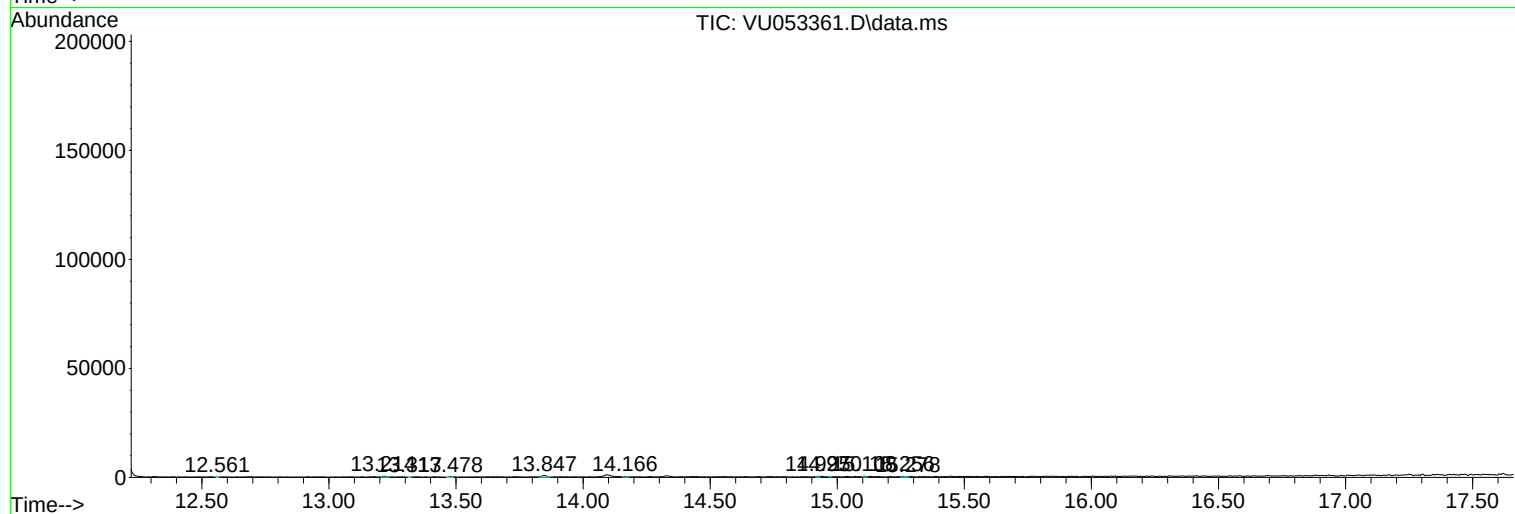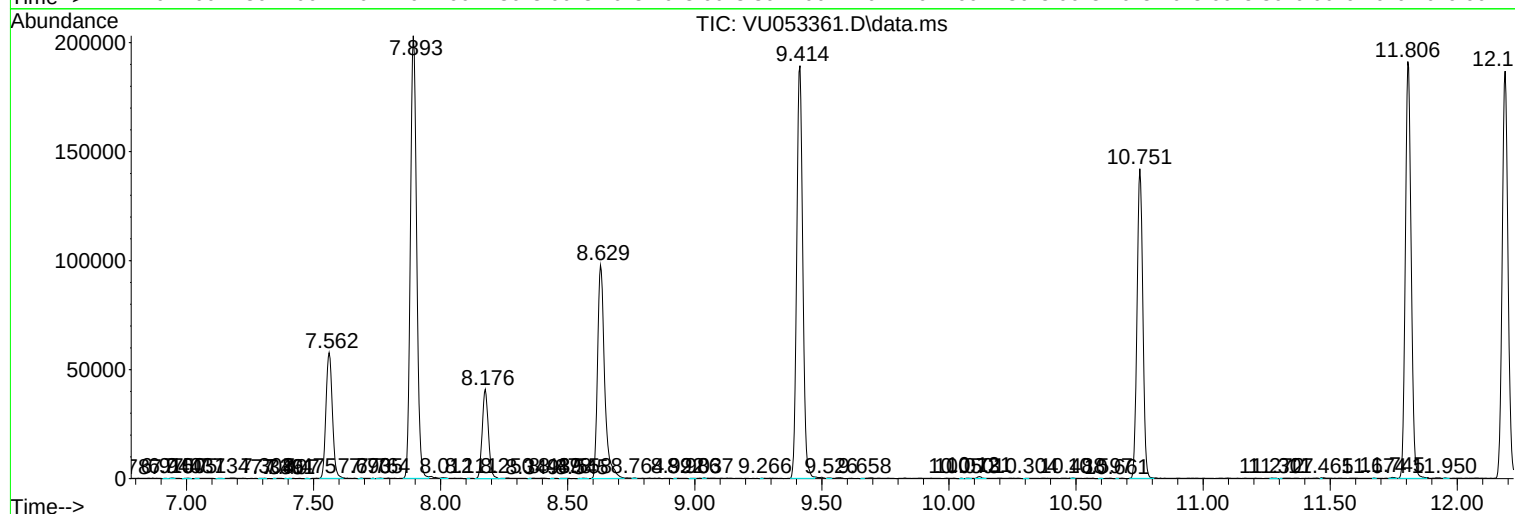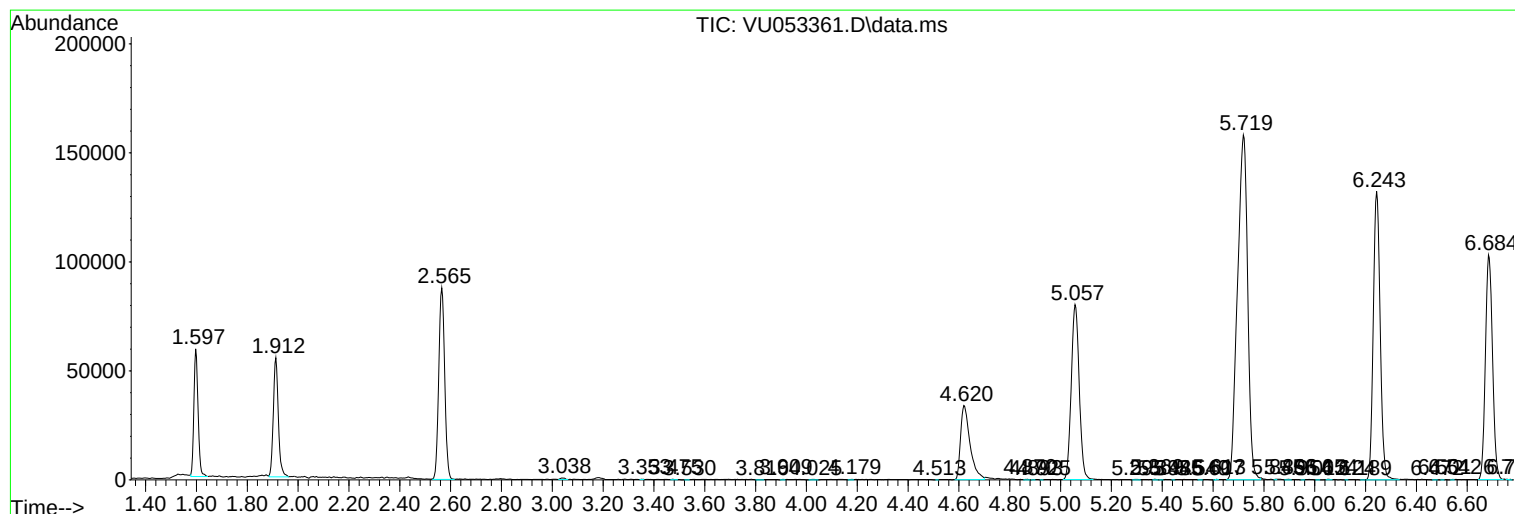

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053361.D
Acq On : 22 Mar 2023 18:44
Operator : JC/MD
Sample : 01995-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053361.D
Acq On : 22 Mar 2023 18:44
Operator : JC/MD
Sample : 01995-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------