

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053362.D
 Acq On : 22 Mar 2023 19:08
 Operator : JC/MD
 Sample : 01961-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	55412	64438	14.88%	1.976%
2	1.912	170	178	194	rVB	53337	74498	17.20%	2.284%
3	2.565	369	381	397	rVB	88838	141132	32.59%	4.327%
4	3.047	525	531	538	rVB3	514	637	0.15%	0.020%
5	3.170	564	569	571	rBV2	724	710	0.16%	0.022%
6	4.002	826	828	831	rBV	164	131	0.03%	0.004%
7	4.160	873	877	879	rBV	227	232	0.05%	0.007%
8	4.305	919	922	926	rBB	152	150	0.03%	0.005%
9	4.440	961	964	967	rBV	215	205	0.05%	0.006%
10	4.546	995	997	999	rBV	142	101	0.02%	0.003%
11	4.623	1007	1021	1047	rBV2	34109	88247	20.38%	2.705%
12	4.935	1114	1118	1120	rBV	141	115	0.03%	0.004%
13	5.057	1142	1156	1173	rBV2	79649	171975	39.71%	5.272%
14	5.153	1184	1186	1195	rVB	302	337	0.08%	0.010%
15	5.256	1215	1218	1223	rBB	199	217	0.05%	0.007%
16	5.285	1224	1227	1229	rBV	173	148	0.03%	0.005%
17	5.481	1286	1288	1290	rBV	161	113	0.03%	0.003%
18	5.536	1302	1305	1311	rBV	270	325	0.08%	0.010%
19	5.719	1342	1362	1386	rBV2	159291	433069	100.00%	13.277%
20	5.916	1419	1423	1426	rBB	188	142	0.03%	0.004%
21	5.951	1430	1434	1437	rBB	151	125	0.03%	0.004%
22	5.996	1445	1448	1453	rBB	205	208	0.05%	0.006%
23	6.034	1458	1460	1462	rBV	168	120	0.03%	0.004%
24	6.108	1480	1483	1485	rBV	189	156	0.04%	0.005%
25	6.176	1500	1504	1508	rBV	203	262	0.06%	0.008%
26	6.243	1512	1525	1544	rBV	131733	248354	57.35%	7.614%
27	6.353	1556	1559	1561	rBV	291	221	0.05%	0.007%
28	6.401	1571	1574	1577	rBV	307	264	0.06%	0.008%
29	6.430	1580	1583	1586	rBV	203	190	0.04%	0.006%
30	6.517	1604	1610	1611	rBV	259	227	0.05%	0.007%
31	6.526	1611	1613	1615	rBV	236	104	0.02%	0.003%
32	6.571	1625	1627	1629	rBV	151	102	0.02%	0.003%
33	6.620	1640	1642	1645	rBV	167	135	0.03%	0.004%
34	6.684	1648	1662	1685	rVB	104405	200182	46.22%	6.137%
35	6.790	1692	1695	1697	rBV	142	123	0.03%	0.004%
36	6.803	1697	1699	1704	rBV	219	118	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053362.D
 Acq On : 22 Mar 2023 19:08
 Operator : JC/MD
 Sample : 01961-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.858	1714	1716	1718	rBV	158	107	0.02%	0.003%
38	7.025	1766	1768	1772	rVB	313	202	0.05%	0.006%
39	7.051	1773	1776	1778	rBV	155	133	0.03%	0.004%
40	7.141	1800	1804	1805	rBV	199	162	0.04%	0.005%
41	7.189	1814	1819	1824	rBV2	391	486	0.11%	0.015%
42	7.276	1841	1846	1847	rBV	223	140	0.03%	0.004%
43	7.362	1868	1873	1875	rBV	200	229	0.05%	0.007%
44	7.401	1882	1885	1888	rBV	201	189	0.04%	0.006%
45	7.449	1895	1900	1902	rBV	208	182	0.04%	0.006%
46	7.562	1923	1935	1955	rBV	58842	100831	23.28%	3.091%
47	7.716	1979	1983	1986	rBV	167	181	0.04%	0.006%
48	7.809	2007	2012	2014	rBV	181	203	0.05%	0.006%
49	7.893	2026	2038	2056	rBV	198184	337886	78.02%	10.359%
50	8.073	2091	2094	2096	rBV	166	125	0.03%	0.004%
51	8.176	2114	2126	2147	rVB	41210	68182	15.74%	2.090%
52	8.263	2150	2153	2157	rVV	187	111	0.03%	0.003%
53	8.304	2164	2166	2169	rBV	194	143	0.03%	0.004%
54	8.343	2175	2178	2181	rBV	191	192	0.04%	0.006%
55	8.382	2188	2190	2192	rBV	148	102	0.02%	0.003%
56	8.423	2198	2203	2206	rBV	217	240	0.06%	0.007%
57	8.513	2228	2231	2233	rBV	205	165	0.04%	0.005%
58	8.629	2255	2267	2295	rBV2	98768	187487	43.29%	5.748%
59	9.031	2387	2392	2396	rBB	214	214	0.05%	0.007%
60	9.218	2447	2450	2452	rBB	183	115	0.03%	0.004%
61	9.247	2453	2459	2463	rBB	239	303	0.07%	0.009%
62	9.269	2463	2466	2468	rBV	173	137	0.03%	0.004%
63	9.411	2499	2510	2530	rBV	185053	309455	71.46%	9.487%
64	9.655	2579	2586	2592	rBV	265	490	0.11%	0.015%
65	9.784	2623	2626	2630	rBV	161	194	0.04%	0.006%
66	9.838	2638	2643	2646	rBV	183	218	0.05%	0.007%
67	9.890	2655	2659	2661	rBV	163	160	0.04%	0.005%
68	10.002	2692	2694	2697	rBV	149	125	0.03%	0.004%
69	10.034	2701	2704	2706	rBV	163	133	0.03%	0.004%
70	10.118	2725	2730	2734	rBV2	798	850	0.20%	0.026%
71	10.195	2750	2754	2756	rBV	175	171	0.04%	0.005%
72	10.320	2789	2793	2797	rBV	228	249	0.06%	0.008%
73	10.629	2886	2889	2891	rBV	171	145	0.03%	0.004%
74	10.751	2911	2927	2945	rBV	141509	221941	51.25%	6.804%
75	10.857	2957	2960	2962	rBV	160	140	0.03%	0.004%
76	10.919	2975	2979	2981	rBV	196	193	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
 Data File : VU053362.D
 Acq On : 22 Mar 2023 19:08
 Operator : JC/MD
 Sample : 01961-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.275	3086	3090	3092	rBV	157	158	0.04%	0.005%
78	11.340	3107	3110	3112	rBV	175	139	0.03%	0.004%
79	11.401	3126	3129	3134	rVB	248	202	0.05%	0.006%
80	11.597	3187	3190	3193	rBV	179	174	0.04%	0.005%
81	11.738	3231	3234	3236	rBV	312	177	0.04%	0.005%
82	11.806	3244	3255	3273	rBV	185711	295955	68.34%	9.073%
83	11.992	3307	3313	3316	rBV	251	316	0.07%	0.010%
84	12.189	3361	3374	3394	rBV	184878	299921	69.25%	9.195%
85	12.308	3407	3411	3412	rBV2	247	214	0.05%	0.007%
86	13.205	3686	3690	3695	rBV	262	391	0.09%	0.012%
87	13.307	3719	3722	3727	rVB2	222	157	0.04%	0.005%
88	13.844	3886	3889	3891	rBV	348	197	0.05%	0.006%
89	14.098	3960	3968	3971	rBV2	635	787	0.18%	0.024%
90	14.327	4036	4039	4046	rVB2	472	509	0.12%	0.016%
91	14.835	4195	4197	4201	rVB	279	119	0.03%	0.004%
92	14.899	4215	4217	4220	rBV	220	108	0.02%	0.003%
93	14.944	4228	4231	4237	rBV2	230	239	0.06%	0.007%
94	15.089	4273	4276	4279	rBV	336	189	0.04%	0.006%
95	15.188	4303	4307	4310	rBV2	384	405	0.09%	0.012%
96	15.301	4339	4342	4345	rBV	260	154	0.04%	0.005%
97	15.478	4394	4397	4401	rBV	218	128	0.03%	0.004%
98	15.590	4429	4432	4434	rBV	210	110	0.03%	0.003%
99	15.709	4465	4469	4471	rBV	303	256	0.06%	0.008%
100	15.941	4538	4541	4542	rBV	211	121	0.03%	0.004%




Sum of corrected areas: 3261850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053362.D
Acq On : 22 Mar 2023 19:08
Operator : JC/MD
Sample : 01961-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

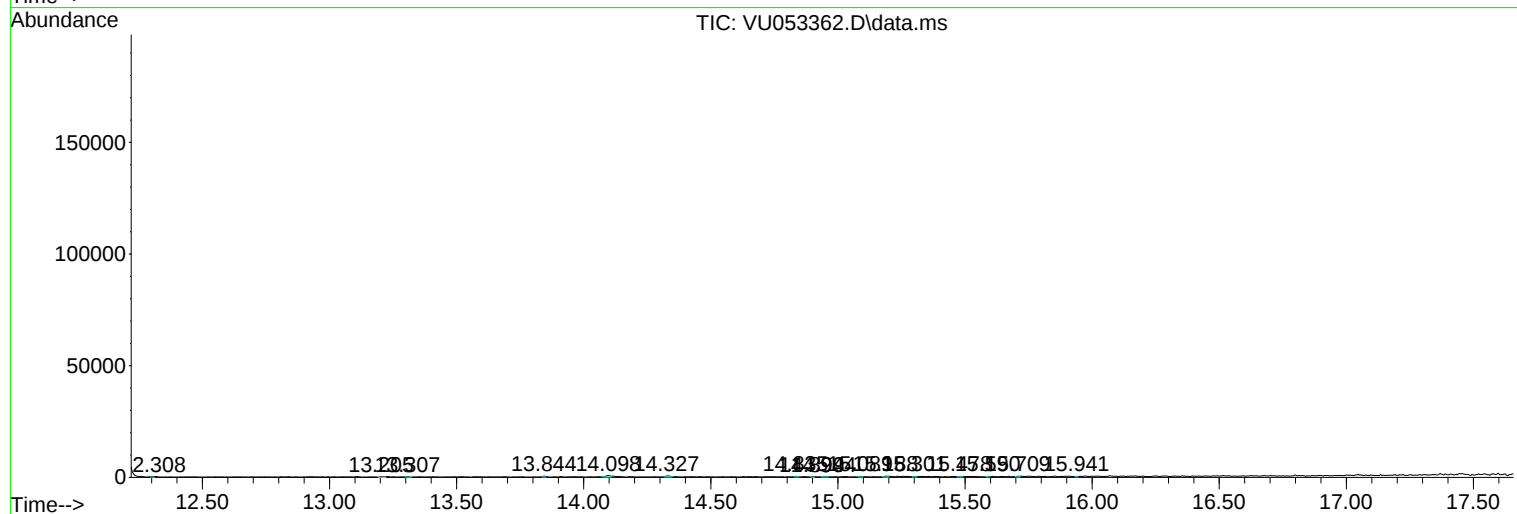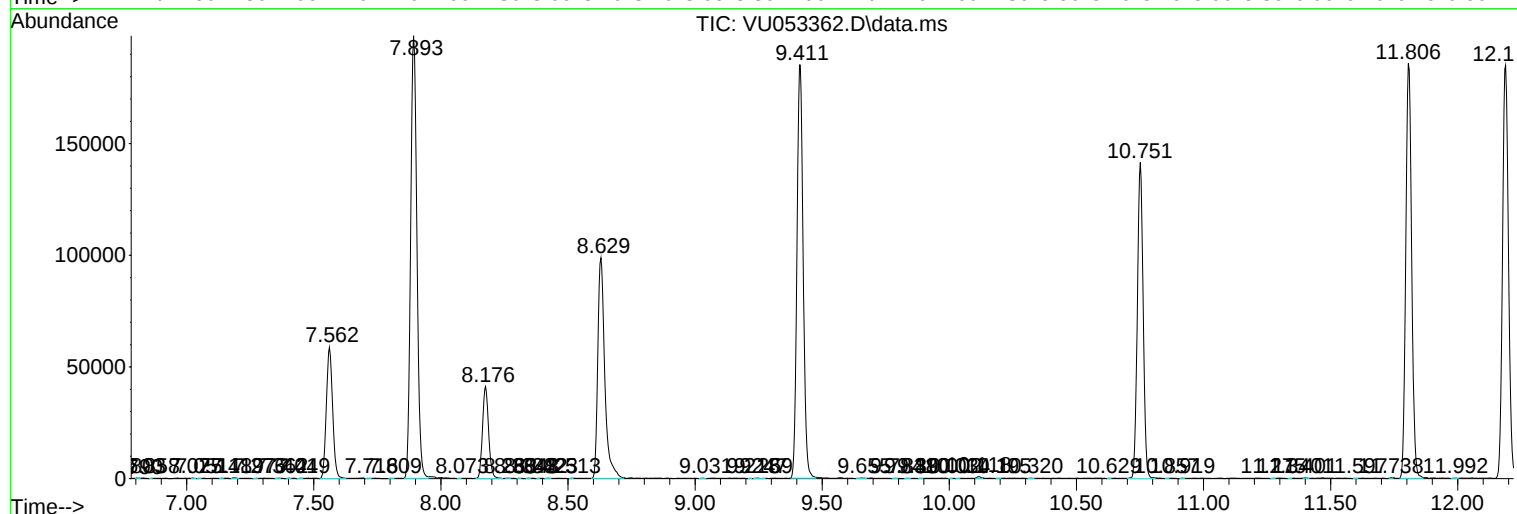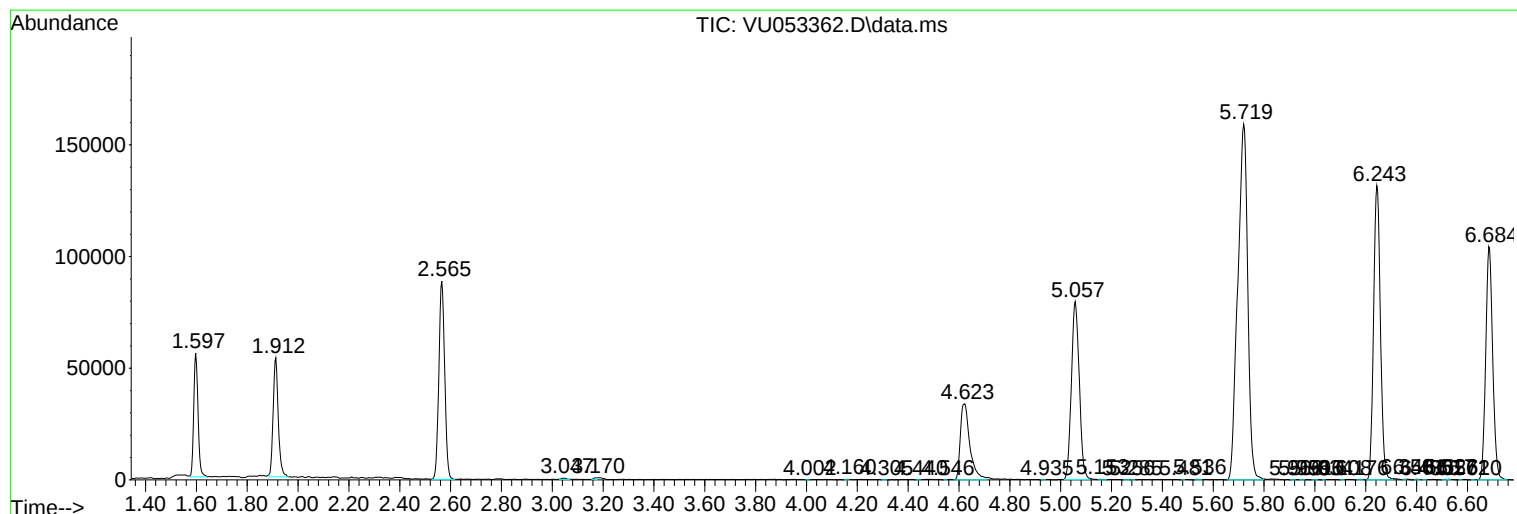

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053362.D
Acq On : 22 Mar 2023 19:08
Operator : JC/MD
Sample : 01961-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053362.D
Acq On : 22 Mar 2023 19:08
Operator : JC/MD
Sample : 01961-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------