


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032223\
Data File : VU053339.D
Acq On : 22 Mar 2023 09:35
Operator : JC/MD
Sample : BFB168
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB168

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Thu Mar 23 02:41:20 2023

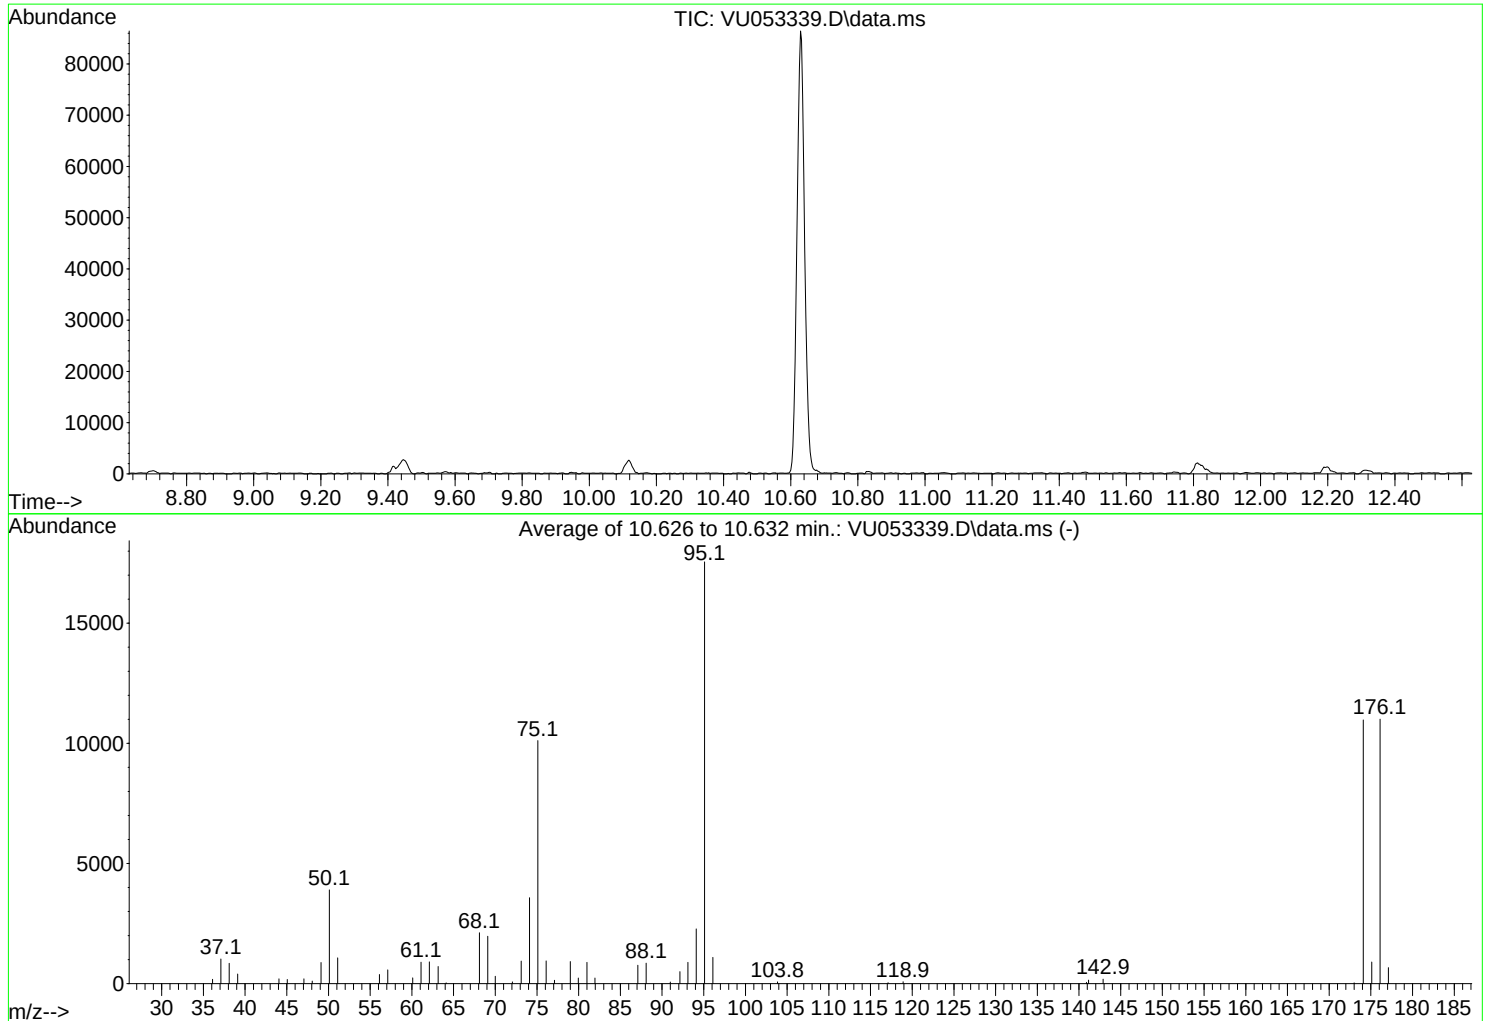

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	3905	PASS
75	95	30	80	57.6	10111	PASS
95	95	100	100	100.0	17552	PASS
96	95	5	9	6.2	1094	PASS
173	174	0.00	2	0.3	34	PASS
174	95	50	120	62.5	10974	PASS
175	174	5	9	8.2	901	PASS
176	174	95	101	100.3	11007	PASS
177	176	5	9	6.1	669	PASS

m/z	Abundance
44.10	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
36.10	109.0
37.10	1009.0
38.10	769.0
39.10	447.0
44.00	343.0
45.10	153.0
47.10	160.0
48.00	113.0
49.10	931.0
50.10	3605.0
51.10	1032.0
56.10	386.0
57.10	571.0
60.10	208.0
61.10	829.0
62.10	875.0
63.20	675.0
64.10	100.0
68.10	2062.0
69.10	1890.0
70.00	287.0
73.10	933.0
74.10	3255.0
75.10	9566.0
76.10	876.0
77.10	163.0
79.00	876.0
80.00	238.0
81.00	862.0
82.00	230.0
87.10	693.0
88.10	752.0
91.00	105.0
92.10	423.0
93.10	898.0
94.10	2136.0
95.10	16880.0
96.10	1196.0
117.10	110.0
141.10	118.0
142.90	192.0
173.00	101.0
174.10	10535.0
175.10	768.0
176.10	10178.0
177.10	712.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
36.10	187.0
37.10	1093.0
38.10	897.0
39.10	414.0
44.10	368.0
45.00	182.0
47.10	198.0
48.00	105.0
49.10	911.0
50.10	4078.0
51.10	1089.0
56.10	380.0
57.10	622.0
60.10	266.0
61.10	884.0
62.10	929.0
63.20	745.0
68.10	2190.0
69.10	2026.0
70.00	344.0
72.00	103.0
73.10	957.0
74.10	3665.0
75.10	10556.0
76.10	1010.0
77.10	157.0
79.00	954.0
79.90	246.0
81.00	906.0
82.00	247.0
87.10	805.0
88.10	877.0
91.00	100.0
92.20	527.0
93.10	923.0
94.10	2372.0
95.10	18144.0
96.10	1125.0
103.80	112.0
118.90	114.0
141.20	161.0
142.90	198.0
174.10	11237.0
175.10	937.0
176.10	11405.0
177.10	663.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
36.10	245.0
37.10	971.0
38.10	877.0
39.10	331.0
44.10	363.0
45.00	189.0
47.00	234.0
48.10	103.0
49.10	787.0
50.10	4033.0
51.10	1086.0
56.10	364.0
57.10	524.0
60.10	255.0
61.10	956.0
62.10	909.0
63.10	725.0
68.10	2098.0
69.10	1995.0
70.00	292.0
72.10	109.0
73.10	920.0
74.10	3806.0
75.10	10212.0
76.10	952.0
77.10	110.0
79.00	926.0
79.90	213.0
81.00	892.0
81.90	219.0
87.10	795.0
88.10	928.0
92.10	553.0
93.10	831.0
94.10	2318.0
95.10	17632.0
96.10	961.0
103.90	112.0
118.90	120.0
140.90	168.0
141.10	165.0
142.90	165.0
174.10	11149.0
175.10	999.0
176.10	11439.0
177.10	632.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168