


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032224\
Data File : VU058187.D
Acq On : 22 Mar 2024 11:09
Operator : MD/SY
Sample : BFB128
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB128

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 22 23:43:24 2024

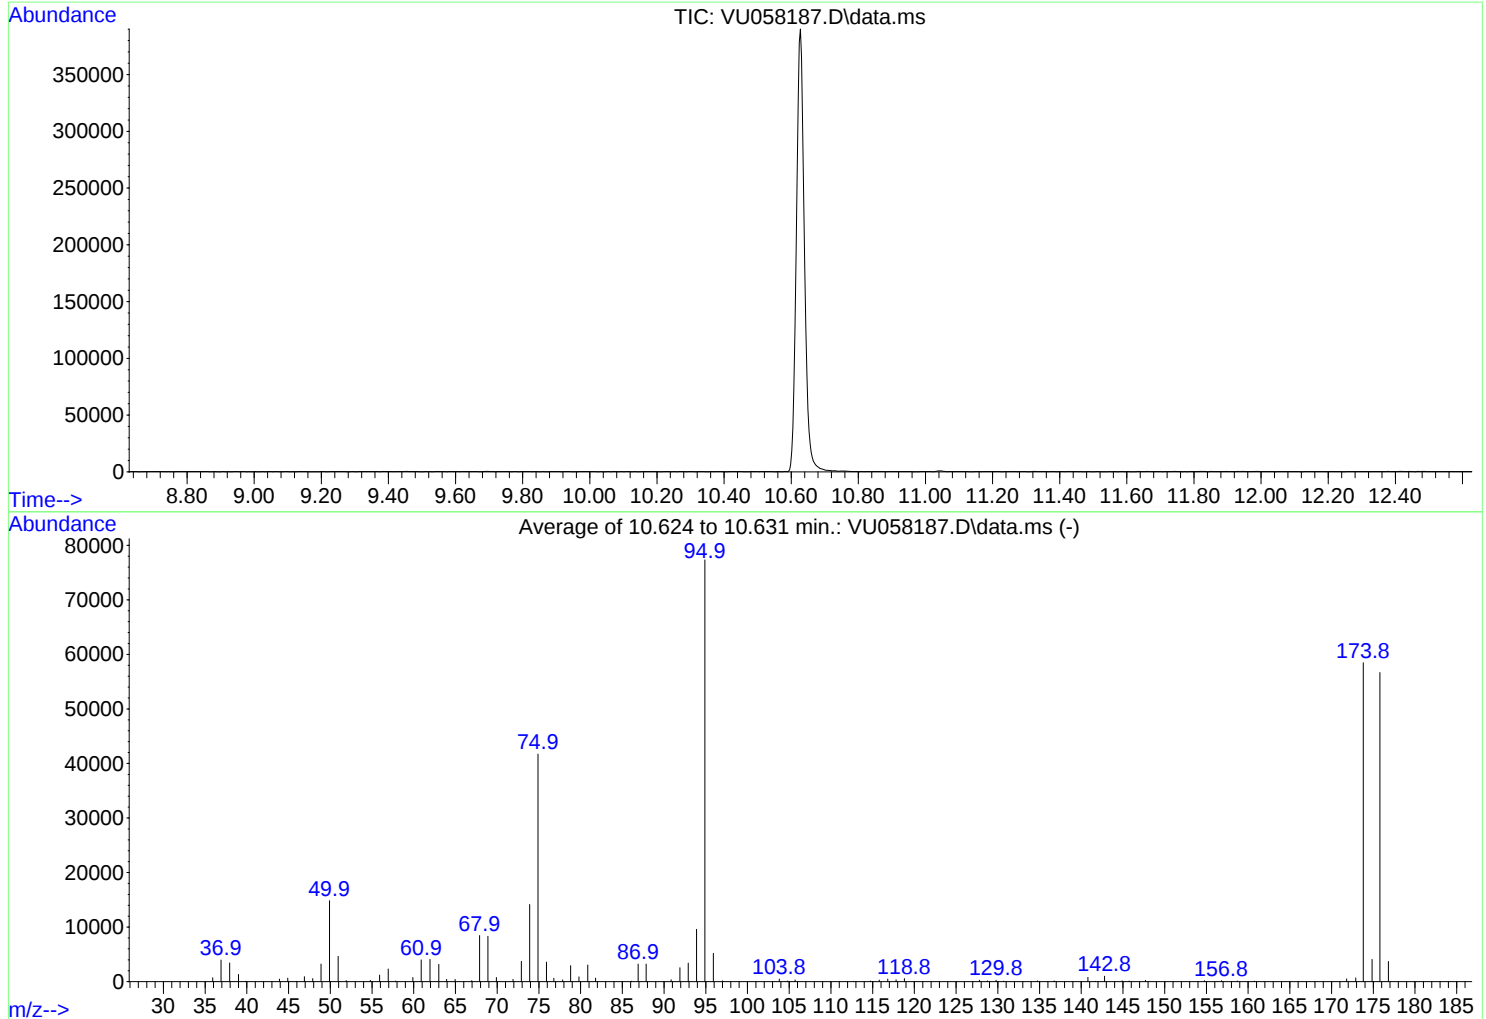

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	14839	PASS
75	95	30	80	54.0	41731	PASS
95	95	100	100	100.0	77336	PASS
96	95	5	9	6.7	5206	PASS
173	174	0.00	2	1.2	680	PASS
174	95	50	120	75.6	58477	PASS
175	174	5	9	7.0	4092	PASS
176	174	95	101	96.9	56688	PASS
177	176	5	9	6.5	3707	PASS

Scan 2890 (10.582 min): VU058187.D\data.ms
BFB128

m/z	Abundance
39.80	129.0
43.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.90	712.0
36.90	3936.0
38.00	3378.0
39.00	1424.0
39.90	174.0
43.90	710.0
44.90	636.0
46.90	902.0
47.90	604.0
48.90	3376.0
49.90	15140.0
51.00	4818.0
51.90	215.0
54.80	237.0
55.90	1131.0
57.00	2312.0
57.90	123.0
59.90	801.0
60.90	4100.0
61.90	4089.0
63.00	3175.0
64.00	436.0
64.90	425.0
67.00	170.0
67.90	8560.0
68.90	8291.0
69.90	760.0
71.90	409.0
72.90	3595.0
73.90	14447.0
74.90	42160.0
75.90	3588.0
76.80	646.0
77.90	334.0
78.80	2825.0
79.80	889.0
80.90	3069.0
81.80	614.0
86.10	101.0
86.90	3216.0
87.80	3276.0
90.90	333.0
91.90	2584.0
92.90	3442.0
93.90	9484.0
94.90	77608.0
95.90	5362.0
97.00	166.0
103.80	417.0
104.80	113.0
105.70	301.0
112.70	102.0
114.80	129.0
115.80	294.0
116.80	468.0
117.80	394.0
118.80	579.0
127.80	272.0
128.70	145.0
129.80	277.0
130.70	136.0
134.70	158.0
136.80	136.0
140.80	822.0
142.80	1012.0
145.00	130.0
145.70	126.0
147.70	221.0
154.70	164.0
156.80	178.0
158.70	138.0
160.80	100.0
171.80	546.0
172.90	646.0
173.80	57576.0
174.80	3983.0
175.80	55928.0
176.80	3854.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.90	723.0
36.90	4164.0
38.00	3550.0
39.00	1344.0
39.90	178.0
43.90	676.0
44.90	654.0
45.90	114.0
46.90	963.0
47.90	597.0
48.90	3353.0
49.90	15226.0
51.00	4771.0
51.90	214.0
54.80	264.0
55.90	1245.0
56.90	2368.0
57.90	127.0
59.90	778.0
60.90	4098.0
62.00	4235.0
63.00	3285.0
63.90	434.0
65.00	439.0
67.00	192.0
67.90	8784.0
68.90	8503.0
69.90	801.0
71.90	425.0
72.90	3809.0
73.90	14564.0
74.90	43048.0
75.90	3736.0
76.80	644.0
77.90	346.0
78.80	3003.0
79.80	910.0
80.90	3158.0
81.80	657.0
86.10	141.0
86.90	3335.0
87.90	3341.0
90.80	375.0
91.90	2624.0
92.90	3484.0
93.90	9927.0
94.90	79672.0
95.90	5341.0
97.00	175.0
103.80	479.0
104.80	137.0
105.70	315.0
114.70	137.0
115.80	310.0
116.80	494.0
117.80	346.0
118.80	599.0
127.80	250.0
128.70	157.0
129.80	281.0
130.70	114.0
134.70	165.0
136.80	142.0
140.80	815.0
141.70	104.0
142.80	1045.0
144.90	149.0
145.80	119.0
147.70	267.0
154.80	180.0
156.80	184.0
158.70	130.0
160.70	107.0
171.80	532.0
172.90	709.0
173.80	60304.0
174.90	4233.0
175.80	58680.0
176.80	3830.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.90	691.0
36.90	3768.0
37.90	3378.0
39.00	1184.0
39.90	184.0
43.90	585.0
44.90	609.0
45.90	104.0
46.90	898.0
47.90	499.0
48.90	2990.0
49.90	14152.0
50.90	4293.0
51.90	186.0
54.80	242.0
55.90	1203.0
56.90	2268.0
57.80	100.0
59.90	676.0
60.90	3754.0
62.00	3928.0
63.00	3011.0
63.90	407.0
65.00	414.0
66.90	192.0
67.90	8000.0
68.90	8083.0
69.90	702.0
71.90	400.0
72.90	3742.0
73.90	13376.0
74.90	39984.0
75.90	3412.0
76.80	563.0
77.80	338.0
78.80	3016.0
79.80	814.0
80.80	2974.0
81.80	661.0
86.90	3162.0
87.90	3041.0
90.80	358.0
91.90	2487.0
92.90	3267.0
93.90	9387.0
94.90	74728.0
95.90	4916.0
97.00	135.0
103.80	520.0
104.80	128.0
105.70	329.0
114.70	124.0
115.80	308.0
116.80	474.0
117.80	297.0
118.80	510.0
127.80	263.0
128.80	164.0
129.80	280.0
134.80	148.0
136.70	139.0
140.80	744.0
141.70	121.0
142.80	986.0
144.80	163.0
145.80	101.0
147.70	239.0
154.80	171.0
156.80	172.0
158.70	103.0
160.70	100.0
171.80	460.0
172.90	685.0
173.80	57552.0
174.90	4060.0
175.80	55456.0
176.80	3438.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128