

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030343.D
 Acq On : 23 Mar 2019 16:30
 Operator : JC/SP
 Sample : VU0323WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	41	rVB	16391	16885	0.97%	0.121%
2	1.399	89	96	110	rBV	248758	253751	14.62%	1.816%
3	1.678	176	183	194	rBV	191703	233481	13.46%	1.671%
4	2.270	357	367	380	rBV	392005	594446	34.26%	4.254%
5	2.479	426	432	438	rVB4	2937	3575	0.21%	0.026%
6	2.534	445	449	452	rBV	1637	1247	0.07%	0.009%
7	2.595	465	468	471	rVB	1796	1202	0.07%	0.009%
8	2.617	471	475	478	rBV2	1535	1094	0.06%	0.008%
9	2.653	478	486	488	rBV	1500	1950	0.11%	0.014%
10	2.694	495	499	502	rBV3	1480	1416	0.08%	0.010%
11	2.942	573	576	583	rBV	978	1260	0.07%	0.009%
12	2.977	583	587	592	rBV2	1396	1644	0.09%	0.012%
13	3.045	602	608	611	rBV	1830	2225	0.13%	0.016%
14	3.315	688	692	698	rBV	2274	2686	0.15%	0.019%
15	3.444	728	732	738	rVB2	1757	1898	0.11%	0.014%
16	3.945	885	888	895	rVB	2047	1837	0.11%	0.013%
17	3.997	900	904	907	rVB	2182	1785	0.10%	0.013%
18	4.032	907	915	918	rBV	1367	1841	0.11%	0.013%
19	4.061	918	924	926	rBV	1145	1333	0.08%	0.010%
20	4.170	946	958	989	rBV	181536	481371	27.74%	3.445%
21	4.643	1090	1105	1125	rBV	272914	649547	37.43%	4.648%
22	4.961	1201	1204	1207	rBV	1820	1369	0.08%	0.010%
23	5.016	1218	1221	1225	rBV	1344	1033	0.06%	0.007%
24	5.042	1226	1229	1235	rVB	1061	1116	0.06%	0.008%
25	5.083	1235	1242	1244	rBV	1513	1356	0.08%	0.010%
26	5.151	1258	1263	1269	rBV	1459	1465	0.08%	0.010%
27	5.337	1298	1321	1349	rBV2	580945	1735234	100.00%	12.418%
28	5.662	1417	1422	1423	rBV2	1408	1039	0.06%	0.007%
29	5.884	1476	1491	1526	rBV	546427	1121649	64.64%	8.027%
30	6.116	1558	1563	1566	rBV2	1356	1313	0.08%	0.009%
31	6.328	1615	1629	1659	rVV	386650	797404	45.95%	5.706%
32	6.492	1676	1680	1684	rBV	1286	1149	0.07%	0.008%
33	6.604	1711	1715	1721	rVB	1720	1931	0.11%	0.014%
34	6.669	1731	1735	1738	rBV	1911	1554	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030343.D
 Acq On : 23 Mar 2019 16:30
 Operator : JC/SP
 Sample : VU0323WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.688	1738	1741	1744	rVV	1400	1040	0.06%	0.007%
36	6.820	1778	1782	1789	rBV	2121	2886	0.17%	0.021%
37	6.903	1804	1808	1811	rBV	1715	1415	0.08%	0.010%
38	6.977	1825	1831	1836	rBV	1323	1791	0.10%	0.013%
39	7.154	1881	1886	1891	rBV2	1787	2084	0.12%	0.015%
40	7.225	1897	1908	1937	rBV	218905	408828	23.56%	2.926%
41	7.344	1941	1945	1955	rVB	2181	2915	0.17%	0.021%
42	7.466	1977	1983	1987	rBV4	2811	3794	0.22%	0.027%
43	7.562	2000	2013	2047	rBV	761178	1382750	79.69%	9.895%
44	7.733	2063	2066	2069	rBV	1756	1150	0.07%	0.008%
45	7.807	2086	2089	2092	rBV	1613	1114	0.06%	0.008%
46	7.845	2092	2101	2119	rBV	150654	271098	15.62%	1.940%
47	8.148	2192	2195	2199	rVV	959	1025	0.06%	0.007%
48	8.308	2234	2245	2280	rBV	589909	1128797	65.05%	8.078%
49	8.627	2341	2344	2348	rBV	1610	1255	0.07%	0.009%
50	8.804	2396	2399	2405	rVB	1892	1793	0.10%	0.013%
51	8.849	2410	2413	2419	rVB	1441	1211	0.07%	0.009%
52	8.884	2419	2424	2427	rBV2	1410	1481	0.09%	0.011%
53	8.932	2436	2439	2442	rBV	1932	1410	0.08%	0.010%
54	8.987	2452	2456	2460	rVB2	1572	1440	0.08%	0.010%
55	9.086	2475	2487	2511	rBV	814165	1380847	79.58%	9.882%
56	9.328	2559	2562	2566	rVV	1429	1179	0.07%	0.008%
57	9.543	2624	2629	2632	rBV	1813	2400	0.14%	0.017%
58	9.614	2647	2651	2653	rBV	1677	1184	0.07%	0.008%
59	9.675	2666	2670	2675	rBV	1549	1765	0.10%	0.013%
60	9.733	2682	2688	2690	rBV	1306	1256	0.07%	0.009%
61	9.913	2742	2744	2748	rVB	1556	1071	0.06%	0.008%
62	9.990	2765	2768	2770	rBV	1550	1132	0.07%	0.008%
63	10.170	2819	2824	2828	rBV2	2084	2493	0.14%	0.018%
64	10.286	2857	2860	2863	rBV	1415	1107	0.06%	0.008%
65	10.427	2892	2904	2922	rVV	525919	839882	48.40%	6.010%
66	10.630	2965	2967	2974	rVB	1540	1417	0.08%	0.010%
67	10.797	3014	3019	3023	rVB	1753	1657	0.10%	0.012%
68	10.823	3023	3027	3032	rBV	1268	1388	0.08%	0.010%
69	10.877	3038	3044	3048	rVB	1716	1926	0.11%	0.014%
70	10.919	3048	3057	3059	rBV2	1557	2078	0.12%	0.015%
71	10.932	3059	3061	3068	rVB2	2295	1532	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030343.D
 Acq On : 23 Mar 2019 16:30
 Operator : JC/SP
 Sample : VU0323WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.964	3068	3071	3075	rBV	1081	1046	0.06%	0.007%
73	11.186	3136	3140	3142	rBV	1502	1008	0.06%	0.007%
74	11.218	3142	3150	3155	rVV	1884	2797	0.16%	0.020%
75	11.257	3158	3162	3165	rVV2	1470	1367	0.08%	0.010%
76	11.305	3173	3177	3182	rBV	1905	1902	0.11%	0.014%
77	11.424	3204	3214	3219	rBV6	4032	6281	0.36%	0.045%
78	11.482	3220	3232	3258	rBV	799987	1298767	74.85%	9.294%
79	11.858	3333	3349	3372	rBV	715345	1204258	69.40%	8.618%
80	12.202	3453	3456	3461	rVB	2261	1931	0.11%	0.014%
81	12.231	3461	3465	3469	rVB	2192	1762	0.10%	0.013%
82	12.257	3469	3473	3476	rBV	2469	2320	0.13%	0.017%
83	12.369	3505	3508	3512	rVB	2124	1414	0.08%	0.010%
84	12.633	3587	3590	3595	rBV2	1500	1084	0.06%	0.008%
85	12.713	3610	3615	3624	rVB	2321	3637	0.21%	0.026%
86	12.755	3624	3628	3634	rBV3	1673	1781	0.10%	0.013%
87	12.823	3644	3649	3655	rVB	2383	2681	0.15%	0.019%
88	12.861	3655	3661	3667	rBV	2364	3173	0.18%	0.023%
89	12.893	3667	3671	3675	rBV3	3493	3938	0.23%	0.028%
90	13.009	3704	3707	3709	rBV	1886	1152	0.07%	0.008%
91	13.414	3827	3833	3836	rBV	1738	1980	0.11%	0.014%
92	13.626	3897	3899	3904	rBV2	1186	1053	0.06%	0.008%
93	13.762	3931	3941	3945	rBV4	9104	17466	1.01%	0.125%
94	13.996	4005	4014	4020	rBV5	6176	11381	0.66%	0.081%
95	14.080	4037	4040	4044	rBV2	1465	1480	0.09%	0.011%
96	14.167	4061	4067	4070	rBV3	1772	2055	0.12%	0.015%
97	14.183	4070	4072	4078	rVB	1597	1467	0.08%	0.010%
98	14.668	4214	4223	4227	rBV2	2490	4159	0.24%	0.030%
99	15.134	4365	4368	4372	rBV	1837	1338	0.08%	0.010%
100	15.311	4420	4423	4427	rVB	1825	1352	0.08%	0.010%


Sum of corrected areas: 13973707

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032319\
Data File : VU030343.D
Acq On : 23 Mar 2019 16:30
Operator : JC/SP
Sample : VU0323WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

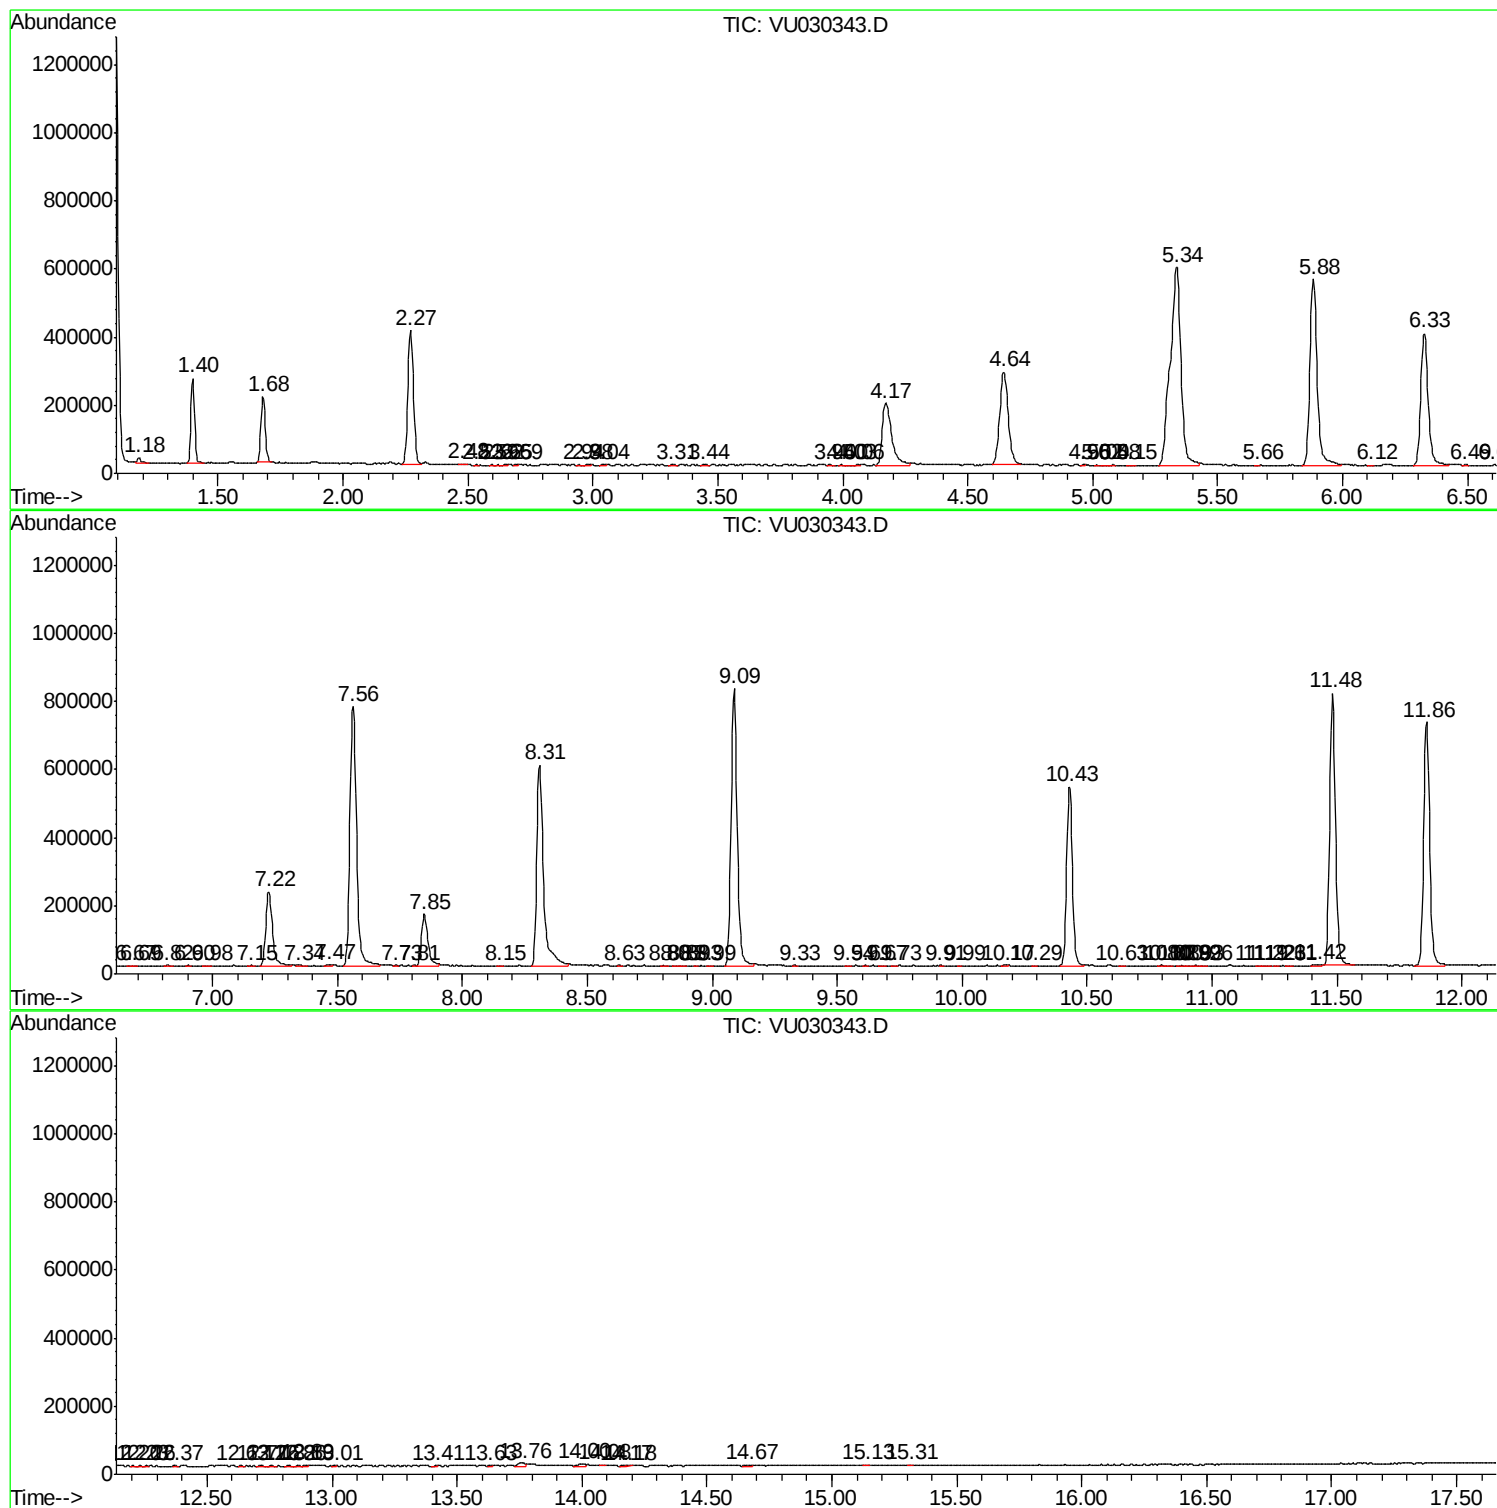

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032319\
Data File : VU030343.D
Acq On : 23 Mar 2019 16:30
Operator : JC/SP
Sample : VU0323WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032319\
Data File : VU030343.D
Acq On : 23 Mar 2019 16:30
Operator : JC/SP
Sample : VU0323WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc