

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030350.D
 Acq On : 23 Mar 2019 19:13
 Operator : JC/SP
 Sample : K2083-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB2	13725	14438	0.85%	0.110%
2	1.399	89	96	108	rVB	239497	238920	14.12%	1.813%
3	1.682	176	184	197	rVB	174008	221103	13.07%	1.678%
4	2.270	356	367	381	rBV	369070	569760	33.67%	4.324%
5	2.444	417	421	422	rBV	1762	1411	0.08%	0.011%
6	2.498	436	438	443	rVB	1388	889	0.05%	0.007%
7	2.640	479	482	485	rVB	1237	875	0.05%	0.007%
8	2.669	485	491	493	rBV2	1210	1041	0.06%	0.008%
9	2.688	493	497	498	rBV	1922	1174	0.07%	0.009%
10	2.739	510	513	519	rVB2	1379	1473	0.09%	0.011%
11	2.775	519	524	526	rBV	1005	1075	0.06%	0.008%
12	2.829	537	541	545	rVB	1806	1194	0.07%	0.009%
13	2.865	545	552	557	rBV	1509	2023	0.12%	0.015%
14	2.965	576	583	587	rBV	1765	2406	0.14%	0.018%
15	3.116	627	630	634	rVB	1385	1141	0.07%	0.009%
16	3.138	634	637	641	rBV	1019	1084	0.06%	0.008%
17	3.161	641	644	648	rVB	1764	1577	0.09%	0.012%
18	3.190	648	653	660	rBV	2365	3626	0.21%	0.028%
19	3.537	758	761	766	rBV2	1211	1315	0.08%	0.010%
20	3.588	771	777	785	rVB	1613	2491	0.15%	0.019%
21	3.640	789	793	796	rBV2	1456	1202	0.07%	0.009%
22	3.733	819	822	827	rBV	1589	1851	0.11%	0.014%
23	3.817	846	848	854	rVB	1396	1091	0.06%	0.008%
24	3.855	856	860	867	rBV2	1929	2284	0.13%	0.017%
25	3.952	885	890	895	rBV	1650	2252	0.13%	0.017%
26	4.109	933	939	942	rVB	913	891	0.05%	0.007%
27	4.132	942	946	948	rBV	1597	1300	0.08%	0.010%
28	4.177	948	960	1004	rVV	169054	497271	29.39%	3.774%
29	4.379	1020	1023	1031	rVB3	2851	2658	0.16%	0.020%
30	4.566	1078	1081	1089	rVV	1043	1185	0.07%	0.009%
31	4.646	1089	1106	1130	rBV	266507	642627	37.98%	4.877%
32	4.990	1211	1213	1217	rBV	1344	984	0.06%	0.007%
33	5.337	1297	1321	1356	rBV2	567117	1691945	100.00%	12.842%
34	5.627	1408	1411	1414	rBV	1889	1420	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030350.D
 Acq On : 23 Mar 2019 19:13
 Operator : JC/SP
 Sample : K2083-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.781	1456	1459	1466	rVB	1773	1765	0.10%	0.013%
36	5.816	1466	1470	1474	rBV	1535	1532	0.09%	0.012%
37	5.884	1477	1491	1534	rBV	512864	1054618	62.33%	8.004%
38	6.193	1577	1587	1595	rBV6	5708	11677	0.69%	0.089%
39	6.328	1616	1629	1661	rBV2	381455	781983	46.22%	5.935%
40	6.530	1690	1692	1695	rVB	1699	911	0.05%	0.007%
41	6.710	1745	1748	1753	rVB	1126	1091	0.06%	0.008%
42	6.791	1767	1773	1777	rBV	1131	1736	0.10%	0.013%
43	6.881	1799	1801	1807	rVB	1502	1228	0.07%	0.009%
44	6.913	1807	1811	1813	rBV	1518	1142	0.07%	0.009%
45	6.955	1818	1824	1827	rBV2	1801	2196	0.13%	0.017%
46	7.090	1862	1866	1869	rBV	1020	995	0.06%	0.008%
47	7.122	1873	1876	1879	rVB	1220	880	0.05%	0.007%
48	7.144	1879	1883	1888	rBV	1776	1971	0.12%	0.015%
49	7.170	1888	1891	1895	rVB	1309	1085	0.06%	0.008%
50	7.225	1895	1908	1930	rBV	208156	389691	23.03%	2.958%
51	7.427	1961	1971	1974	rBV2	2600	3848	0.23%	0.029%
52	7.562	1998	2013	2040	rBV	726803	1313419	77.63%	9.969%
53	7.849	2090	2102	2124	rBV	139498	261513	15.46%	1.985%
54	8.077	2167	2173	2177	rVV	1686	1828	0.11%	0.014%
55	8.141	2188	2193	2198	rBV	810	1166	0.07%	0.009%
56	8.177	2200	2204	2209	rBV3	1597	1807	0.11%	0.014%
57	8.225	2213	2219	2221	rBV3	2378	2505	0.15%	0.019%
58	8.308	2234	2245	2281	rBV	556737	1050867	62.11%	7.976%
59	8.578	2325	2329	2334	rBV2	1565	1707	0.10%	0.013%
60	8.810	2397	2401	2403	rBV	1224	916	0.05%	0.007%
61	8.913	2430	2433	2441	rBV	2323	2998	0.18%	0.023%
62	8.980	2450	2454	2457	rBV	1661	1436	0.08%	0.011%
63	9.086	2474	2487	2512	rBV	763105	1280354	75.67%	9.718%
64	9.260	2539	2541	2544	rBV	1556	1140	0.07%	0.009%
65	9.357	2567	2571	2574	rBV	1161	1027	0.06%	0.008%
66	9.392	2576	2582	2585	rVV2	957	1141	0.07%	0.009%
67	9.469	2602	2606	2612	rBV	1758	2427	0.14%	0.018%
68	9.717	2679	2683	2686	rVV	1122	1044	0.06%	0.008%
69	9.816	2712	2714	2718	rVB	1897	1367	0.08%	0.010%
70	9.942	2747	2753	2756	rBV	2388	2898	0.17%	0.022%
71	10.080	2793	2796	2801	rBV	1686	1461	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032319\
 Data File : VU030350.D
 Acq On : 23 Mar 2019 19:13
 Operator : JC/SP
 Sample : K2083-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.164	2817	2822	2826	rBV2	1569	1988	0.12%	0.015%
73	10.234	2840	2844	2846	rBV	1494	1042	0.06%	0.008%
74	10.254	2846	2850	2855	rVV	1439	1725	0.10%	0.013%
75	10.302	2861	2865	2868	rBV2	1322	1046	0.06%	0.008%
76	10.357	2879	2882	2884	rBV2	1756	1189	0.07%	0.009%
77	10.427	2892	2904	2926	rBV	505551	822599	48.62%	6.243%
78	10.537	2934	2938	2942	rBV	1450	1420	0.08%	0.011%
79	10.594	2952	2956	2957	rBV2	1609	1138	0.07%	0.009%
80	10.639	2967	2970	2973	rBV	2046	1525	0.09%	0.012%
81	10.691	2982	2986	2989	rBV2	1438	1232	0.07%	0.009%
82	10.746	3000	3003	3006	rBV	1685	1063	0.06%	0.008%
83	10.848	3032	3035	3041	rVB	1303	1163	0.07%	0.009%
84	10.964	3067	3071	3072	rBV	1565	1087	0.06%	0.008%
85	11.035	3086	3093	3097	rBV	2549	3668	0.22%	0.028%
86	11.180	3134	3138	3140	rBV	1128	916	0.05%	0.007%
87	11.389	3199	3203	3205	rBV	1245	1074	0.06%	0.008%
88	11.482	3220	3232	3255	rBV	685646	1130132	66.79%	8.577%
89	11.726	3306	3308	3315	rVB2	1921	1381	0.08%	0.010%
90	11.858	3337	3349	3369	rBV	654110	1076593	63.63%	8.171%
91	12.292	3481	3484	3487	rBV	1468	1168	0.07%	0.009%
92	12.446	3529	3532	3536	rBV	1857	1642	0.10%	0.012%
93	12.694	3605	3609	3614	rBV	2096	1950	0.12%	0.015%
94	12.771	3629	3633	3638	rBV	2763	2511	0.15%	0.019%
95	12.839	3651	3654	3657	rBV	1044	875	0.05%	0.007%
96	14.543	4181	4184	4187	rBV	1811	1420	0.08%	0.011%
97	14.909	4295	4298	4303	rVB	1469	1150	0.07%	0.009%
98	14.935	4303	4306	4310	rBV	1599	1150	0.07%	0.009%
99	15.099	4355	4357	4360	rBV	1388	1013	0.06%	0.008%
100	15.237	4397	4400	4402	rBV	1913	1379	0.08%	0.010%


Sum of corrected areas: 13175586

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032319\
Data File : VU030350.D
Acq On : 23 Mar 2019 19:13
Operator : JC/SP
Sample : K2083-05 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

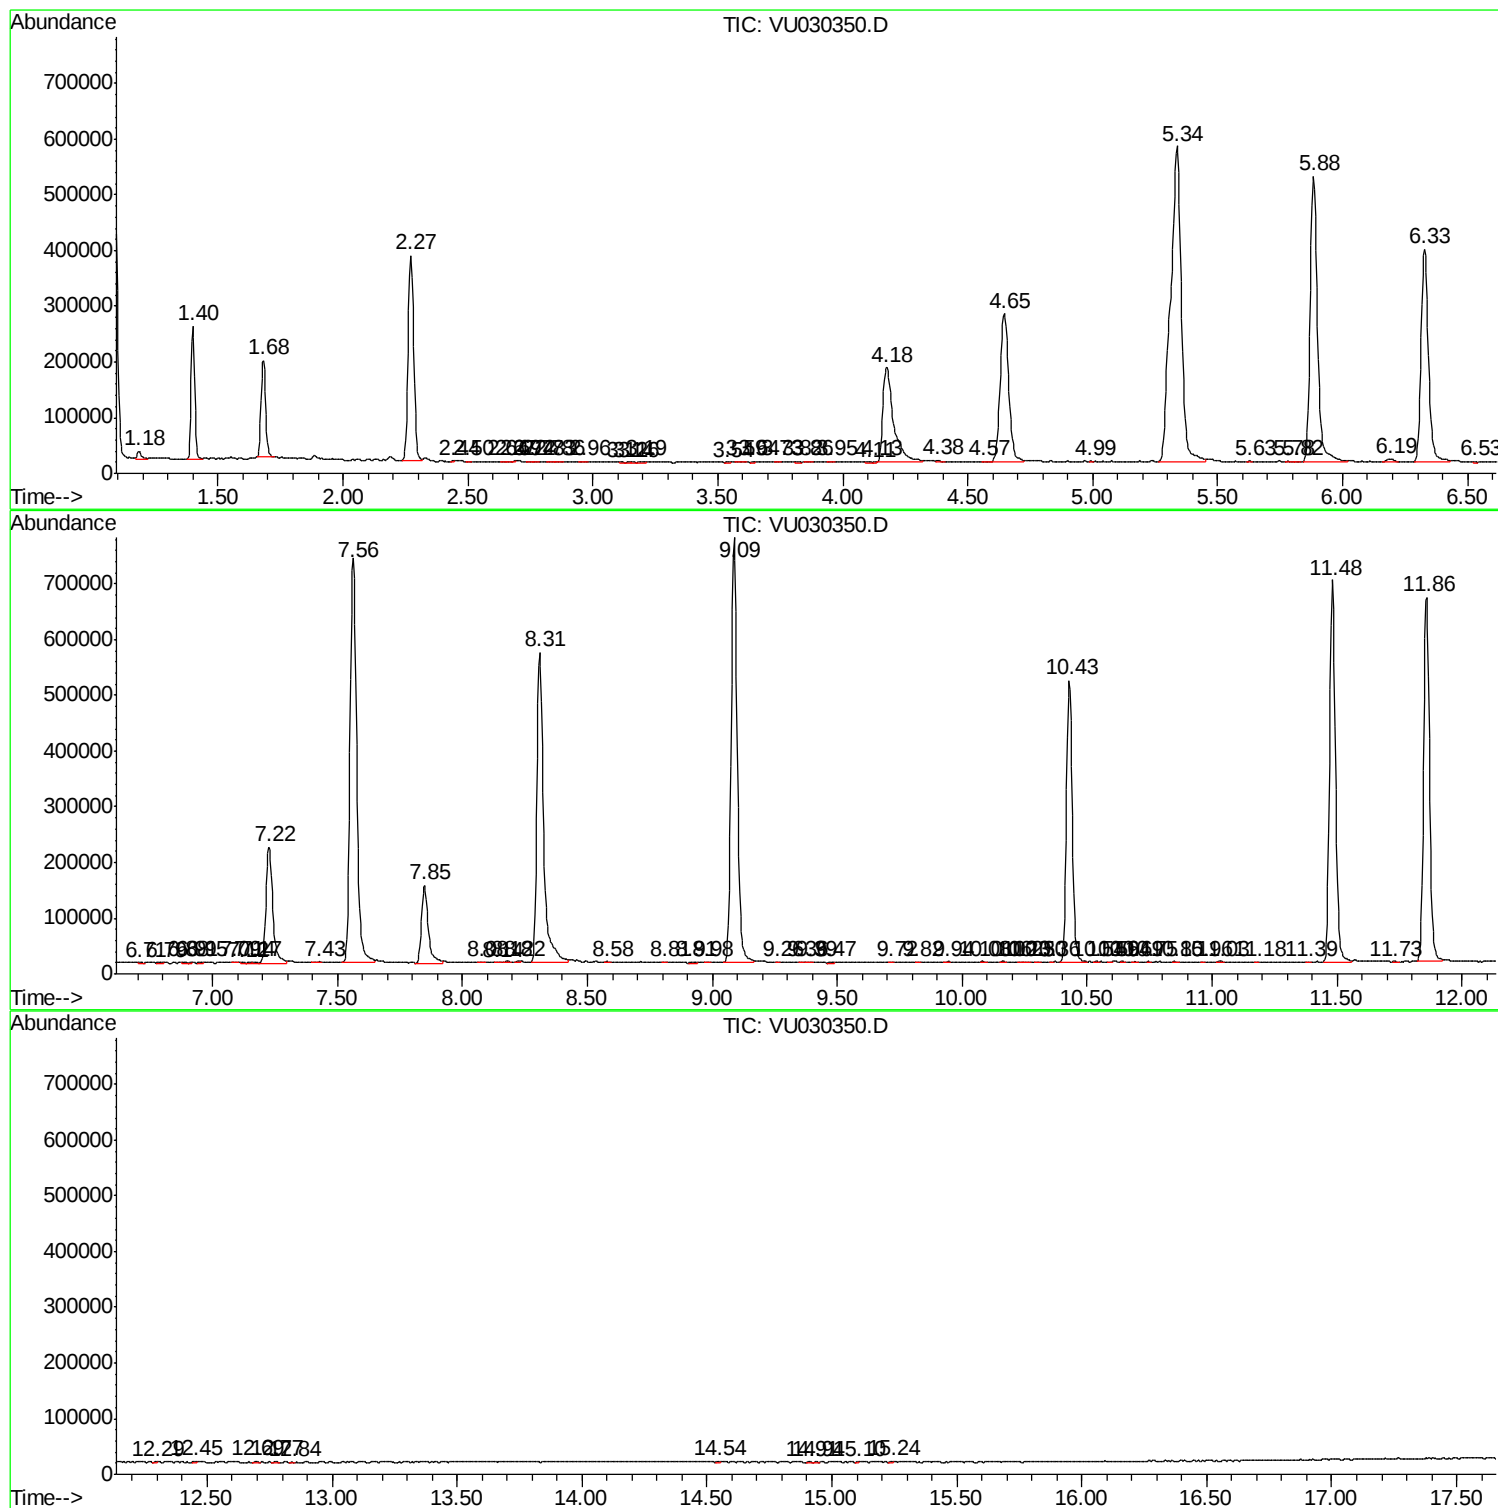

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032319\
Data File : VU030350.D
Acq On : 23 Mar 2019 19:13
Operator : JC/SP
Sample : K2083-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU032319\
Data File : VU030350.D
Acq On : 23 Mar 2019 19:13
Operator : JC/SP
Sample : K2083-05 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
BF1A3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc