


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032319\
 Data File : VU030335.D
 Acq On : 23 Mar 2019 12:08
 Operator : JC/SP
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 25 05:48:44 2019

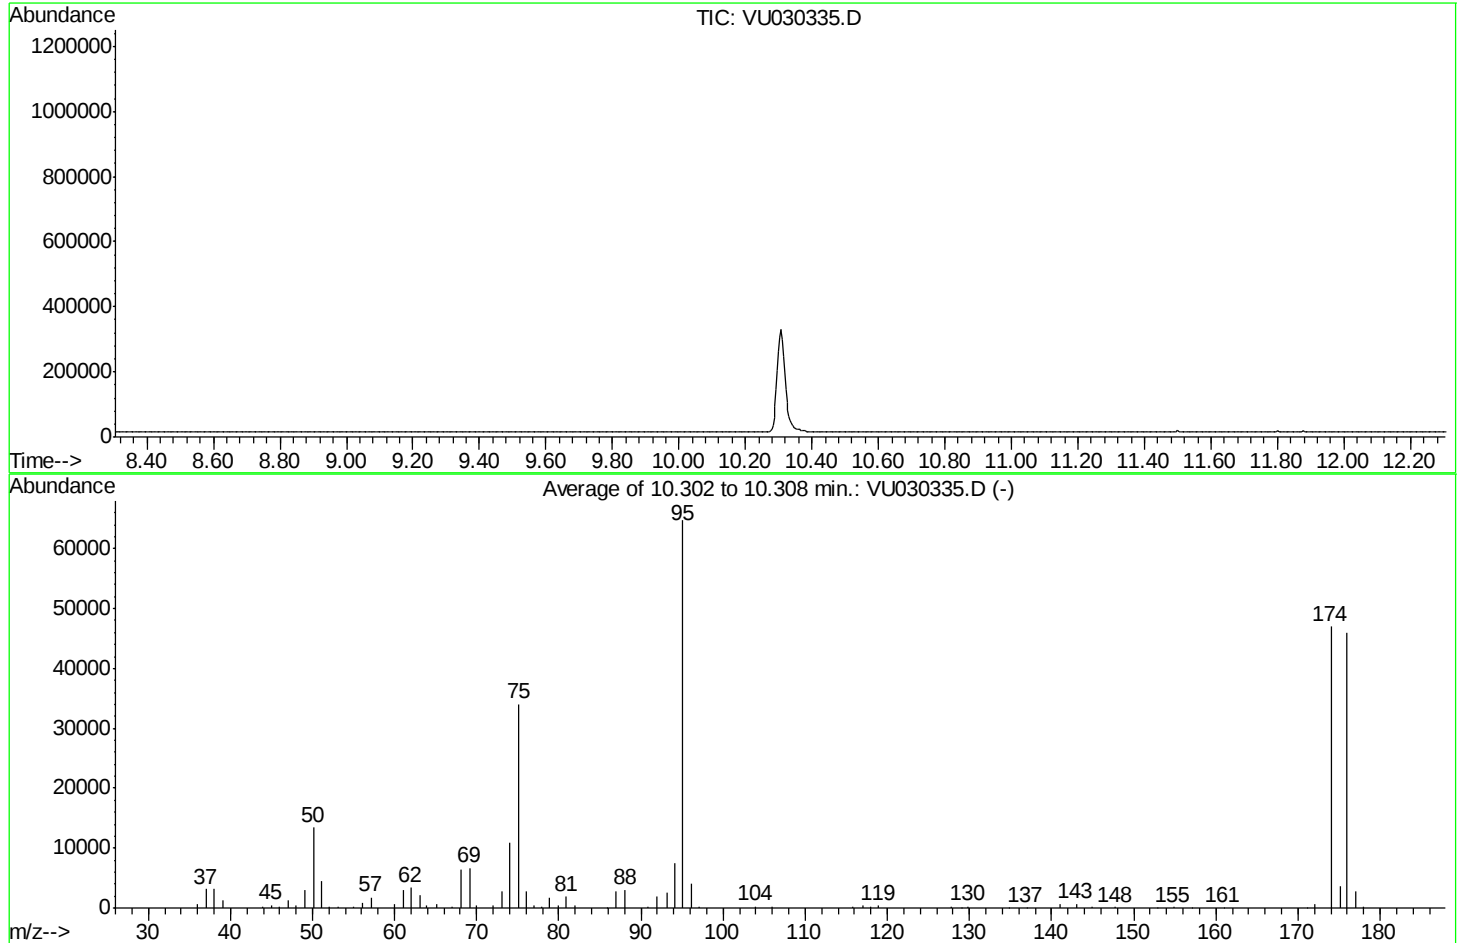

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	13380	PASS
75	95	30	80	52.6	34016	PASS
95	95	100	100	100.0	64730	PASS
96	95	5	9	6.4	4151	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.5	46946	PASS
175	174	5	9	7.6	3549	PASS
176	174	95	101	98.1	46056	PASS
177	176	5	9	6.0	2755	PASS

Scan 2854 (10.266 min): VU030335.D
BFB41

m/z	Abundance
40.00	16456.0
44.00	599.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	708.0
37.10	3125.0
38.10	3073.0
39.10	1251.0
40.00	15399.0
43.90	934.0
45.00	509.0
46.00	114.0
47.10	1172.0
48.10	294.0
49.10	2953.0
50.10	13141.0
51.00	4349.0
52.00	200.0
53.10	206.0
55.00	218.0
56.10	905.0
57.10	1733.0
60.00	574.0
61.00	2853.0
62.00	3092.0
63.10	2160.0
63.90	440.0
65.10	555.0
67.00	246.0
68.10	6343.0
69.10	6381.0
70.00	514.0
72.10	445.0
73.10	2793.0
74.00	10354.0
75.10	32608.0
76.10	2645.0
77.00	460.0
77.90	334.0
78.90	1564.0
79.90	456.0
80.90	1884.0
82.00	354.0
87.00	2620.0
88.10	2927.0
90.90	176.0
92.00	1929.0
93.10	2551.0
94.10	7020.0
95.10	62120.0
96.10	4200.0
97.00	200.0
104.00	261.0
106.00	211.0
115.90	268.0
116.90	318.0
117.90	147.0
118.90	314.0
127.80	232.0
129.90	219.0
141.00	619.0
143.00	705.0
144.90	150.0
147.80	163.0
154.90	128.0
157.10	107.0
161.00	110.0
171.10	130.0
172.00	608.0
174.00	44104.0
175.10	3293.0
176.00	42176.0
177.00	2417.0
177.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	696.0
37.00	3275.0
38.10	3226.0
39.10	1246.0
40.00	15415.0
44.00	883.0
45.00	531.0
46.00	144.0
47.10	1317.0
48.10	337.0
49.10	3135.0
50.10	13869.0
51.10	4669.0
52.10	200.0
53.20	192.0
55.00	272.0
56.10	856.0
57.10	1723.0
60.00	557.0
61.00	3086.0
62.00	3562.0
63.10	2275.0
63.90	414.0
65.10	632.0
67.00	220.0
68.00	6550.0
69.10	6890.0
70.00	526.0
72.00	416.0
73.10	2864.0
74.10	11273.0
75.10	35104.0
76.10	2869.0
77.00	466.0
77.90	311.0
78.90	1677.0
79.90	472.0
80.90	2005.0
82.00	417.0
87.00	2732.0
88.10	3125.0
90.80	223.0
92.00	2142.0
93.10	2719.0
94.10	7640.0
95.10	66736.0
96.10	4211.0
97.00	154.0
103.90	230.0
105.90	207.0
115.80	306.0
117.00	356.0
118.00	184.0
118.90	389.0
127.80	208.0
129.00	103.0
129.90	262.0
134.70	113.0
136.90	104.0
141.00	647.0
143.00	770.0
144.90	176.0
147.70	189.0
152.90	108.0
154.90	143.0
157.10	121.0
161.00	114.0
172.00	680.0
174.00	48320.0
175.10	3627.0
176.00	47432.0
177.00	2810.0
178.00	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	632.0
37.00	3105.0
38.00	3136.0
39.10	1140.0
40.00	15561.0
44.00	925.0
45.00	533.0
46.00	171.0
47.10	1285.0
48.00	376.0
49.10	3027.0
50.10	13132.0
51.10	4501.0
52.10	157.0
53.20	108.0
54.90	252.0
56.00	780.0
57.10	1747.0
60.00	522.0
61.00	3139.0
62.00	3576.0
63.10	2248.0
63.90	369.0
65.10	602.0
67.00	194.0
68.10	6295.0
69.10	6810.0
70.00	455.0
71.90	349.0
73.00	2836.0
74.10	11235.0
75.10	34336.0
76.10	2984.0
77.00	473.0
77.80	261.0
78.90	1638.0
80.00	490.0
80.90	1836.0
82.00	418.0
85.90	101.0
86.90	2707.0
88.10	3039.0
90.80	275.0
92.00	1980.0
93.10	2698.0
94.10	7517.0
95.10	65336.0
96.10	4043.0
103.90	197.0
105.90	194.0
115.90	271.0
117.00	369.0
118.00	235.0
118.90	376.0
127.80	194.0
129.00	121.0
129.80	254.0
134.80	140.0
136.90	157.0
141.00	594.0
143.00	677.0
144.90	174.0
147.70	188.0
154.90	141.0
160.90	114.0
172.00	645.0
174.00	48416.0
175.10	3727.0
176.00	48560.0
177.00	3039.0
178.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41