

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030370.D
 Acq On : 24 Mar 2019 15:02
 Operator : JC/SP
 Sample : K2016-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0981

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	90	96	106	rBV	223810	235685	14.83%	1.857%
2	2.270	357	367	378	rBV	331823	503904	31.70%	3.971%
3	2.447	415	422	436	rBV	24742	40500	2.55%	0.319%
4	3.576	765	773	775	rBV	2217	2675	0.17%	0.021%
5	3.704	809	813	817	rVB	1264	1189	0.07%	0.009%
6	3.727	817	820	823	rBV	1402	872	0.05%	0.007%
7	3.785	835	838	841	rBV	1507	1141	0.07%	0.009%
8	3.939	882	886	890	rBV2	1254	1584	0.10%	0.012%
9	3.987	898	901	903	rBV	1019	609	0.04%	0.005%
10	4.003	903	906	912	rVB	1412	1218	0.08%	0.010%
11	4.032	912	915	917	rBV2	816	470	0.03%	0.004%
12	4.058	920	923	927	rBV2	1095	1069	0.07%	0.008%
13	4.125	941	944	947	rBV	936	735	0.05%	0.006%
14	4.177	948	960	989	rBV2	172407	496263	31.22%	3.910%
15	4.643	1092	1105	1125	rBV	247201	576470	36.27%	4.542%
16	4.926	1191	1193	1200	rVB2	1680	1363	0.09%	0.011%
17	4.993	1210	1214	1217	rBV	1357	1257	0.08%	0.010%
18	5.058	1229	1234	1238	rVB	1538	1471	0.09%	0.012%
19	5.077	1238	1240	1242	rBV	897	412	0.03%	0.003%
20	5.145	1257	1261	1263	rBV	1004	890	0.06%	0.007%
21	5.196	1274	1277	1283	rVB	1875	1555	0.10%	0.012%
22	5.222	1283	1285	1287	rBV2	657	352	0.02%	0.003%
23	5.338	1297	1321	1350	rBV2	528550	1589449	100.00%	12.524%
24	5.884	1478	1491	1513	rBV	470867	946536	59.55%	7.458%
25	6.328	1616	1629	1649	rBV	351519	719000	45.24%	5.665%
26	6.723	1745	1752	1755	rBV	1950	2644	0.17%	0.021%
27	6.775	1762	1768	1773	rVB	2093	2570	0.16%	0.020%
28	6.807	1773	1778	1781	rBV	1406	1700	0.11%	0.013%
29	6.878	1796	1800	1801	rBV	1491	1071	0.07%	0.008%
30	7.180	1892	1894	1896	rBV	268	106	0.01%	0.001%
31	7.225	1896	1908	1927	rBV	177685	327398	20.60%	2.580%
32	7.460	1976	1981	1983	rBV	1703	1578	0.10%	0.012%
33	7.563	2000	2013	2025	rBV	661008	1169405	73.57%	9.214%
34	7.633	2027	2035	2058	rVB	438581	795654	50.06%	6.269%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030370.D
 Acq On : 24 Mar 2019 15:02
 Operator : JC/SP
 Sample : K2016-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0981

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	7.849	2092	2102	2124	rBV	121083	215677	13.57%	1.699%
36	8.180	2196	2205	2209	rBV4	3386	5423	0.34%	0.043%
37	8.308	2232	2245	2281	rBV	505744	948967	59.70%	7.477%
38	8.627	2342	2344	2347	rBV	826	492	0.03%	0.004%
39	8.665	2353	2356	2358	rBV	740	399	0.03%	0.003%
40	8.788	2387	2394	2398	rBV	2061	2511	0.16%	0.020%
41	8.823	2402	2405	2407	rBV2	1008	670	0.04%	0.005%
42	8.868	2414	2419	2423	rBV	1420	1689	0.11%	0.013%
43	8.942	2437	2442	2446	rBV	1159	1343	0.08%	0.011%
44	8.997	2457	2459	2460	rBV	469	229	0.01%	0.002%
45	9.013	2460	2464	2468	rVB	1343	1111	0.07%	0.009%
46	9.038	2468	2472	2475	rBV	1317	1226	0.08%	0.010%
47	9.087	2475	2487	2490	rBV	724481	1044521	65.72%	8.230%
48	9.421	2587	2591	2598	rVB2	1607	2204	0.14%	0.017%
49	9.453	2598	2601	2603	rBV	811	375	0.02%	0.003%
50	9.476	2603	2608	2610	rBV	964	689	0.04%	0.005%
51	9.501	2610	2616	2619	rBV	1186	1248	0.08%	0.010%
52	9.550	2628	2631	2635	rVB	890	654	0.04%	0.005%
53	9.575	2635	2639	2641	rBV2	839	648	0.04%	0.005%
54	9.759	2694	2696	2697	rBV	381	193	0.01%	0.002%
55	9.778	2698	2702	2705	rVV2	1866	1501	0.09%	0.012%
56	9.932	2743	2750	2753	rBV2	1889	2016	0.13%	0.016%
57	9.951	2753	2756	2758	rBV	606	429	0.03%	0.003%
58	10.013	2772	2775	2778	rBV	1109	815	0.05%	0.006%
59	10.202	2829	2834	2840	rVB	1300	1141	0.07%	0.009%
60	10.228	2840	2842	2844	rBV	510	241	0.02%	0.002%
61	10.244	2844	2847	2849	rBV2	768	479	0.03%	0.004%
62	10.366	2877	2885	2887	rBV	2189	2621	0.16%	0.021%
63	10.427	2892	2904	2921	rVV	463006	757702	47.67%	5.970%
64	10.643	2968	2971	2973	rBV	1170	758	0.05%	0.006%
65	10.701	2985	2989	2992	rBV	1296	1100	0.07%	0.009%
66	10.881	3038	3045	3050	rBV	1766	2491	0.16%	0.020%
67	10.942	3061	3064	3068	rBV2	1163	922	0.06%	0.007%
68	11.019	3085	3088	3090	rBV	1393	1134	0.07%	0.009%
69	11.067	3098	3103	3105	rBV	1445	1105	0.07%	0.009%
70	11.122	3116	3120	3122	rBV	1800	1449	0.09%	0.011%
71	11.218	3146	3150	3154	rBV	1773	1860	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030370.D
 Acq On : 24 Mar 2019 15:02
 Operator : JC/SP
 Sample : K2016-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0981

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.292	3169	3173	3175	rVB2	1458	852	0.05%	0.007%
73	11.308	3175	3178	3181	rBV	673	413	0.03%	0.003%
74	11.337	3181	3187	3193	rBV	1234	1790	0.11%	0.014%
75	11.373	3193	3198	3202	rBV	1428	1715	0.11%	0.014%
76	11.418	3202	3212	3221	rBV	26403	42592	2.68%	0.336%
77	11.482	3221	3232	3258	rVB2	589224	1090119	68.58%	8.590%
78	11.858	3335	3349	3373	rBV2	594239	1106471	69.61%	8.719%
79	12.414	3514	3522	3524	rBV	1352	1806	0.11%	0.014%
80	12.450	3529	3533	3535	rBV	1033	882	0.06%	0.007%
81	12.694	3603	3609	3614	rBV	2682	3791	0.24%	0.030%
82	13.083	3725	3730	3732	rBV2	1074	1121	0.07%	0.009%
83	13.189	3760	3763	3766	rBV	1201	856	0.05%	0.007%
84	13.665	3908	3911	3917	rBV2	1902	1733	0.11%	0.014%


Sum of corrected areas: 12690969

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032419\
Data File : VU030370.D
Acq On : 24 Mar 2019 15:02
Operator : JC/SP
Sample : K2016-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0981

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

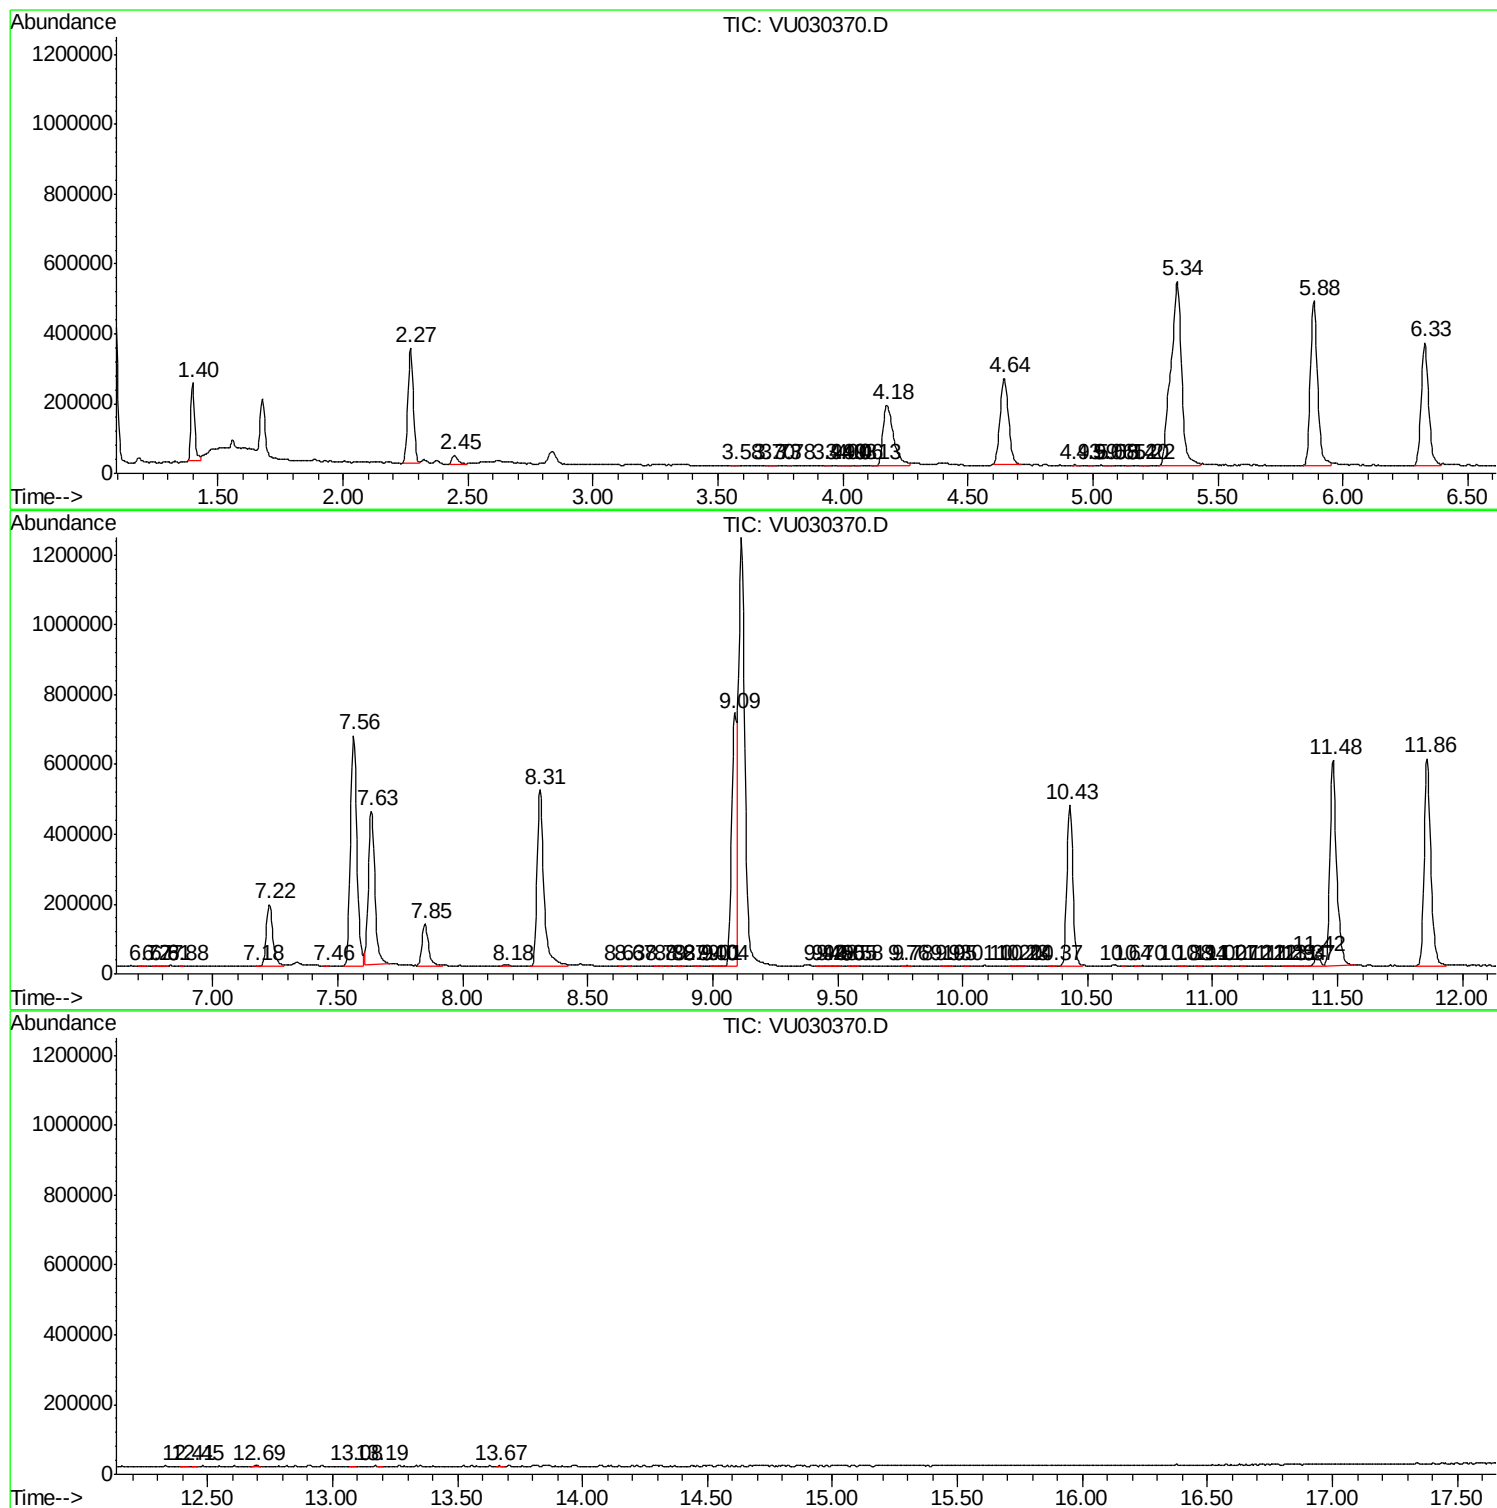

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032419\
Data File : VU030370.D
Acq On : 24 Mar 2019 15:02
Operator : JC/SP
Sample : K2016-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0981

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032419\
Data File : VU030370.D
Acq On : 24 Mar 2019 15:02
Operator : JC/SP
Sample : K2016-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0981

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc