

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030381.D
 Acq On : 24 Mar 2019 19:23
 Operator : JC/SP
 Sample : K2062-07 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rVB	17063	16017	0.96%	0.109%
2	1.399	88	96	108	rBV	220034	225390	13.58%	1.529%
3	1.672	174	181	199	rVB	166687	221496	13.34%	1.503%
4	2.270	356	367	379	rBV	339089	510013	30.73%	3.460%
5	2.450	409	423	430	rBV2	4751	11177	0.67%	0.076%
6	2.698	495	500	502	rBV2	2150	1956	0.12%	0.013%
7	2.768	515	522	525	rBV	1082	1725	0.10%	0.012%
8	2.955	576	580	586	rBV	2553	2923	0.18%	0.020%
9	3.106	623	627	631	rBV	1938	1665	0.10%	0.011%
10	3.170	642	647	650	rBV	2309	2043	0.12%	0.014%
11	3.238	665	668	677	rVB	1636	2246	0.14%	0.015%
12	3.434	726	729	734	rVB2	1669	1500	0.09%	0.010%
13	3.553	760	766	771	rVB	1437	1595	0.10%	0.011%
14	3.694	804	810	816	rBV	2698	3716	0.22%	0.025%
15	3.730	817	821	829	rVB	2343	2939	0.18%	0.020%
16	3.926	878	882	886	rVB	1748	1285	0.08%	0.009%
17	4.032	912	915	920	rBV2	1265	1130	0.07%	0.008%
18	4.174	942	959	991	rBV	167602	464852	28.01%	3.154%
19	4.643	1089	1105	1130	rBV	256985	613672	36.97%	4.164%
20	4.887	1172	1181	1187	rBV3	2518	4589	0.28%	0.031%
21	5.241	1285	1291	1293	rBV	1705	1968	0.12%	0.013%
22	5.337	1298	1321	1354	rVV2	544469	1659839	100.00%	11.262%
23	5.582	1393	1397	1400	rBV2	1414	1399	0.08%	0.009%
24	5.659	1418	1421	1424	rVV2	1247	1088	0.07%	0.007%
25	5.688	1427	1430	1434	rVB	1781	1198	0.07%	0.008%
26	5.884	1476	1491	1516	rBV	487781	986501	59.43%	6.693%
27	6.183	1571	1584	1606	rBV	400771	787971	47.47%	5.346%
28	6.328	1615	1629	1648	rBV	367659	738127	44.47%	5.008%
29	6.501	1681	1683	1687	rVB	1833	1130	0.07%	0.008%
30	6.768	1762	1766	1770	rBV2	1289	1037	0.06%	0.007%
31	6.874	1794	1799	1803	rBV	1592	1792	0.11%	0.012%
32	7.080	1861	1863	1873	rVB	2010	2482	0.15%	0.017%
33	7.125	1873	1877	1882	rBV2	939	1039	0.06%	0.007%
34	7.225	1896	1908	1931	rBV	187742	345952	20.84%	2.347%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030381.D
 Acq On : 24 Mar 2019 19:23
 Operator : JC/SP
 Sample : K2062-07 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	7.450	1975	1978	1985	rVB2	1807	1702	0.10%	0.012%
36	7.562	1999	2013	2033	rBV	657982	1192936	71.87%	8.094%
37	7.730	2062	2065	2070	rBV3	1341	1247	0.08%	0.008%
38	7.775	2075	2079	2083	rVB	2327	2142	0.13%	0.015%
39	7.849	2092	2102	2128	rBV	126795	226541	13.65%	1.537%
40	7.945	2128	2132	2135	rVV2	1760	1693	0.10%	0.011%
41	7.964	2135	2138	2143	rVB	2637	1857	0.11%	0.013%
42	8.029	2154	2158	2162	rBV	1074	1079	0.07%	0.007%
43	8.308	2232	2245	2285	rBV	550335	1011827	60.96%	6.865%
44	8.665	2350	2356	2359	rBV	2044	1872	0.11%	0.013%
45	8.717	2370	2372	2377	rVB	1844	1329	0.08%	0.009%
46	8.755	2379	2384	2387	rBV2	1360	1604	0.10%	0.011%
47	8.816	2401	2403	2408	rVV2	1284	1211	0.07%	0.008%
48	8.839	2408	2410	2417	rVB2	1504	1404	0.08%	0.010%
49	8.884	2421	2424	2428	rVB	1530	1363	0.08%	0.009%
50	8.929	2434	2438	2444	rBV	1682	1809	0.11%	0.012%
51	8.958	2444	2447	2451	rVB	2091	1530	0.09%	0.010%
52	8.987	2451	2456	2461	rBV	2165	2327	0.14%	0.016%
53	9.087	2475	2487	2521	rBV2	698559	1589014	95.73%	10.782%
54	9.296	2549	2552	2556	rVB	1529	1112	0.07%	0.008%
55	9.373	2569	2576	2579	rBV2	2108	2532	0.15%	0.017%
56	9.472	2602	2607	2613	rVB	1628	2240	0.13%	0.015%
57	9.505	2613	2617	2620	rBV2	1422	1344	0.08%	0.009%
58	9.575	2633	2639	2644	rVB	1839	2279	0.14%	0.015%
59	9.604	2644	2648	2654	rBV	1426	1618	0.10%	0.011%
60	9.633	2654	2657	2660	rBV	1554	1057	0.06%	0.007%
61	9.903	2737	2741	2744	rBV	1504	1605	0.10%	0.011%
62	10.032	2777	2781	2787	rVV2	1313	1519	0.09%	0.010%
63	10.164	2818	2822	2824	rBV	1736	1307	0.08%	0.009%
64	10.270	2841	2855	2858	rBV	2109	4222	0.25%	0.029%
65	10.427	2890	2904	2927	rBV	480738	781578	47.09%	5.303%
66	10.530	2934	2936	2942	rVB	1657	1263	0.08%	0.009%
67	10.607	2955	2960	2971	rVB2	2129	3197	0.19%	0.022%
68	10.668	2975	2979	2982	rVB2	1403	1047	0.06%	0.007%
69	10.746	2999	3003	3006	rBV	1641	1260	0.08%	0.009%
70	10.987	3075	3078	3083	rVB	1695	1366	0.08%	0.009%
71	11.045	3091	3096	3099	rBV	1951	1736	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032419\
 Data File : VU030381.D
 Acq On : 24 Mar 2019 19:23
 Operator : JC/SP
 Sample : K2062-07 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.154	3123	3130	3133	rVB2	1132	1278	0.08%	0.009%
73	11.276	3165	3168	3173	rVB	1605	1309	0.08%	0.009%
74	11.418	3203	3212	3221	rBV3	27955	44850	2.70%	0.304%
75	11.482	3221	3232	3256	rVV2	619184	1461074	88.03%	9.914%
76	11.675	3289	3292	3296	rVB	1873	1608	0.10%	0.011%
77	11.858	3337	3349	3376	rVV2	643564	1397061	84.17%	9.479%
78	12.218	3457	3461	3463	rBV	1843	1310	0.08%	0.009%
79	12.276	3476	3479	3483	rVB	1781	1110	0.07%	0.008%
80	12.305	3483	3488	3492	rBV2	1274	1230	0.07%	0.008%
81	12.527	3554	3557	3560	rBV	1727	1276	0.08%	0.009%
82	12.636	3588	3591	3596	rBV	1376	1363	0.08%	0.009%
83	13.019	3705	3710	3714	rBV2	1643	1385	0.08%	0.009%
84	13.051	3714	3720	3723	rVV	2091	2194	0.13%	0.015%
85	13.186	3757	3762	3765	rBV2	1033	1281	0.08%	0.009%
86	13.430	3835	3838	3841	rVB	1827	1204	0.07%	0.008%
87	13.450	3841	3844	3850	rVB	1575	1302	0.08%	0.009%
88	13.504	3850	3861	3889	rBV2	98870	209487	12.62%	1.421%
89	13.742	3931	3935	3939	rBV4	1450	1732	0.10%	0.012%
90	13.819	3955	3959	3962	rBV	2218	1602	0.10%	0.011%
91	13.990	4002	4012	4027	rBV4	27068	53910	3.25%	0.366%
92	14.247	4089	4092	4096	rBV	1362	1154	0.07%	0.008%
93	14.324	4113	4116	4118	rBV	2234	1593	0.10%	0.011%
94	14.893	4290	4293	4299	rBV	1300	1449	0.09%	0.010%
95	15.083	4345	4352	4361	rBV6	5915	9726	0.59%	0.066%
96	15.199	4382	4388	4391	rBV	2600	2858	0.17%	0.019%
97	15.488	4475	4478	4482	rVB	1761	1332	0.08%	0.009%
98	15.517	4482	4487	4491	rBV	2119	2680	0.16%	0.018%
99	15.655	4521	4530	4547	rBV4	21225	46742	2.82%	0.317%
100	15.749	4556	4559	4566	rVB	2483	2891	0.17%	0.020%


Sum of corrected areas: 14738212

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032419\
Data File : VU030381.D
Acq On : 24 Mar 2019 19:23
Operator : JC/SP
Sample : K2062-07 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BF1A2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

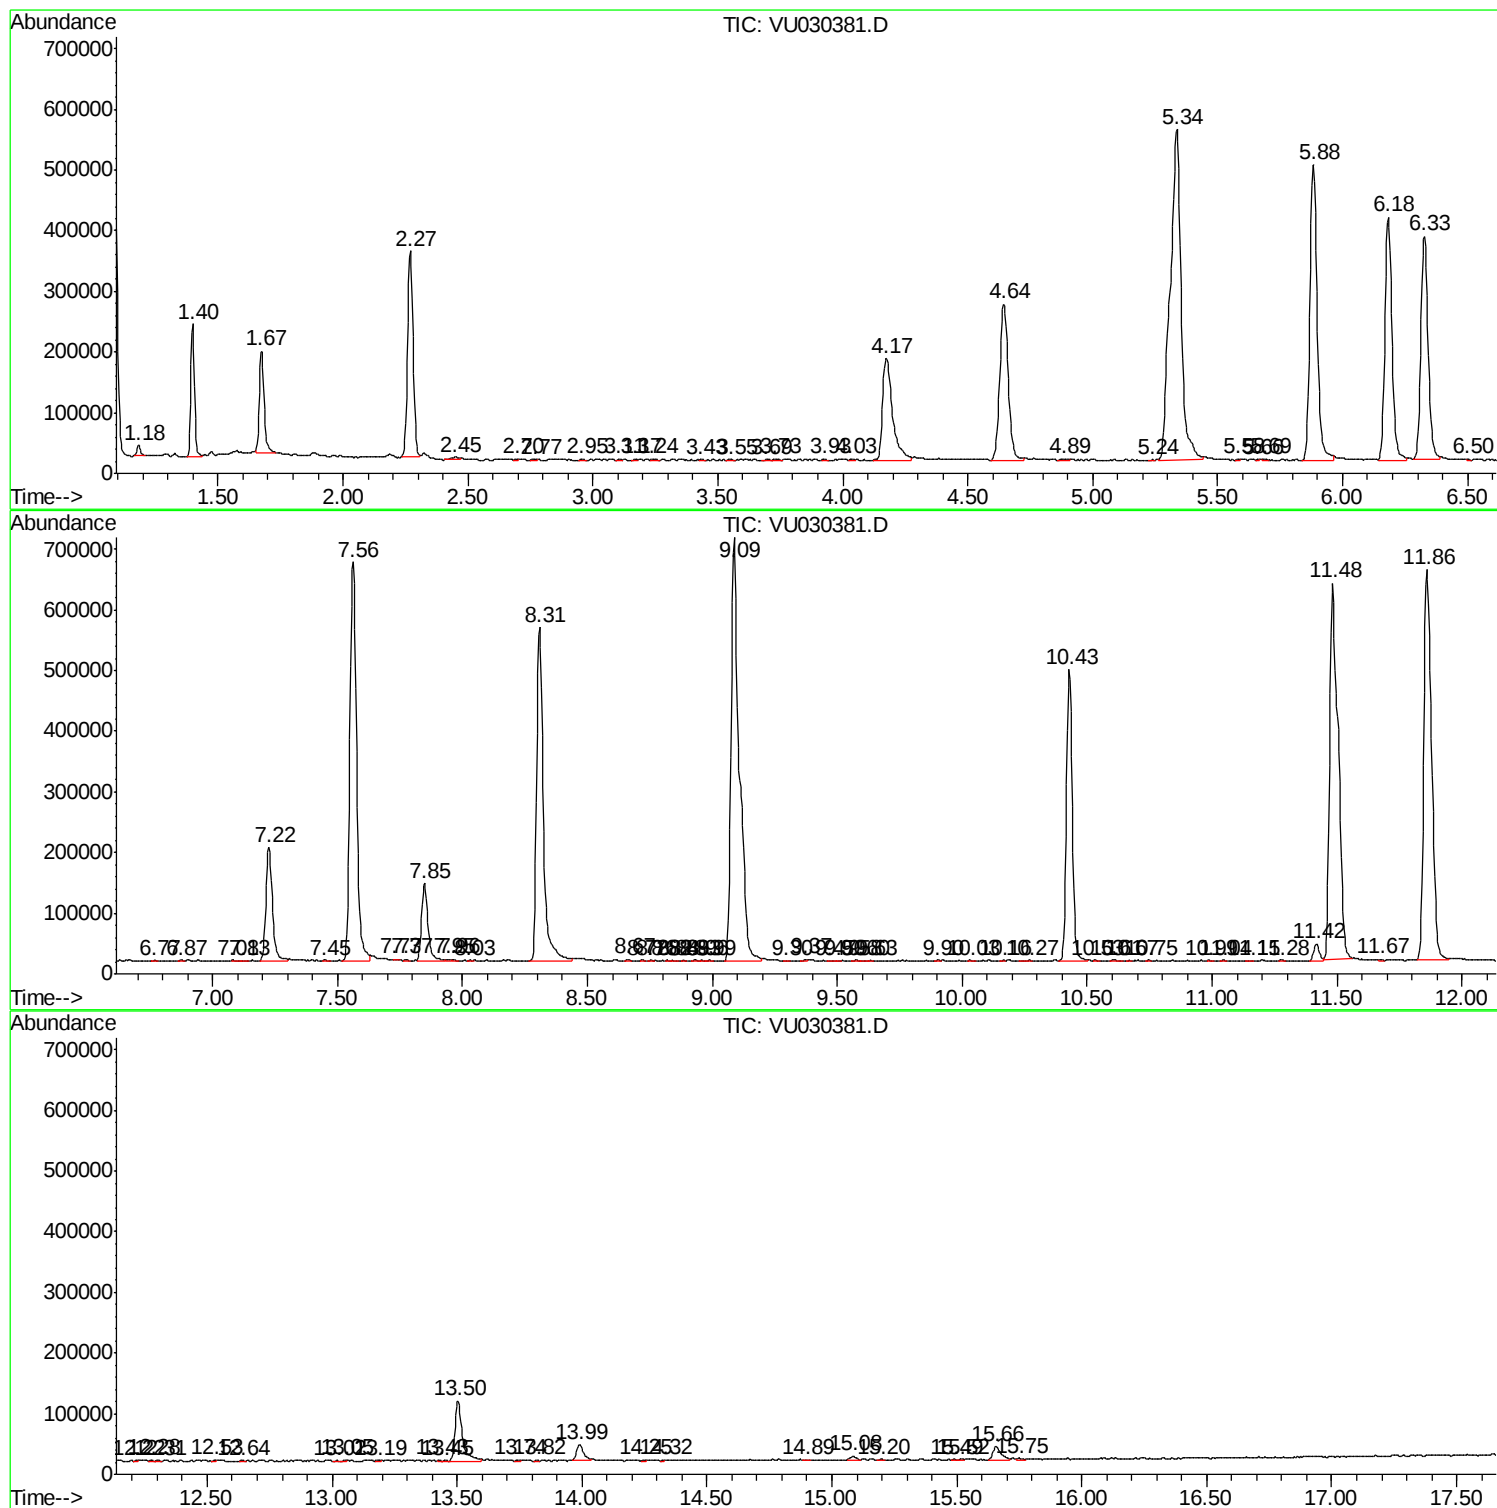

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032419\
Data File : VU030381.D
Acq On : 24 Mar 2019 19:23
Operator : JC/SP
Sample : K2062-07 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032419\
Data File : VU030381.D
Acq On : 24 Mar 2019 19:23
Operator : JC/SP
Sample : K2062-07 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc