
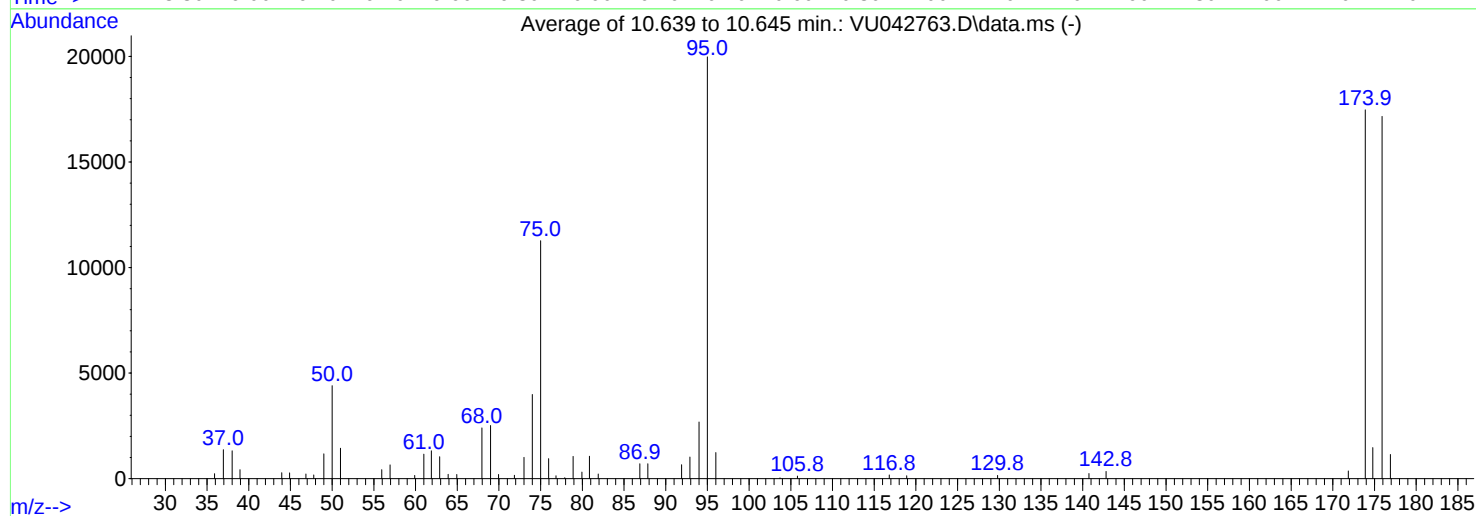


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032421\
Data File : VU042763.D
Acq On : 24 Mar 2021 13:35
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
Title : SW846 8260
Last Update : Thu Mar 25 05:42:00 2021

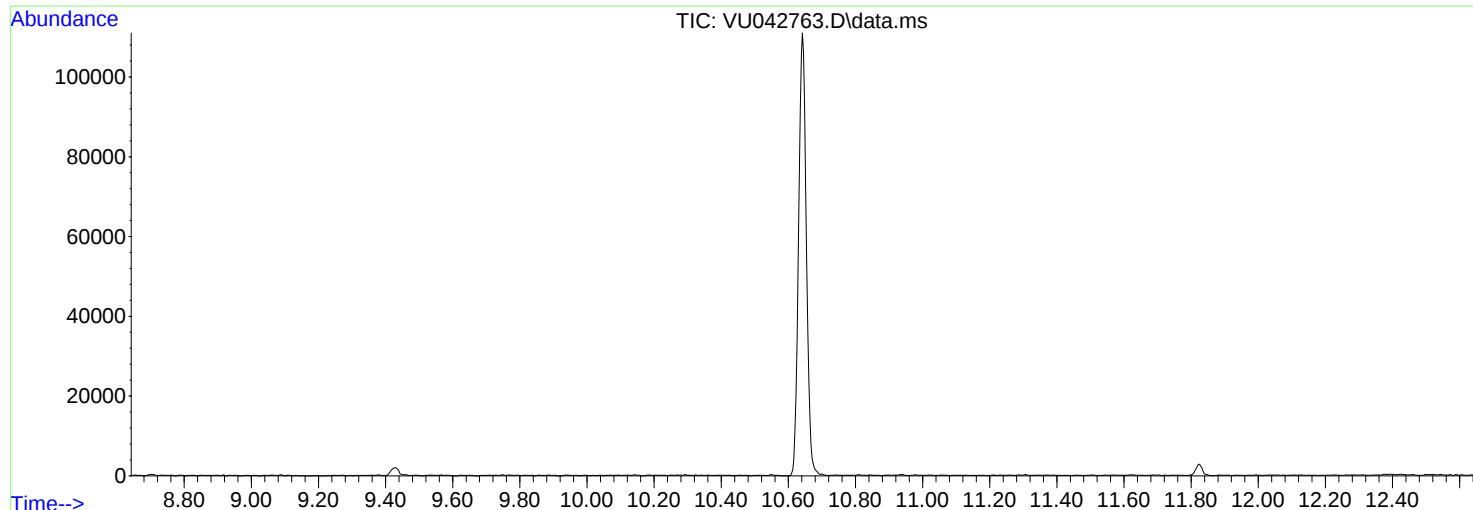

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.0	4405	PASS
75	95	30	60	56.4	11268	PASS
95	95	100	100	100.0	19979	PASS
96	95	5	9	6.2	1235	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.4	17467	PASS
175	174	5	9	8.4	1468	PASS
176	174	95	101	98.2	17157	PASS
177	176	5	9	6.7	1141	PASS