




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047661.D
Acq On : 25 Mar 2022 02:25
Operator : SY/MD
Sample : N2081-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/25/2022
Supervised By :Mahesh Dadoda 03/29/2022

Quant Time: Mar 25 05:31:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 24 23:34:42 2022
Response via : Initial Calibration

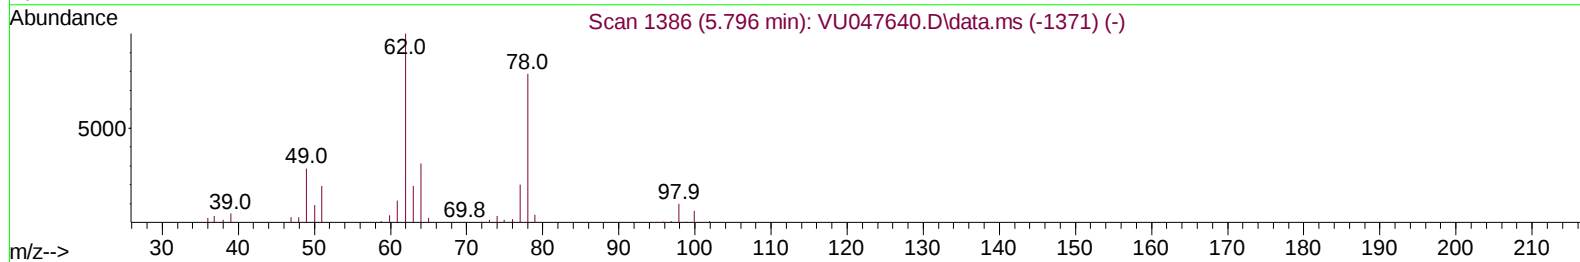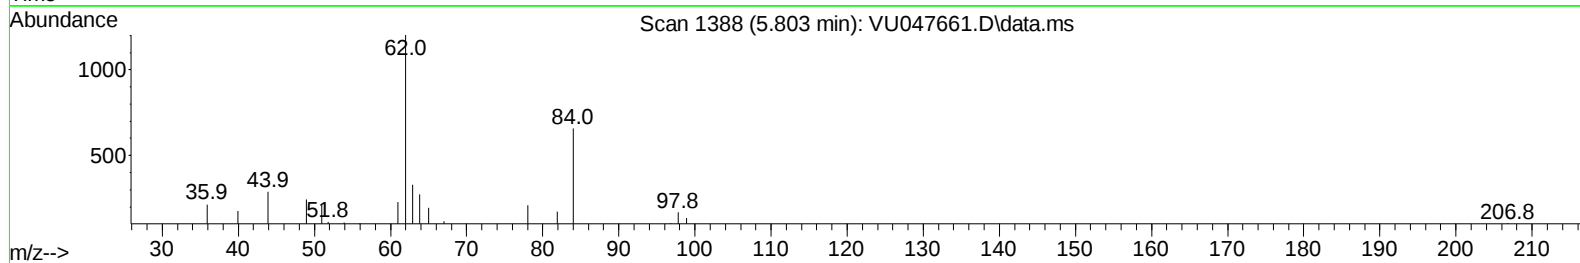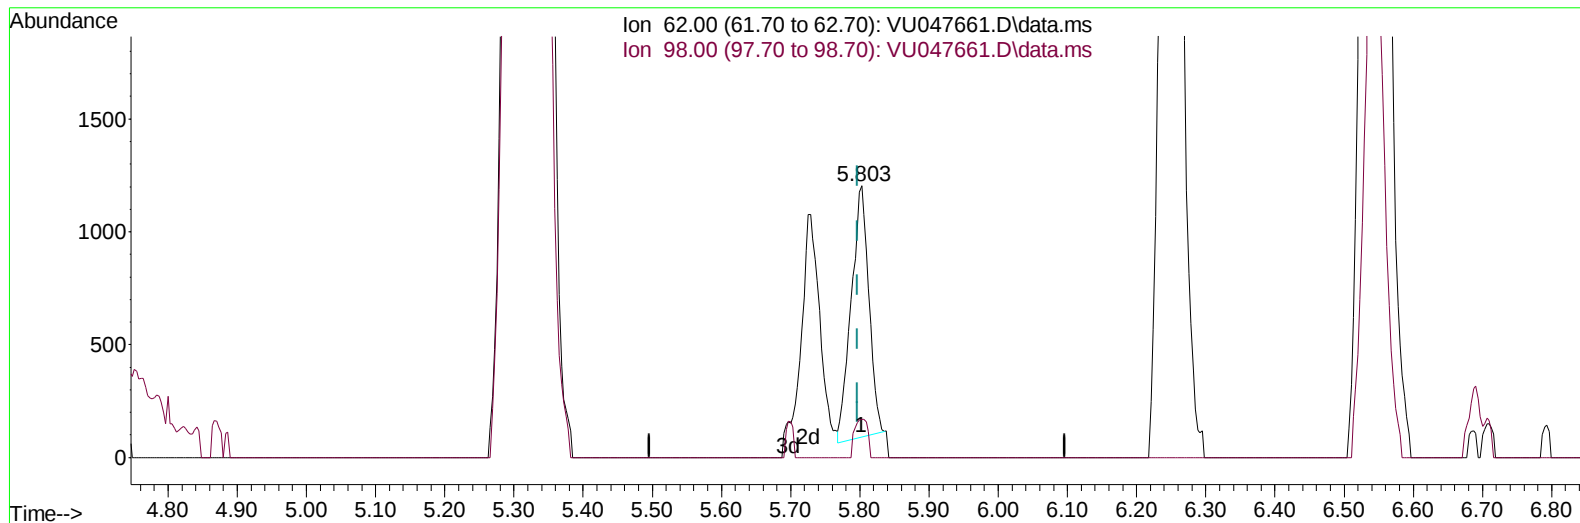

TIC: VU047661.D\data.ms

(27) 1,2-Dichloroethane (T)

5.803min (+ 0.006) 0.53 ug/L

response 1988

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	9.20	13.97#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047661.D
 Acq On : 25 Mar 2022 02:25
 Operator : SY/MD
 Sample : N2081-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7

Manual IntegrationsAPPROVED

Quant Time: Mar 25 05:31:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 24 23:34:42 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/25/2022
 Supervised By :Mahesh Dadoda 03/29/2022

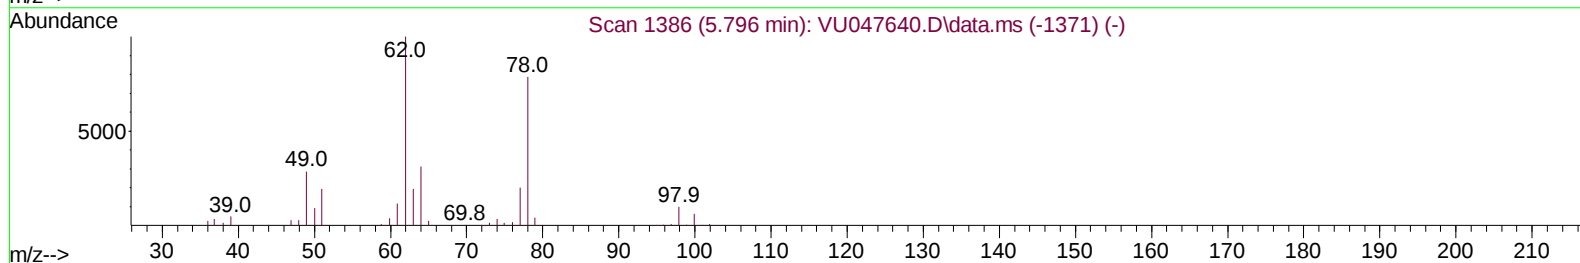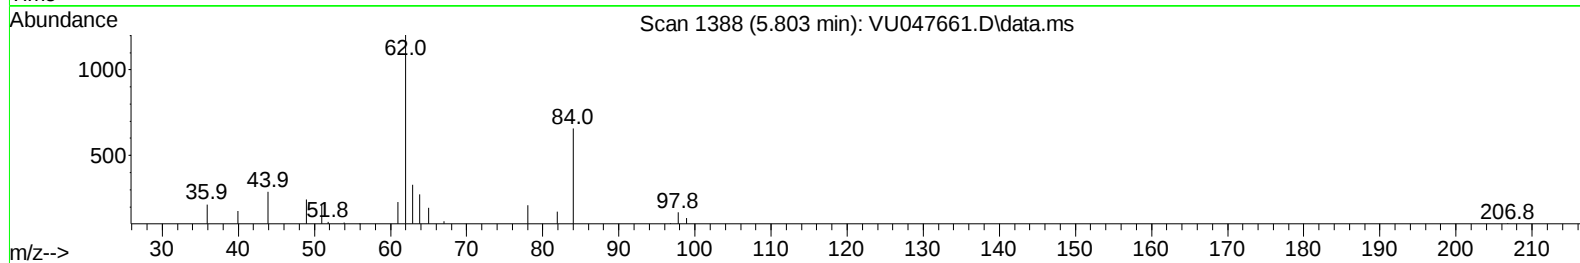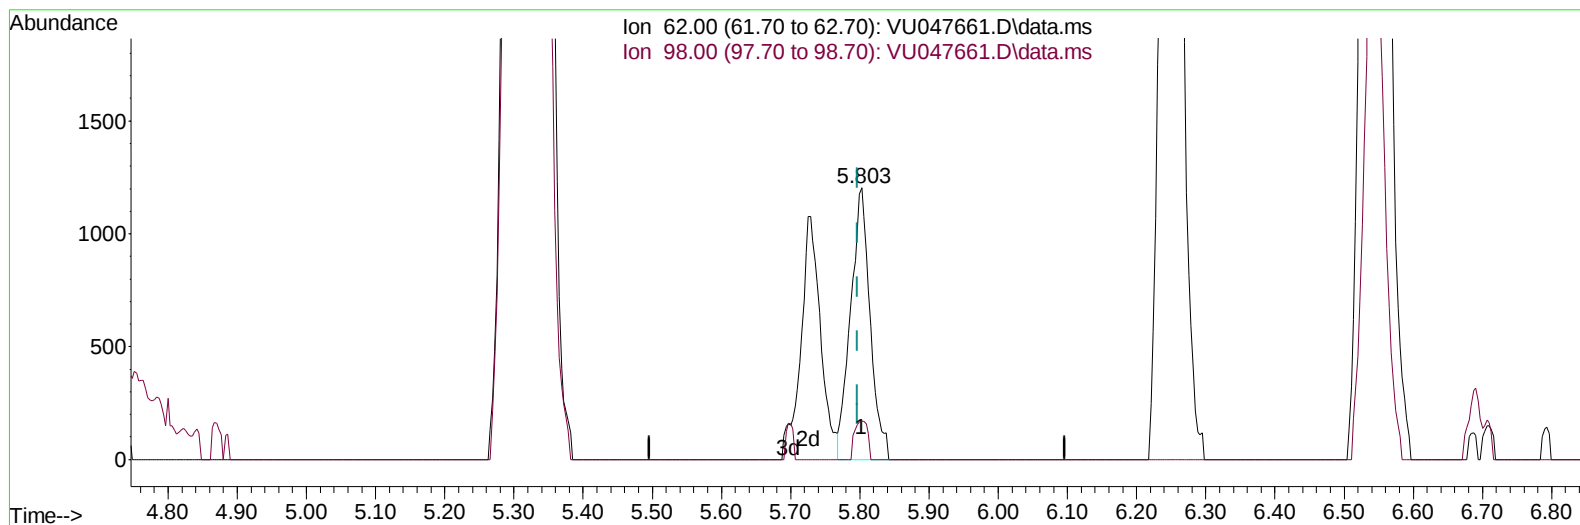

TIC: VU047661.D\data.ms

(27) 1,2-Dichloroethane (T)

5.803min (+ 0.006) 0.63 ug/L m

response 2373

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	9.20	13.97#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047661.D
 Acq On : 25 Mar 2022 02:25
 Operator : SY/MD
 Sample : N2081-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7

Manual IntegrationsAPPROVED

Quant Time: Mar 25 05:31:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 24 23:34:42 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/25/2022
 Supervised By : Mahesh Dadoda 03/29/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	352810	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	364992	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	194176	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	93462	36.531	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	73.060%	
7) Chloroethane-d5	1.919	69	76260	37.802	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	75.600%	
11) 1,1-Dichloroethene-d2	2.578	63	293273	62.653	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	125.300%#	
21) 2-Butanone-d5	4.642	46	200254	91.191	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.190%	
24) Chloroform-d	5.066	84	185916	39.715	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.420%	
26) 1,2-Dichloroethane-d4	5.706	65	120719	42.046	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.100%	
32) Benzene-d6	5.729	84	383026	41.705	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	6.693	67	121172	42.960	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	85.920%	
41) Toluene-d8	7.899	98	357584	39.962	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.920%#	
43) trans-1,3-Dichloroprop...	8.182	79	55657	38.950	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	77.900%	
47) 2-Hexanone-d5	8.635	63	144223	87.347	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	87.350%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	192413	39.750	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	79.500%	
66) 1,2-Dichlorobenzene-d4	12.195	152	151569	43.875	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.740%	
Target Compounds						
					Qvalue	
9) Trichlorofluoromethane	2.144	101	10193	2.266	ug/L	94
12) 1,1-Dichloroethene	2.584	96	309780	128.002	ug/L #	74
17) trans-1,2-Dichloroethene	3.359	96	13585	5.204	ug/L	93
19) 1,1-Dichloroethane	3.874	63	809678	179.851	ug/L	99
20) cis-1,2-Dichloroethene	4.671	96	255387	89.242	ug/L	95
27) 1,2-Dichloroethane	5.803	62	2373m	0.634	ug/L	
30) 1,1,1-Trichloroethane	5.321	97	1943655	469.637	ug/L	99
34) Trichloroethene	6.546	95	186471	67.324	ug/L	99
45) 1,1,2-Trichloroethane	8.401	97	7059	2.478	ug/L	96
46) Tetrachloroethene	8.555	164	227575	91.431	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047661.D
Acq On : 25 Mar 2022 02:25
Operator : SY/MD
Sample : N2081-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y7

Manual IntegrationsAPPROVED

Quant Time: Mar 25 05:31:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 24 23:34:42 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/25/2022
Supervised By :Mahesh Dadoda 03/29/2022

